

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045087.D
 Acq On : 28 Feb 2025 14:33
 Operator : JC/MD
 Sample : Q1403-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Storage-Blank-WATER-REF-5

Quant Time: Feb 28 23:08:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	70861	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	140925	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	129094	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	54421	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	58538	51.935	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	103.860%
35) Dibromofluoromethane	5.379	113	48403	51.365	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.740%
50) Toluene-d8	8.647	98	174605	51.110	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.220%
62) 4-Bromofluorobenzene	11.079	95	59324	52.404	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	104.800%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045087.D
Acq On : 28 Feb 2025 14:33
Operator : JC/MD
Sample : Q1403-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5

Quant Time: Feb 28 23:08:24 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration




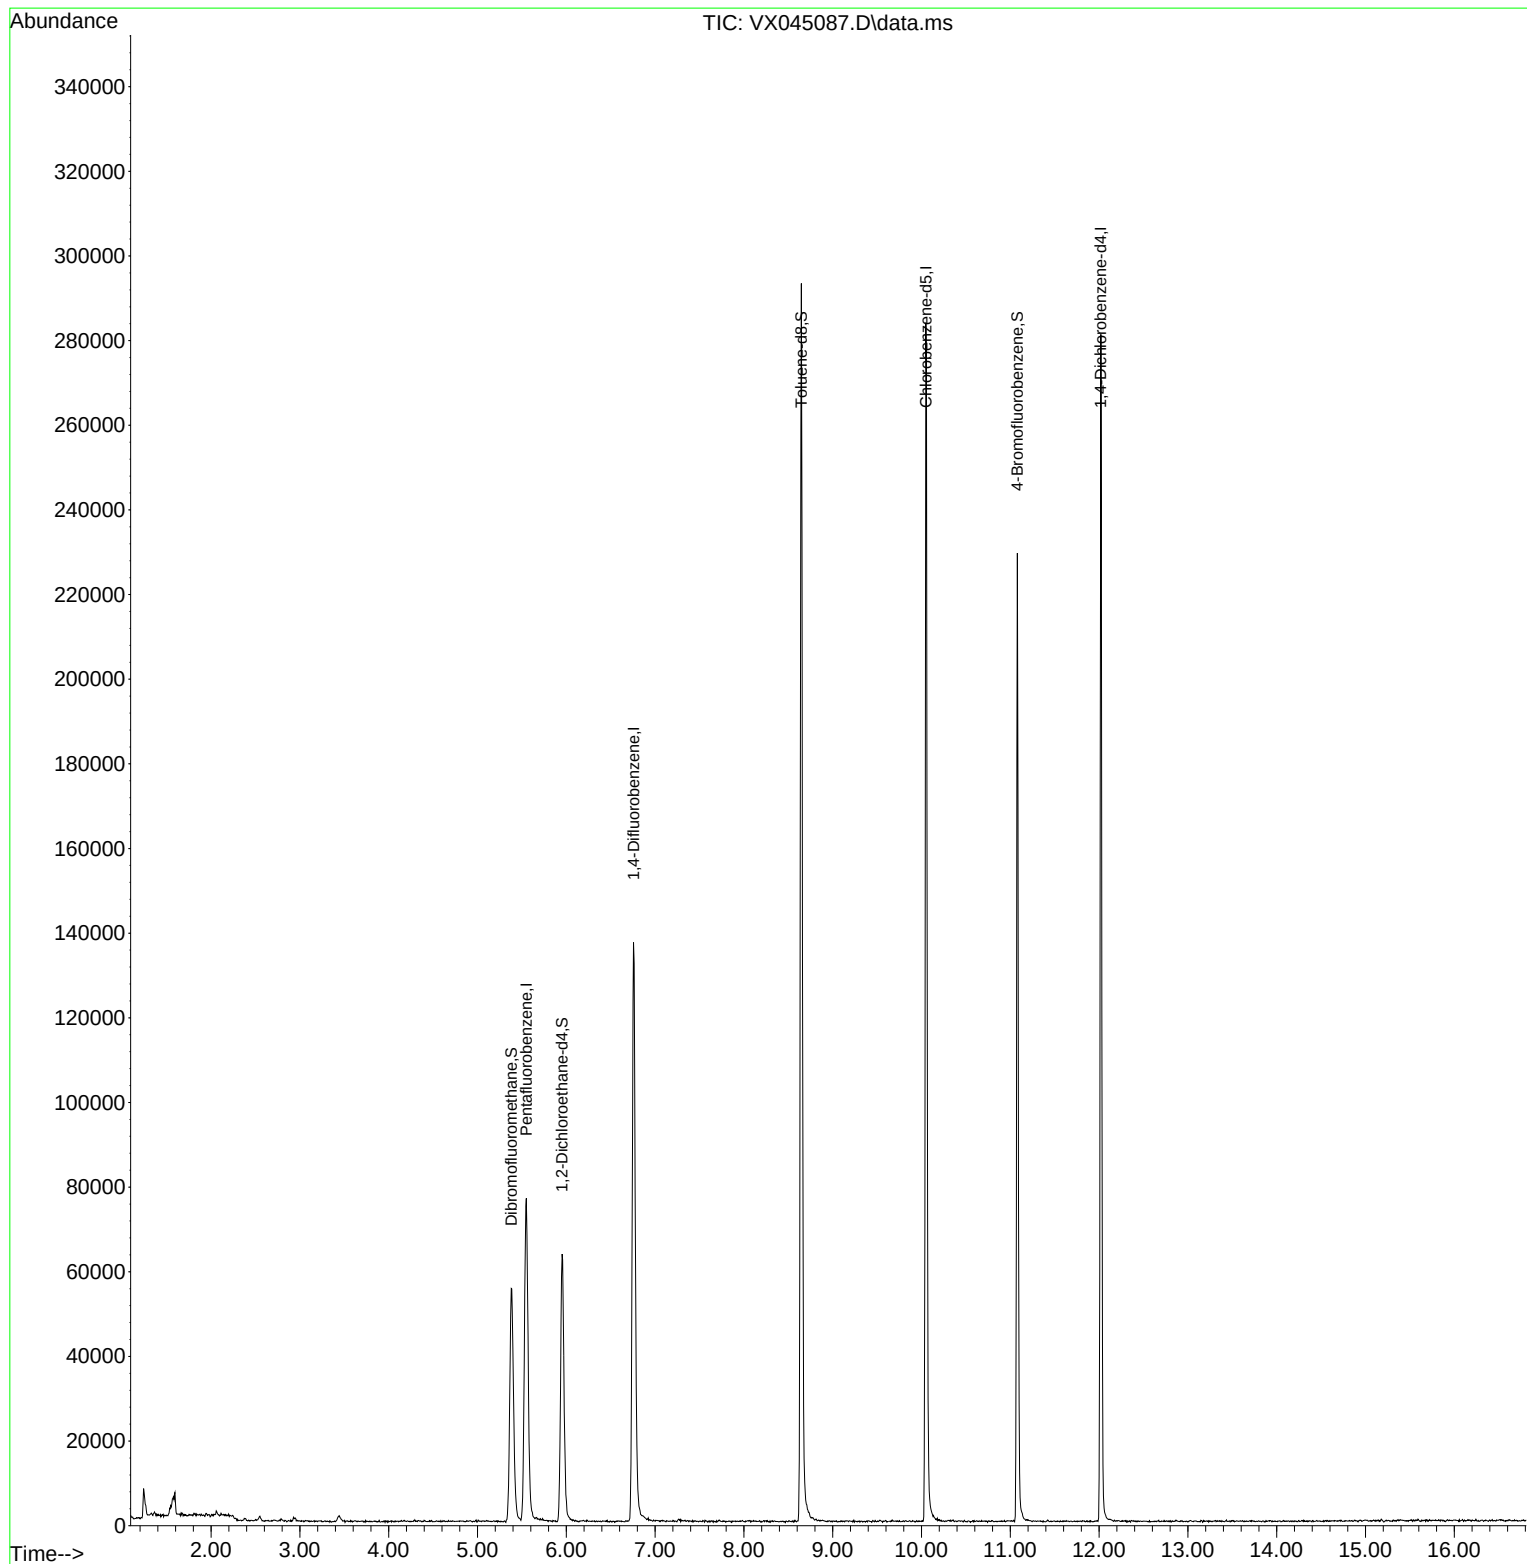


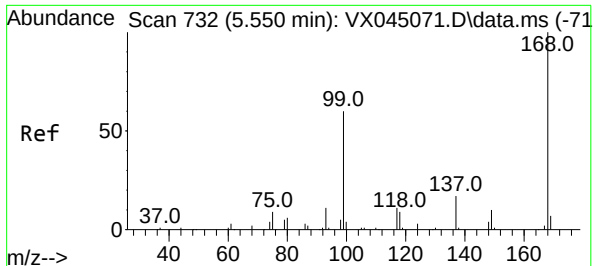

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.000 min
Lab File: VX045087.D
Acq: 28 Feb 2025 14:33




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5


Tgt Ion:168 Resp: 70861
Ion Ratio Lower Upper
168 100
99 61.8 48.2 72.4

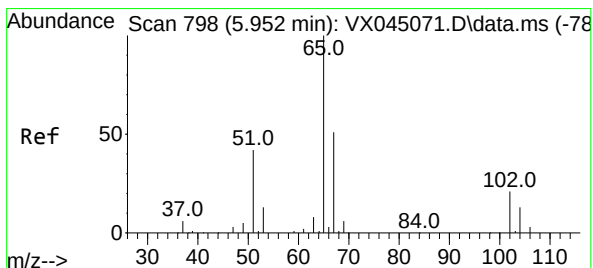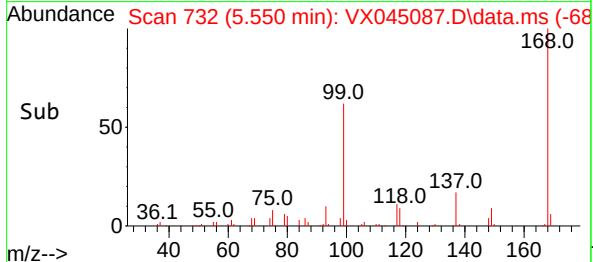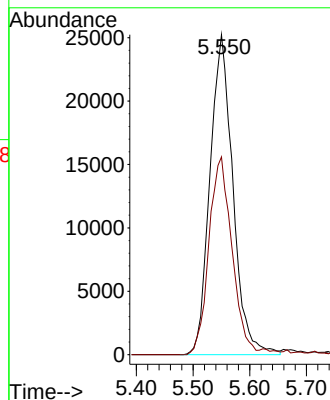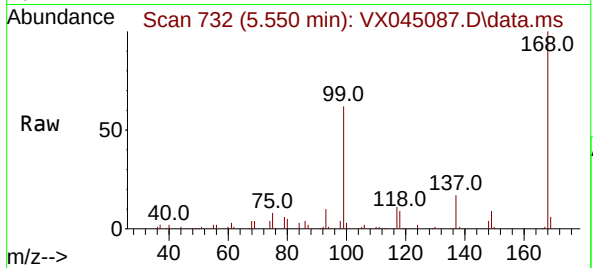

#33
1,2-Dichloroethane-d4
Concen: 51.935 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX045087.D
Acq: 28 Feb 2025 14:33

Tgt Ion: 65 Resp: 58538
Ion Ratio Lower Upper
65 100
67 51.8 0.0 106.2


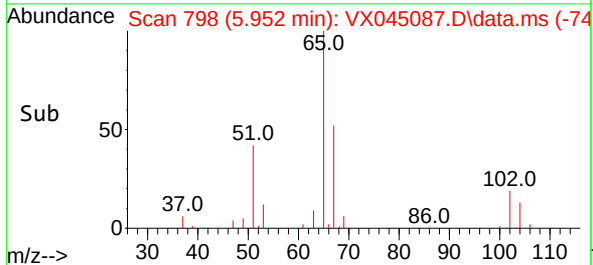
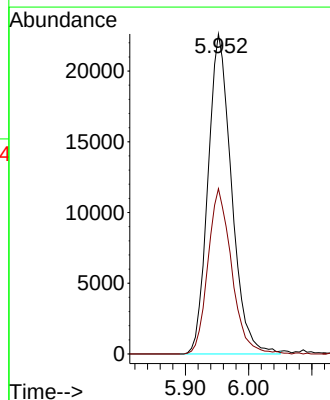
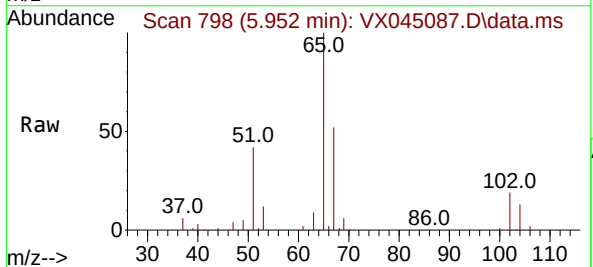


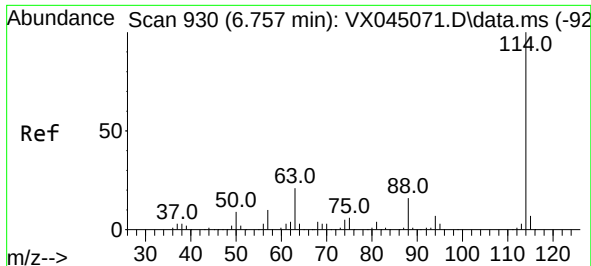

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX045087.D
Acq: 28 Feb 2025 14:33




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5


Tgt Ion:114 Resp: 140925
Ion Ratio Lower Upper
114 100
63 22.4 0.0 41.8
88 15.2 0.0 32.8

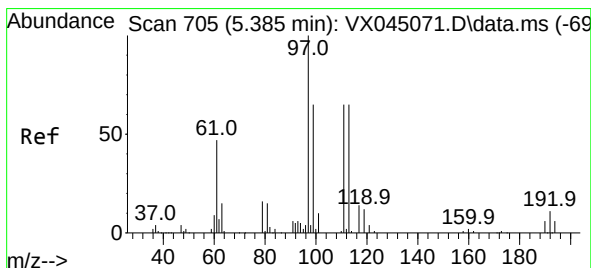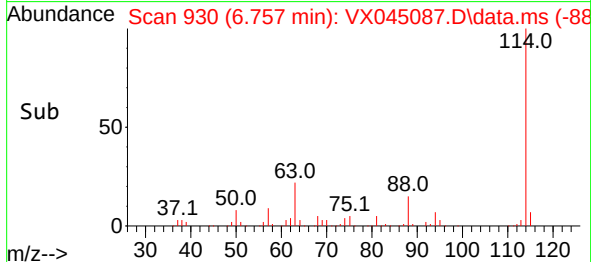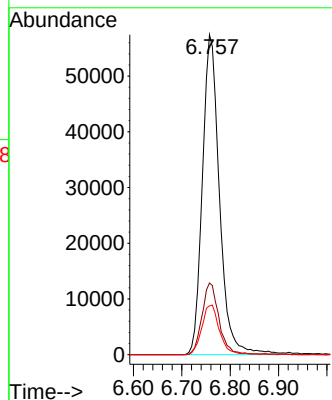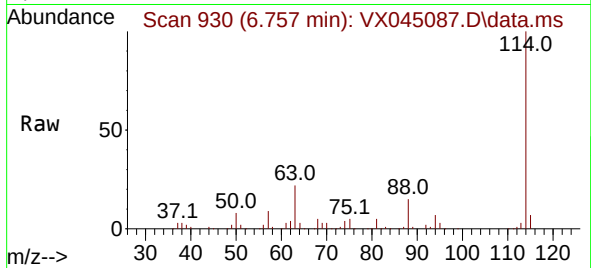

#35
Dibromofluoromethane
Concen: 51.365 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX045087.D
Acq: 28 Feb 2025 14:33

Tgt Ion:113 Resp: 48403
Ion Ratio Lower Upper
113 100
111 103.0 81.8 122.6
192 17.9 14.3 21.5


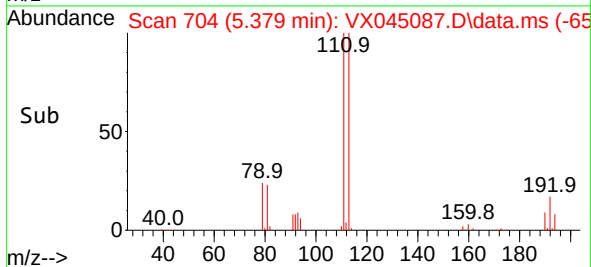
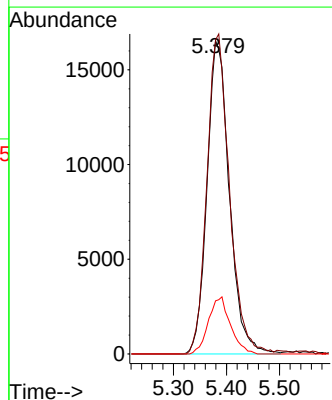
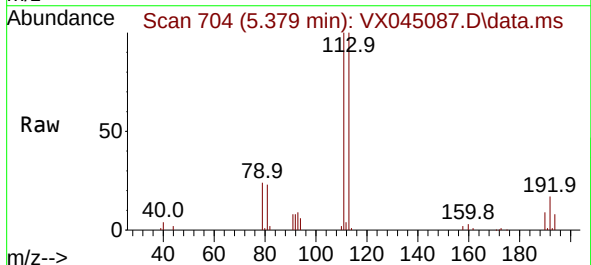


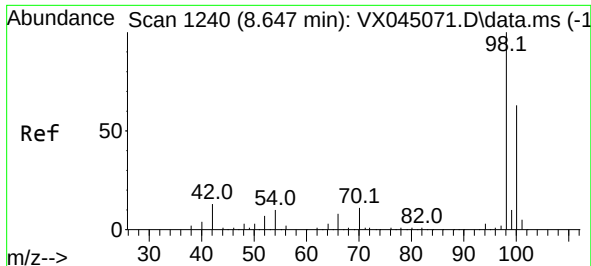

#50
Toluene-d8
Concen: 51.110 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045087.D
Acq: 28 Feb 2025 14:33




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5


Tgt Ion: 98 Resp: 174605
Ion Ratio Lower Upper
98 100
100 65.9 52.0 78.0

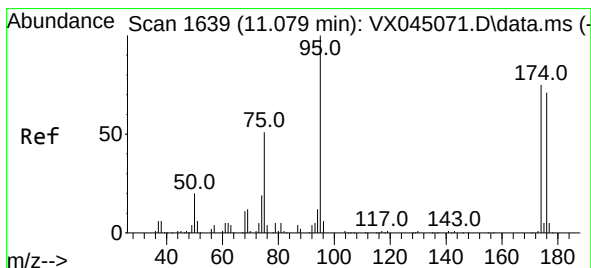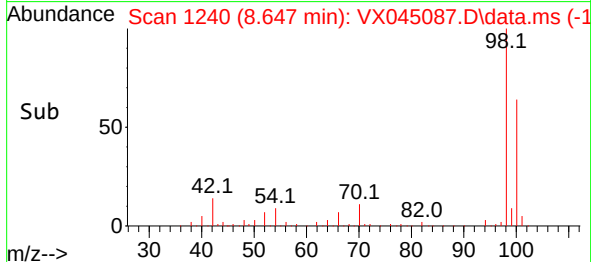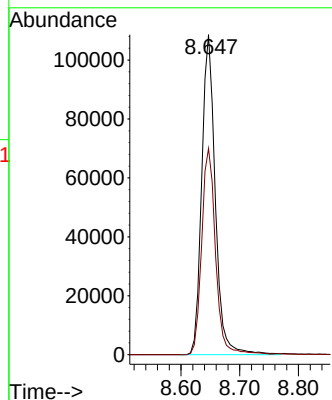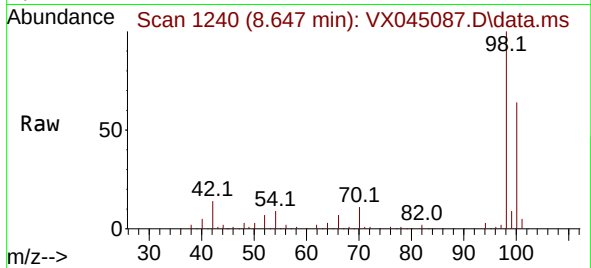

#62
4-Bromofluorobenzene
Concen: 52.404 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045087.D
Acq: 28 Feb 2025 14:33

Tgt Ion: 95 Resp: 59324
Ion Ratio Lower Upper
95 100
174 75.4 0.0 148.2
176 72.1 0.0 141.4


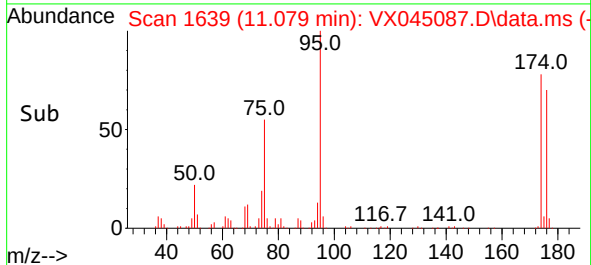
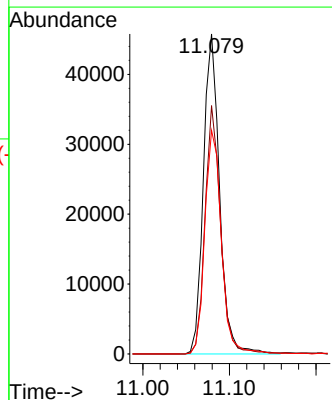
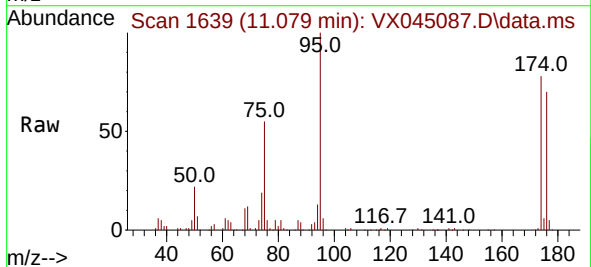


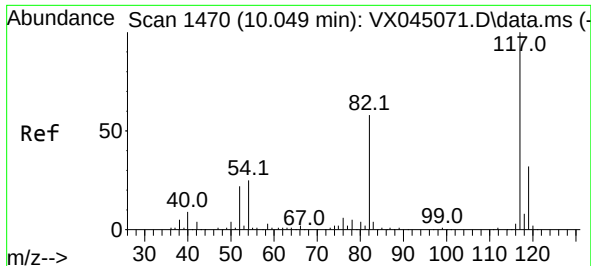

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045087.D
Acq: 28 Feb 2025 14:33

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-WATER-REF-5

Tgt Ion:117 Resp: 129094
Ion Ratio Lower Upper
117 100
82 59.5 46.3 69.5
119 31.4 25.7 38.5

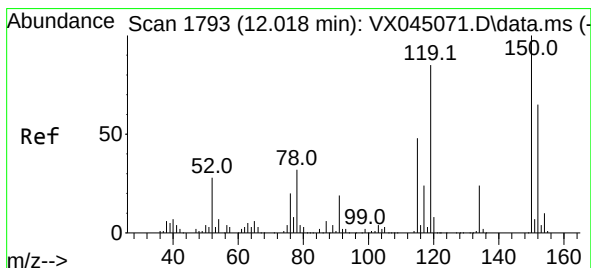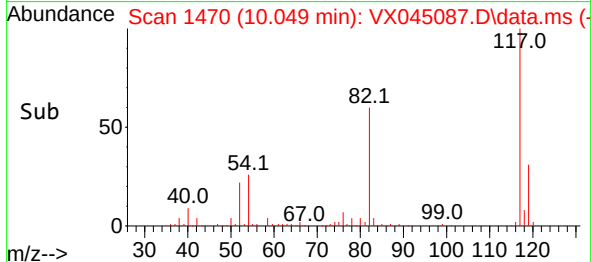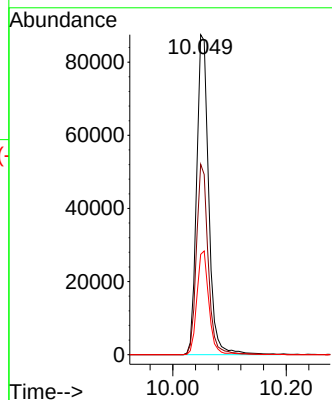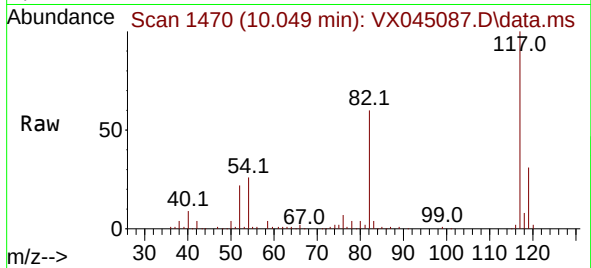

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045087.D
Acq: 28 Feb 2025 14:33

Tgt Ion:152 Resp: 54421
Ion Ratio Lower Upper
152 100
115 63.0 44.2 132.6
150 156.9 0.0 349.0

