
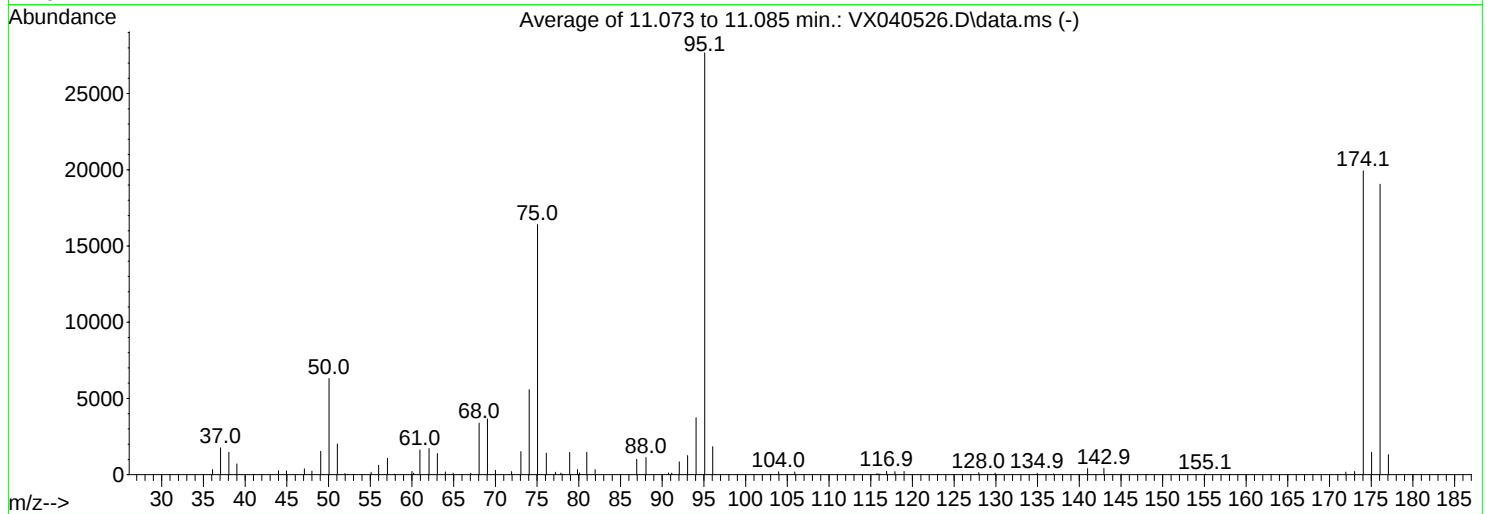


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022924\
Data File : VX040526.D
Acq On : 29 Feb 2024 09:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
Title : SW846 8260
Last Update : Tue Feb 27 05:01:33 2024

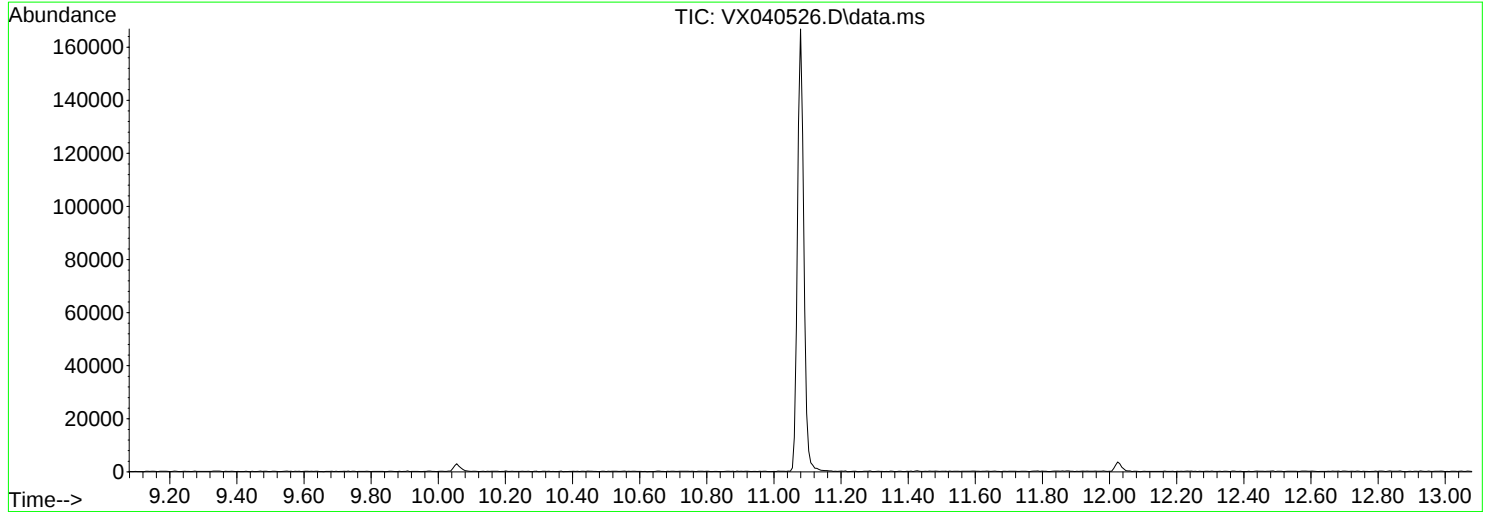

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.8	6306	PASS
75	95	30	60	59.3	16411	PASS
95	95	100	100	100.0	27672	PASS
96	95	5	9	6.6	1837	PASS
173	174	0.00	2	1.1	211	PASS
174	95	50	100	72.0	19931	PASS
175	174	5	9	7.4	1465	PASS
176	174	95	101	95.6	19050	PASS
177	176	5	9	6.9	1312	PASS