

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030121\
 Data File : VX020933.D
 Acq On : 01 Mar 2021 10:18
 Operator : JC/MD
 Sample : VX0301WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK406

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Title : VOC Analysis

Signal : TIC: VX020933.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	30	32	35	rBV	2976	2547	0.19%	0.026%
2	1.393	48	52	62	rVB	151415	170588	12.72%	1.756%
3	1.693	98	103	112	rVB	141000	171963	12.83%	1.770%
4	2.346	207	214	226	rBV	277008	462079	34.47%	4.756%
5	2.829	291	296	305	rBV8	1961	4346	0.32%	0.045%
6	2.982	320	322	324	rBV3	584	459	0.03%	0.005%
7	4.246	535	537	539	rVB	439	347	0.03%	0.004%
8	4.529	574	585	603	rBV	92033	268969	20.06%	2.769%
9	5.141	675	689	706	rBV	174086	533416	39.79%	5.491%
10	5.429	736	738	739	rBV2	395	271	0.02%	0.003%
11	5.458	739	743	753	rVB5	1274	3470	0.26%	0.036%
12	5.623	766	771	780	rVB4	2586	6594	0.49%	0.068%
13	6.041	829	842	860	rBV2	456876	1340674	100.00%	13.800%
14	6.341	890	893	897	rBV3	486	793	0.06%	0.008%
15	6.506	919	921	922	rBV	548	370	0.03%	0.004%
16	6.611	937	939	942	rBV2	388	275	0.02%	0.003%
17	6.829	966	976	993	rBV	326205	763049	56.92%	7.854%
18	7.059	1011	1015	1017	rBV2	403	468	0.03%	0.005%
19	7.170	1026	1034	1043	rBV	9492	20094	1.50%	0.207%
20	7.364	1058	1067	1081	rBV	277786	604846	45.12%	6.226%
21	7.523	1091	1094	1100	rVB4	835	1562	0.12%	0.016%
22	7.594	1104	1106	1108	rBV	322	324	0.02%	0.003%
23	7.729	1125	1129	1131	rBV2	512	638	0.05%	0.007%
24	7.965	1166	1169	1170	rBV2	999	908	0.07%	0.009%
25	8.229	1212	1214	1216	rBV2	353	287	0.02%	0.003%
26	8.282	1219	1223	1224	rBV3	1023	1202	0.09%	0.012%
27	8.370	1230	1238	1252	rBV	210990	339506	25.32%	3.495%
28	8.512	1259	1262	1268	rVB4	1068	1584	0.12%	0.016%
29	8.694	1286	1293	1318	rBV	695396	1098012	81.90%	11.302%
30	8.994	1338	1344	1355	rBV	152408	224728	16.76%	2.313%
31	9.153	1368	1371	1372	rBV2	458	457	0.03%	0.005%
32	9.318	1393	1399	1401	rVV3	828	1223	0.09%	0.013%
33	9.341	1401	1403	1410	rVB3	290	530	0.04%	0.005%
34	9.424	1410	1417	1439	rBV	416930	592458	44.19%	6.098%
35	9.565	1439	1441	1444	rVV3	536	547	0.04%	0.006%
36	9.594	1444	1446	1449	rVB3	311	300	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030121\
 Data File : VX020933.D
 Acq On : 01 Mar 2021 10:18
 Operator : JC/MD
 Sample : VX0301WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK406

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Title : VOC Analysis

37	9.665	1455	1458	1460	rVB2	368	383	0.03%	0.004%
38	9.812	1481	1483	1486	rVB2	280	303	0.02%	0.003%
39	9.882	1492	1495	1499	rVV4	481	514	0.04%	0.005%
40	9.953	1504	1507	1508	rVV2	346	291	0.02%	0.003%
41	10.000	1511	1515	1516	rVV2	367	402	0.03%	0.004%
42	10.018	1516	1518	1520	rVV	399	375	0.03%	0.004%
43	10.047	1521	1523	1525	rVV	336	289	0.02%	0.003%
44	10.094	1525	1531	1550	rVV	653021	882920	65.86%	9.088%
45	10.235	1551	1555	1560	rVV3	835	1339	0.10%	0.014%
46	10.277	1560	1562	1566	rVV4	429	610	0.05%	0.006%
47	10.312	1566	1568	1570	rVV3	451	481	0.04%	0.005%
48	10.341	1570	1573	1579	rVV3	1279	1683	0.13%	0.017%
49	10.388	1579	1581	1585	rVV3	310	311	0.02%	0.003%
50	10.447	1590	1591	1594	rVV2	314	301	0.02%	0.003%
51	10.577	1611	1613	1617	rVB2	286	389	0.03%	0.004%
52	10.688	1628	1632	1635	rVV4	986	1543	0.12%	0.016%
53	10.759	1642	1644	1649	rVB2	239	345	0.03%	0.004%
54	10.888	1663	1666	1667	rVV3	242	267	0.02%	0.003%
55	10.918	1670	1671	1674	rVV2	250	306	0.02%	0.003%
56	10.994	1683	1684	1688	rVB2	432	466	0.03%	0.005%
57	11.118	1699	1705	1711	rBV4	627	1079	0.08%	0.011%
58	11.230	1718	1724	1731	rBV	459299	577867	43.10%	5.948%
59	11.412	1751	1755	1758	rVB3	376	375	0.03%	0.004%
60	11.489	1764	1768	1771	rBV4	748	1120	0.08%	0.012%
61	11.565	1779	1781	1783	rVB2	351	314	0.02%	0.003%
62	11.747	1809	1812	1815	rBV2	524	663	0.05%	0.007%
63	11.783	1815	1818	1823	rBV2	441	711	0.05%	0.007%
64	12.006	1854	1856	1859	rVB2	726	781	0.06%	0.008%
65	12.059	1860	1865	1874	rBV	605025	756115	56.40%	7.783%
66	12.259	1896	1899	1903	rVB3	307	377	0.03%	0.004%
67	12.359	1910	1916	1929	rBV	690498	842830	62.87%	8.675%
68	12.648	1962	1965	1968	rVB3	216	287	0.02%	0.003%
69	12.689	1968	1972	1975	rVB2	333	419	0.03%	0.004%
70	12.800	1984	1991	1996	rBV2	1940	3415	0.25%	0.035%
71	13.018	2026	2028	2032	rVB2	364	422	0.03%	0.004%
72	13.153	2046	2051	2055	rVV2	654	939	0.07%	0.010%
73	13.230	2062	2064	2068	rVB2	268	350	0.03%	0.004%
74	13.442	2097	2100	2104	rVB2	253	352	0.03%	0.004%
75	13.630	2127	2132	2136	rBV3	1046	1179	0.09%	0.012%
76	13.730	2146	2149	2151	rVB3	443	431	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030121\
 Data File : VX020933.D
 Acq On : 01 Mar 2021 10:18
 Operator : JC/MD
 Sample : VX0301WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK406

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Title : VOC Analysis

77	13.759	2151	2154	2156	rVB2	237	257	0.02%	0.003%
78	13.818	2161	2164	2167	rVB2	628	561	0.04%	0.006%
79	13.942	2182	2185	2186	rBV2	246	311	0.02%	0.003%
80	14.007	2193	2196	2198	rVB2	702	603	0.04%	0.006%
81	14.101	2206	2212	2213	rBV3	154	257	0.02%	0.003%
82	14.165	2218	2223	2229	rBV4	1156	1882	0.14%	0.019%
83	14.259	2238	2239	2244	rVB3	379	471	0.04%	0.005%
84	14.307	2244	2247	2250	rBV3	326	524	0.04%	0.005%
85	14.465	2271	2274	2275	rBV2	289	361	0.03%	0.004%
86	14.518	2281	2283	2286	rVB4	399	442	0.03%	0.005%
87	14.554	2286	2289	2290	rBV3	254	319	0.02%	0.003%
88	14.642	2298	2304	2305	rBV3	269	389	0.03%	0.004%
89	14.718	2313	2317	2319	rBV4	371	451	0.03%	0.005%
90	14.765	2323	2325	2328	rBV3	313	442	0.03%	0.005%
91	14.824	2332	2335	2337	rBV3	282	403	0.03%	0.004%
92	14.860	2339	2341	2343	rBV3	383	389	0.03%	0.004%
93	14.954	2355	2357	2359	rBV2	398	291	0.02%	0.003%
94	15.413	2433	2435	2436	rBV2	496	337	0.03%	0.003%
95	15.436	2436	2439	2444	rVV6	700	1181	0.09%	0.012%
96	15.530	2453	2455	2456	rBV	532	359	0.03%	0.004%
97	15.813	2501	2503	2504	rBV2	548	395	0.03%	0.004%
98	15.895	2514	2517	2518	rBV3	386	449	0.03%	0.005%
99	16.272	2579	2581	2583	rBV2	447	284	0.02%	0.003%
100	16.542	2625	2627	2630	rBV3	443	298	0.02%	0.003%


Sum of corrected areas: 9715084

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030121\
Data File : VX020933.D
Acq On : 01 Mar 2021 10:18
Operator : JC/MD
Sample : VX0301WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK406

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

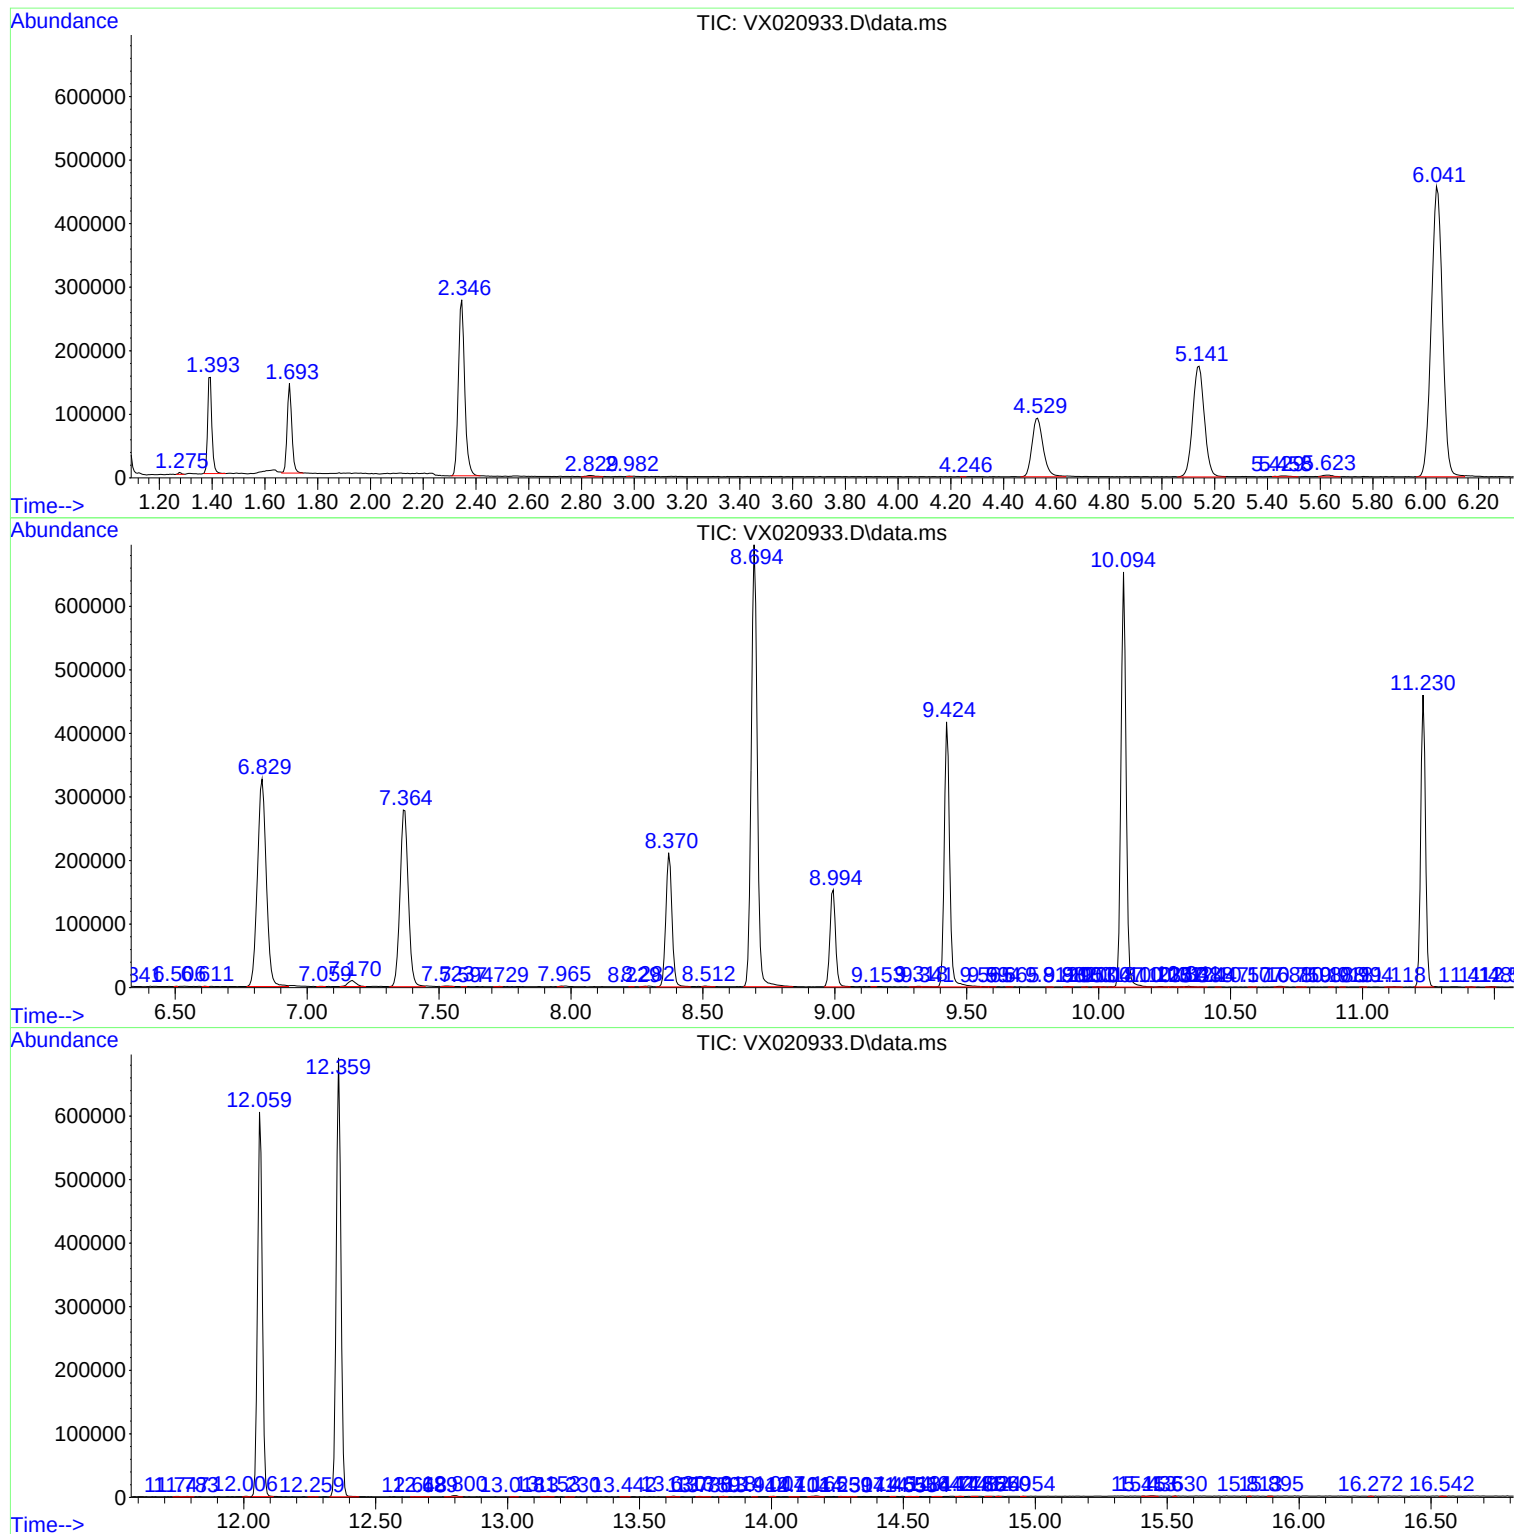

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030121\
Data File : VX020933.D
Acq On : 01 Mar 2021 10:18
Operator : JC/MD
Sample : VX0301WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK406

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030121\
Data File : VX020933.D
Acq On : 01 Mar 2021 10:18
Operator : JC/MD
Sample : VX0301WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK406

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
