


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030121\
 Data File : VX020931.D
 Acq On : 01 Mar 2021 08:30
 Operator : JC/MD
 Sample : BFB68
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB68

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM022621WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 03 01:05:22 2021

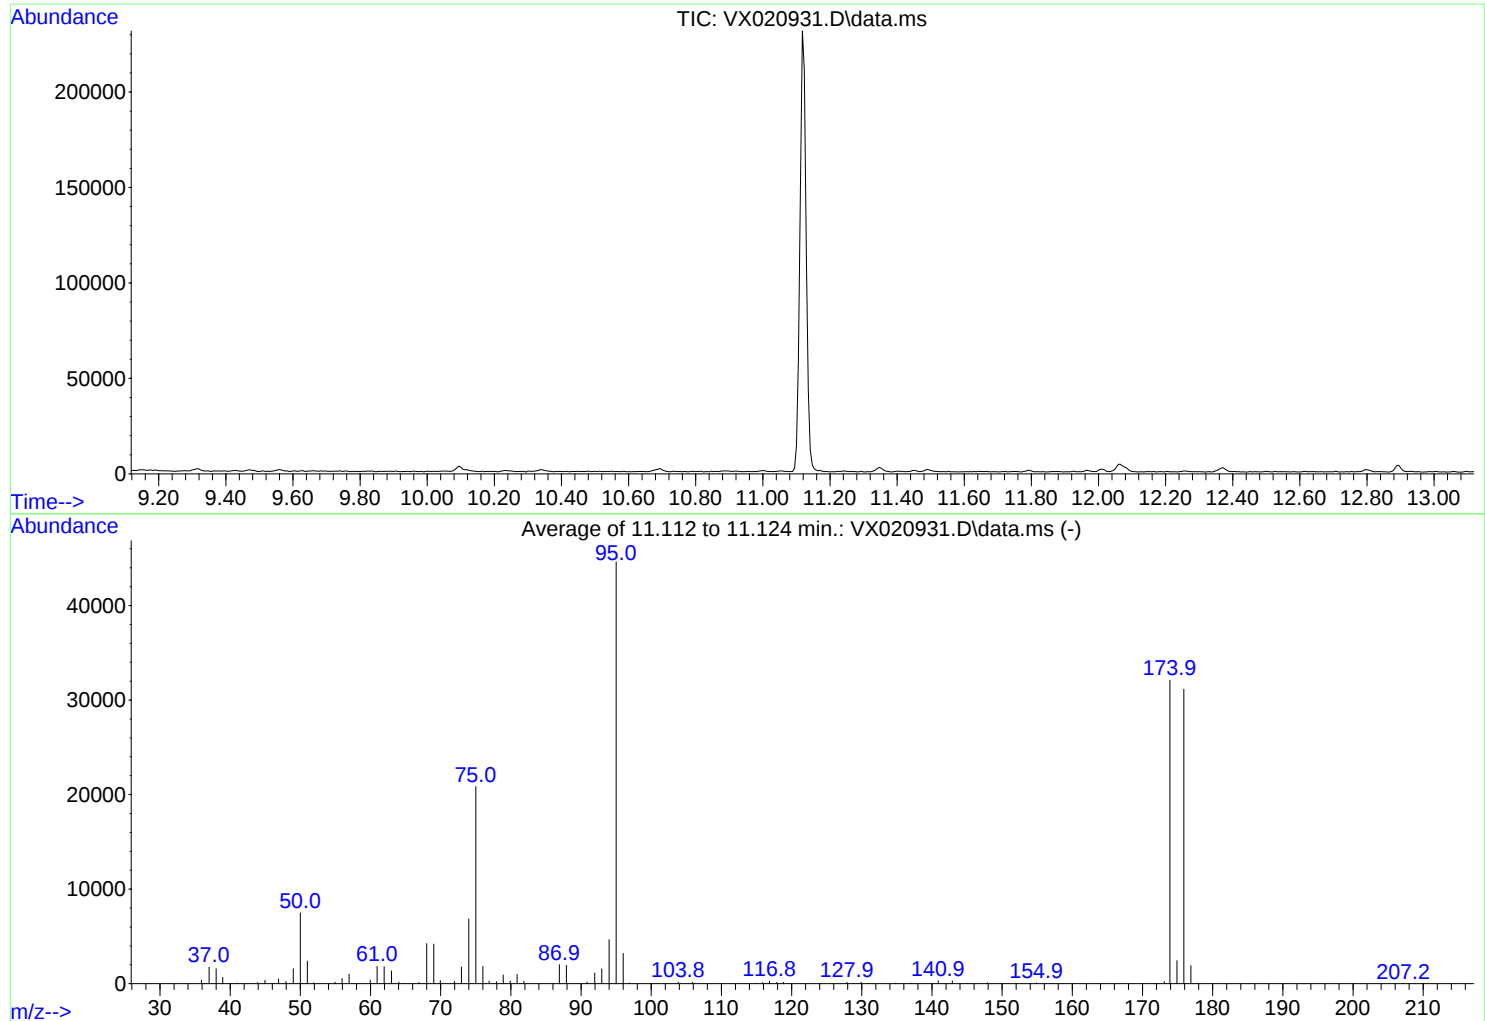

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1699

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	7477	PASS
75	95	30	80	46.7	20861	PASS
95	95	100	100	100.0	44624	PASS
96	95	5	9	7.2	3197	PASS
173	174	0.00	2	0.6	205	PASS
174	95	50	120	71.9	32101	PASS
175	174	5	9	7.6	2446	PASS
176	174	95	101	97.0	31141	PASS
177	176	5	9	6.1	1908	PASS

m/z	Abundance
35.90	291.0
37.00	1540.0
38.00	1363.0
39.00	576.0
39.90	484.0
41.00	77.0
43.10	59.0
43.90	753.0
44.90	293.0
46.90	396.0
48.00	180.0
49.00	1358.0
50.00	6378.0
51.00	1992.0
51.90	89.0
54.90	143.0
56.00	484.0
56.90	855.0
60.00	280.0
61.00	1544.0
62.00	1501.0
63.00	1255.0
64.10	167.0
66.90	94.0
68.00	3514.0
69.00	3586.0
70.00	269.0
71.90	232.0
72.90	1563.0
74.00	5629.0
75.00	17440.0
76.00	1592.0
76.90	205.0
77.90	217.0
78.90	746.0
79.90	243.0
80.90	867.0
81.80	226.0
86.90	1610.0
87.90	1539.0
90.90	143.0
91.90	785.0
93.00	1146.0
94.00	3797.0
95.00	34464.0
96.00	2643.0
96.90	59.0
103.80	85.0
105.90	145.0
115.90	111.0
116.90	171.0
117.90	98.0
118.80	140.0
127.90	114.0
129.90	77.0
140.90	287.0
142.90	164.0
147.90	91.0
156.80	54.0
173.20	259.0
173.90	22744.0
174.90	1694.0
175.90	19688.0
176.90	1408.0
207.00	87.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68

m/z	Abundance
35.90	379.0
37.00	2150.0
38.00	1916.0
38.90	774.0
39.90	571.0
41.00	91.0
43.00	68.0
43.90	672.0
44.90	428.0
46.90	537.0
47.90	220.0
49.00	1815.0
50.00	8786.0
51.00	2855.0
51.90	111.0
55.00	149.0
55.90	602.0
56.90	1203.0
59.90	401.0
60.90	2186.0
62.00	2067.0
63.00	1471.0
64.00	195.0
64.90	78.0
66.90	142.0
68.00	4936.0
69.00	4915.0
70.00	409.0
72.00	233.0
73.00	2046.0
74.00	8158.0
75.00	24336.0
76.00	2230.0
76.90	361.0
78.00	208.0
78.90	949.0
79.90	324.0
80.90	1058.0
81.90	308.0
86.90	2511.0
87.90	2301.0
90.90	177.0
92.00	1293.0
93.00	1941.0
94.00	5476.0
95.00	53248.0
96.00	3561.0
96.90	86.0
103.90	195.0
105.80	142.0
115.00	81.0
115.80	136.0
116.80	295.0
117.90	127.0
118.80	147.0
127.90	169.0
129.00	54.0
129.90	152.0
131.00	53.0
134.90	76.0
137.00	81.0
140.90	345.0
142.90	342.0
144.90	63.0
147.90	113.0
149.90	55.0
154.90	116.0
171.80	61.0
173.00	355.0
173.90	36392.0
174.90	2725.0
175.90	36416.0
176.90	2193.0
177.80	63.0
207.20	64.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68

m/z	Abundance
35.90	379.0
37.00	1552.0
38.00	1451.0
39.00	639.0
39.90	462.0
43.10	83.0
43.90	659.0
45.00	350.0
46.90	552.0
48.00	262.0
49.00	1537.0
50.00	7266.0
51.00	2309.0
51.90	73.0
55.00	158.0
56.00	539.0
57.00	982.0
59.90	431.0
61.00	1780.0
61.90	1836.0
63.00	1294.0
64.00	118.0
66.90	121.0
68.00	4260.0
69.00	4037.0
69.90	301.0
72.00	193.0
73.00	1691.0
74.00	6732.0
75.00	20808.0
76.00	1669.0
76.90	245.0
78.00	206.0
78.90	1069.0
79.90	302.0
80.90	1033.0
81.90	209.0
86.90	1908.0
87.90	1968.0
90.80	134.0
91.90	1266.0
92.90	1615.0
94.00	4683.0
95.00	46160.0
96.00	3388.0
96.90	87.0
103.80	176.0
105.90	128.0
115.80	132.0
116.90	272.0
117.90	156.0
118.90	147.0
127.90	142.0
129.90	167.0
130.90	68.0
134.80	76.0
137.00	68.0
140.90	307.0
142.90	346.0
145.00	59.0
147.90	111.0
149.90	56.0
154.90	151.0
157.00	74.0
173.90	37168.0
174.90	2919.0
175.90	37320.0
176.90	2124.0
177.80	79.0
207.00	140.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68

m/z	Abundance
39.90	510.0
42.20	56.0
43.00	59.0
43.90	578.0
207.10	61.0

Instrument :
MSVOA_X
ClientSampleId :
BFB68