

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030122\
 Data File : VX027260.D
 Acq On : 01 Mar 2022 19:48
 Operator : JC/MD
 Sample : N1725-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M

Title : SW846 8260

Signal : TIC: VX027260.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	21	27	41	rBV	21152	61771	14.81%	2.613%
2	1.453	57	60	65	rBV	3640	4582	1.10%	0.194%
3	2.386	206	213	221	rBV	5352	8731	2.09%	0.369%
4	2.538	231	238	244	rBV2	5415	11150	2.67%	0.472%
5	5.391	695	706	722	rBV	49117	141445	33.92%	5.983%
6	5.556	722	733	751	rVB	85192	238482	57.19%	10.087%
7	5.964	789	800	813	rBV2	50578	135433	32.48%	5.729%
8	6.769	920	932	947	rBV	129468	307920	73.84%	13.025%
9	8.653	1234	1241	1250	rBV	267859	417002	100.00%	17.638%
10	9.458	1367	1373	1380	rBV	3197	4730	1.13%	0.200%
11	10.055	1465	1471	1485	rBV	280645	368350	88.33%	15.581%
12	11.079	1634	1639	1650	rBV	216859	280181	67.19%	11.851%
13	12.024	1789	1794	1803	rVB	299742	359266	86.15%	15.196%
14	13.780	2075	2082	2086	rBV	13225	17234	4.13%	0.729%
15	16.328	2494	2500	2507	rVB2	4520	7882	1.89%	0.333%




Sum of corrected areas: 2364159

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030122\
Data File : VX027260.D
Acq On : 01 Mar 2022 19:48
Operator : JC/MD
Sample : N1725-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

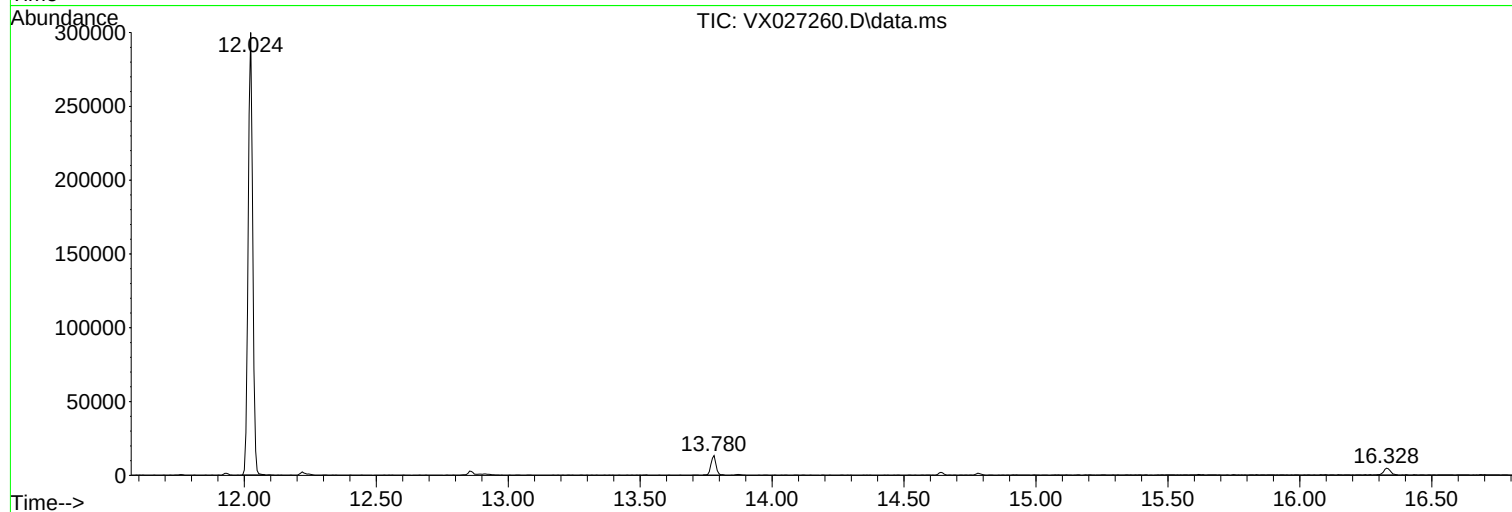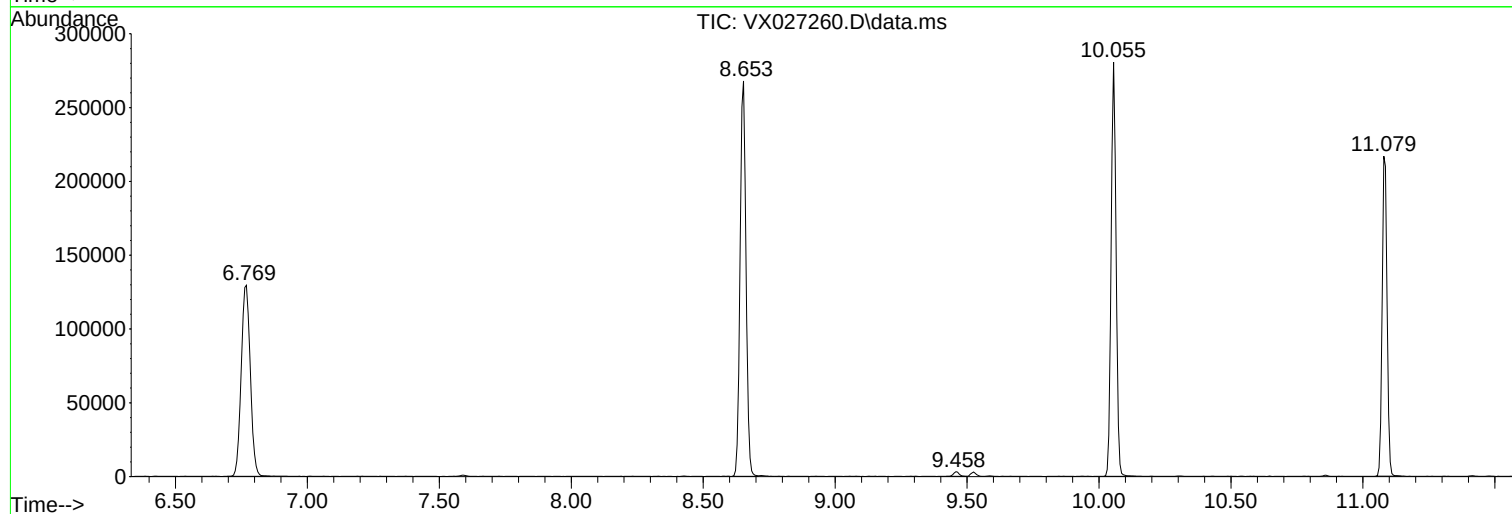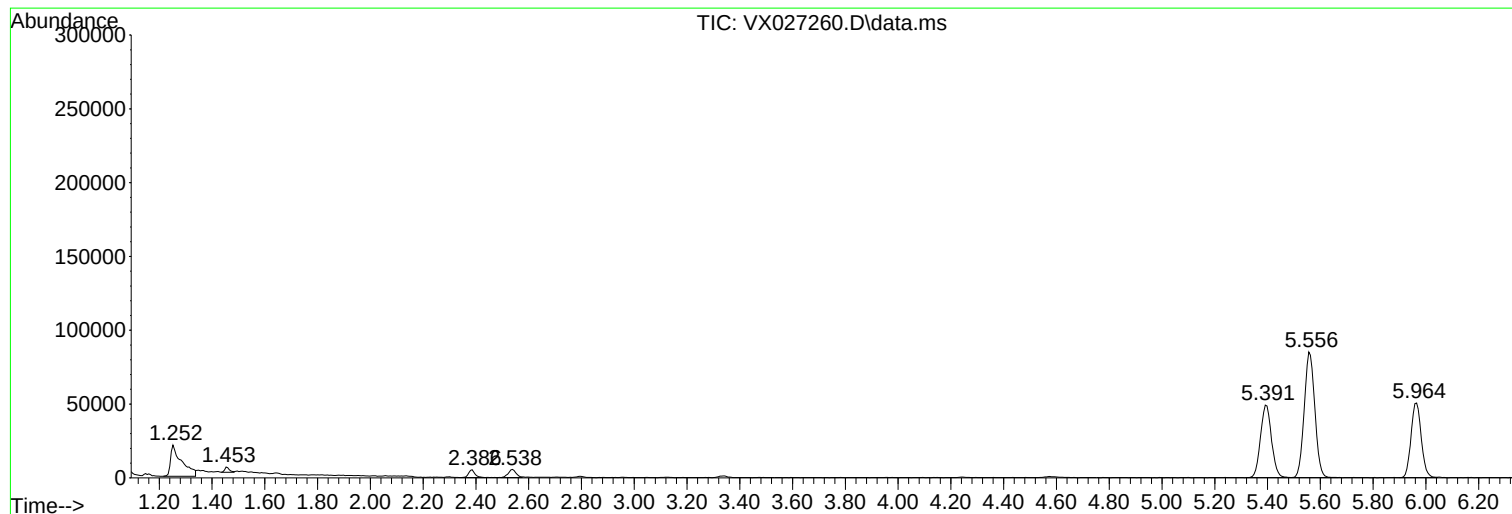

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030122\
Data File : VX027260.D
Acq On : 01 Mar 2022 19:48
Operator : JC/MD
Sample : N1725-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-01










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.252	12.95 ug/l	61771	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethyl Chloride	64	C2H5Cl	000075-00-3	3
5			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	3

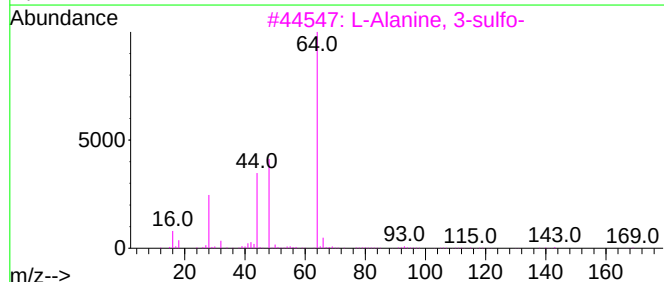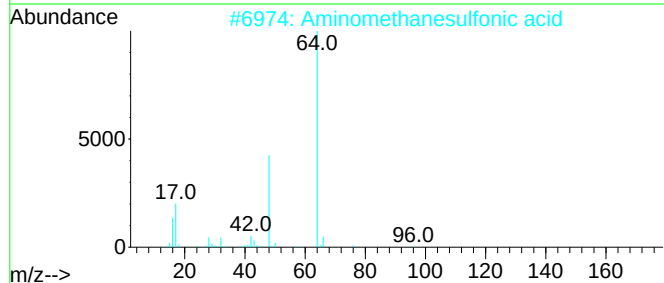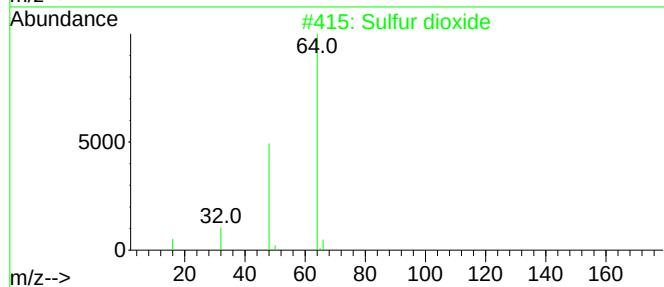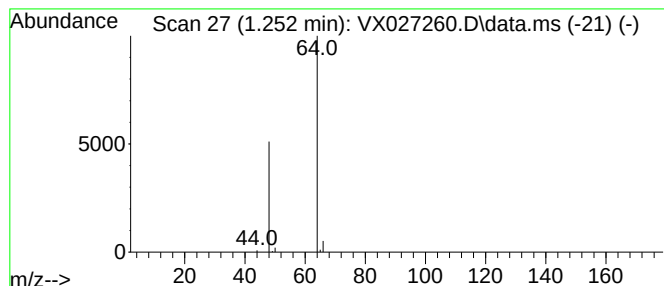

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030122\
Data File : VX027260.D
Acq On : 01 Mar 2022 19:48
Operator : JC/MD
Sample : N1725-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.252	12.9	ug/l	61771	1	5.556	238482	50.0