


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030123\
Data File : VX034279.D
Acq On : 01 Mar 2023 08:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Title : SW846 8260
Last Update : Fri Feb 17 12:33:35 2023

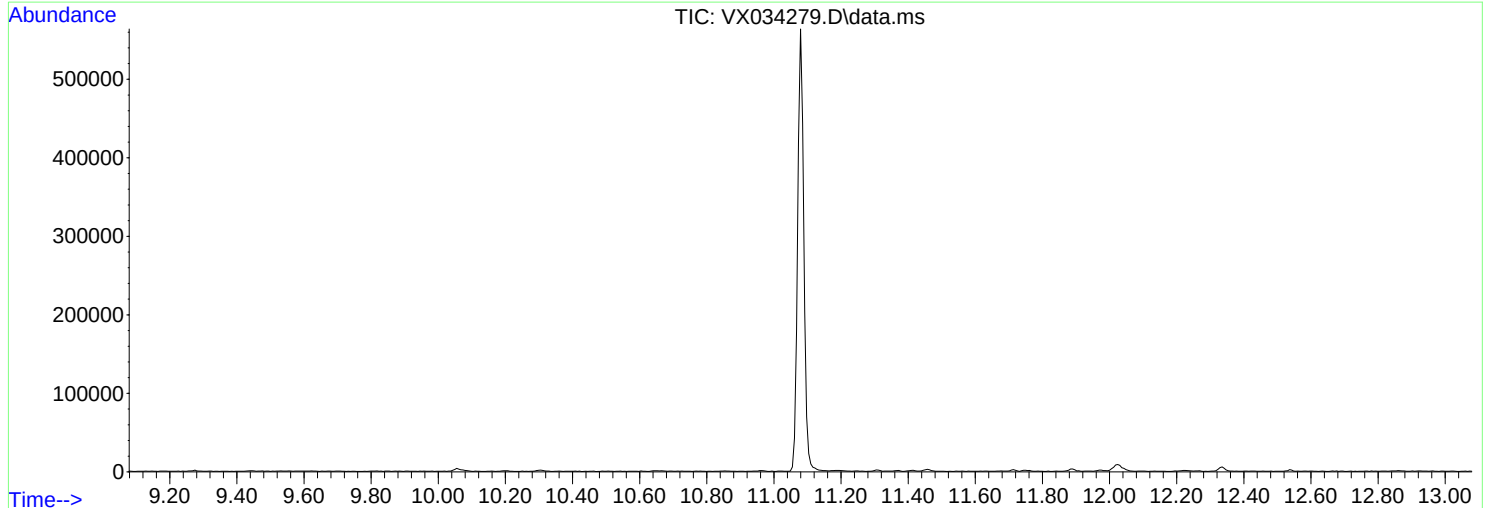

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	18654	PASS
75	95	30	60	49.0	48216	PASS
95	95	100	100	100.0	98488	PASS
96	95	5	9	6.5	6432	PASS
173	174	0.00	2	0.9	681	PASS
174	95	50	100	80.6	79352	PASS
175	174	5	9	7.5	5936	PASS
176	174	95	101	96.6	76664	PASS
177	176	5	9	6.6	5023	PASS