

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030221\
 Data File : VX020952.D
 Acq On : 01 Mar 2021 22:14
 Operator : JC/MD
 Sample : M1535-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW807-41-46-022721

Quant Time: Mar 02 00:34:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 24 13:50:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.623	168	196052	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	363044	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	343037	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	144188	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	128185	48.41	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	96.82%
35) Dibromofluoromethane	5.464	113	111711	50.64	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	101.28%
50) Toluene-d8	8.694	98	439314	51.08	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	102.16%
62) 4-Bromofluorobenzene	11.118	95	163145	51.30	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	102.60%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.164	85	466	0.22	ug/l	98
4) Vinyl Chloride	1.399	62	1532	0.56	ug/l	98
5) Bromomethane	1.640	94	351	Below Cal		88
9) 1,1,2-Trichlorotrifluo...	2.358	101	461	0.22	ug/l #	19
11) Tert butyl alcohol	2.993	59	2378	4.03	ug/l #	76
12) 1,1-Dichloroethene	2.358	96	176187	80.29	ug/l	98
13) Acrolein	2.275	56	378	1.04	ug/l #	14
16) Acetone	2.423	43	5323	4.88	ug/l	97
17) Carbon Disulfide	2.552	76	1635	0.26	ug/l #	94
18) Methyl Acetate	2.752	43	744	0.29	ug/l #	73
20) Methylene Chloride	2.834	84	962	0.37	ug/l	97
21) trans-1,2-Dichloroethene	3.146	96	15390	6.24	ug/l	90
24) 1,1-Dichloroethane	3.670	63	33431	7.87	ug/l	99
25) 2-Butanone	4.640	43	1559	0.94	ug/l #	83
27) cis-1,2-Dichloroethene	4.564	96	168009	59.16	ug/l	85
29) Tetrahydrofuran	5.111	42	628	0.59	ug/l #	61
30) Chloroform	5.170	83	19301	4.51	ug/l	97
31) Cyclohexane	5.623	56	3991	1.04	ug/l #	1
36) 1,1-Dichloropropene	5.629	75	15098	4.38	ug/l #	48
38) Carbon Tetrachloride	5.623	117	18810	5.63	ug/l #	16
40) Benzene	6.117	78	4762	0.46	ug/l	96
42) 1,2-Dichloroethane	6.158	62	23500	6.83	ug/l	98
44) Trichloroethene	7.188	130	86670	31.87	ug/l	100
47) Bromodichloromethane	7.876	83	1741	0.48	ug/l	90
49) 1,4-Dioxane	7.723	88	5580	85.34	ug/l	95
51) 4-Methyl-2-Pentanone	8.617	43	1005	0.31	ug/l #	50
74) N-amyl acetate	10.894	43	4279	0.93	ug/l #	3
76) 1,2,3-Trichloropropane	11.118	75	77331	24.93	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.118	75	77331	55.20	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030221\
Data File : VX020952.D
Acq On : 01 Mar 2021 22:14
Operator : JC/MD
Sample : M1535-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721


Quant Time: Mar 02 00:34:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 24 13:50:55 2021
Response via : Initial Calibration

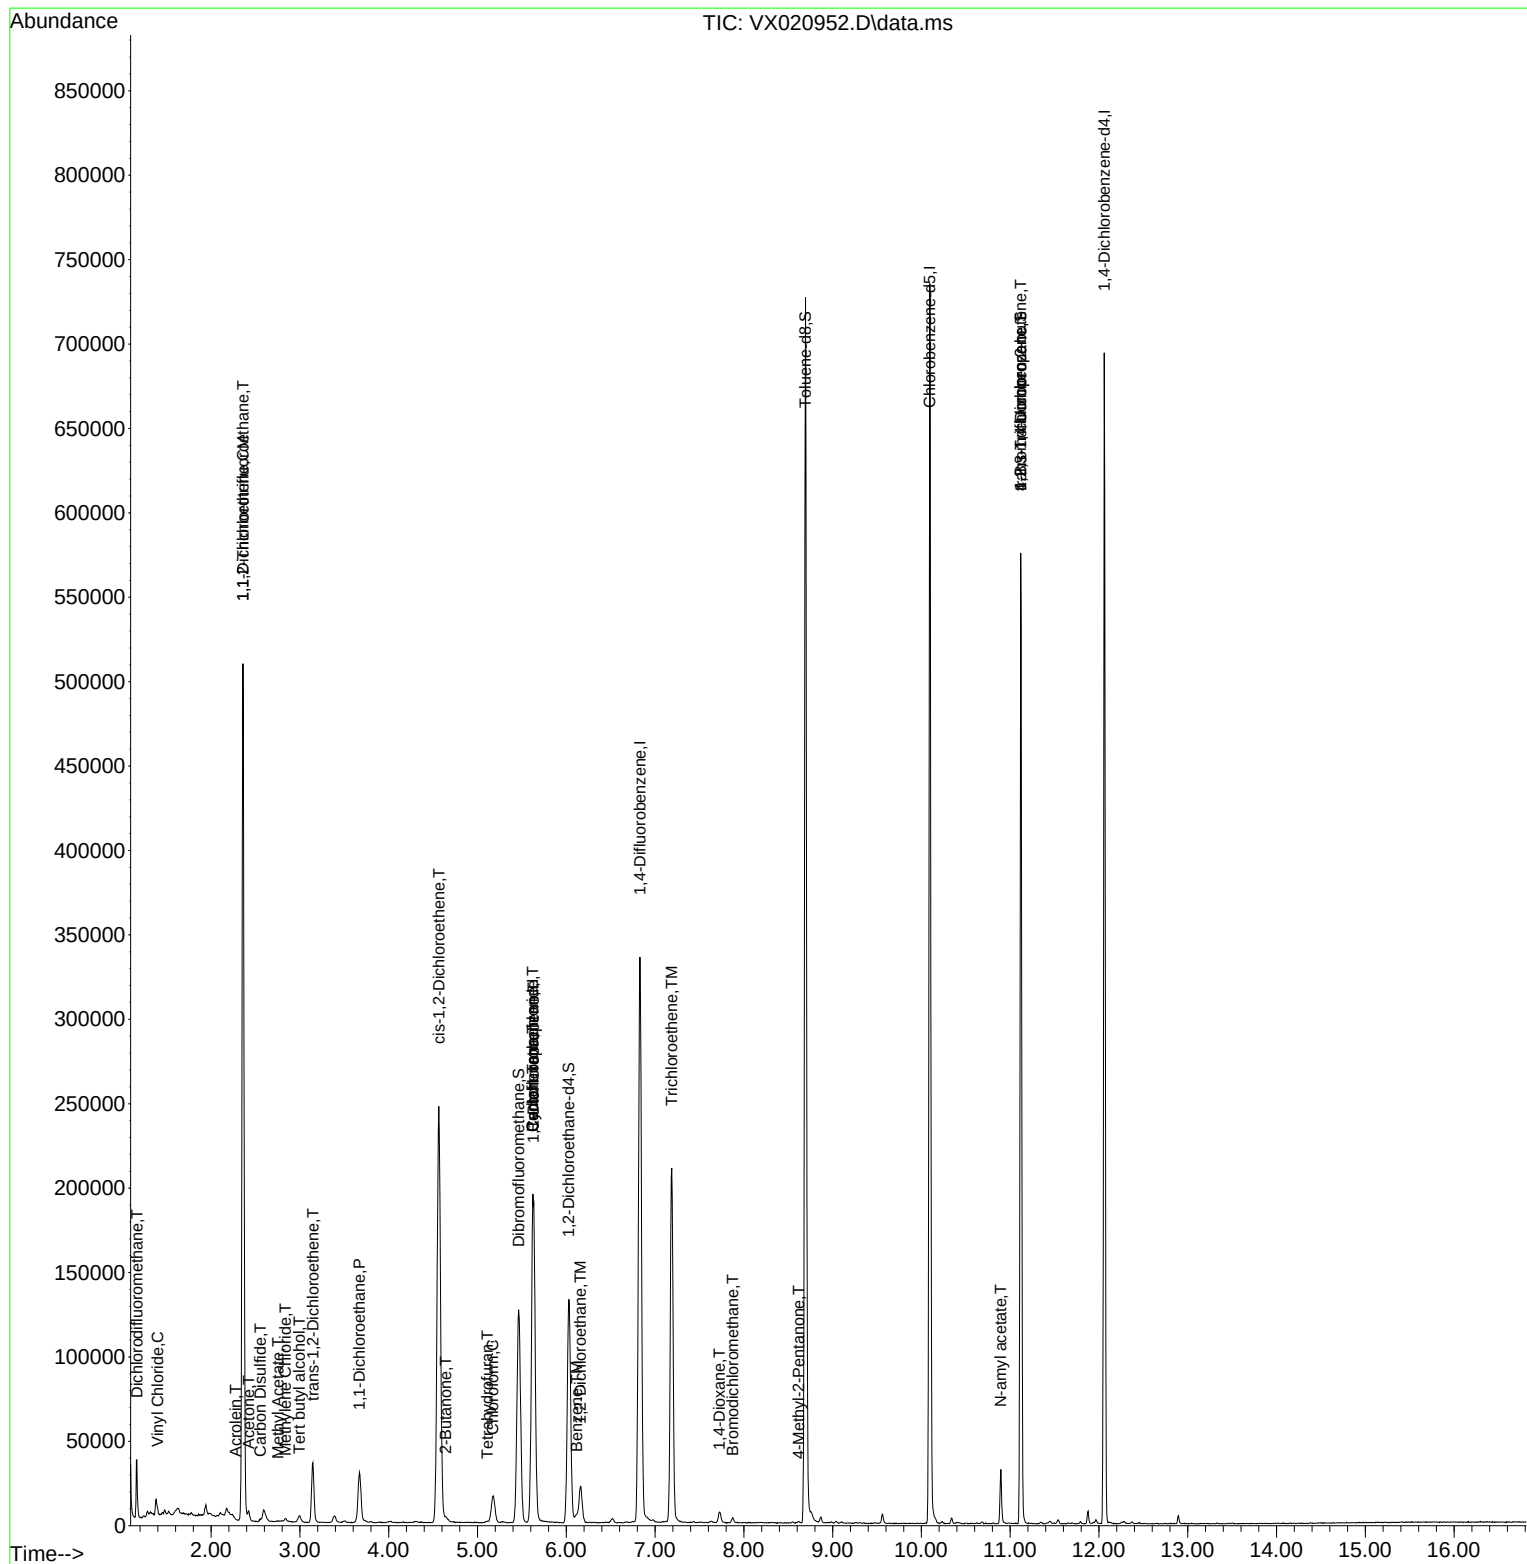






#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721



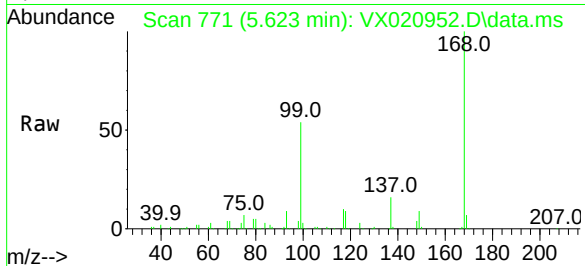



Tgt Ion:168 Resp: 196052
Ion Ratio Lower Upper
168 100
99 54.5 45.8 68.6



#2
Dichlorodifluoromethane
Concen: 0.22 ug/l
RT: 1.164 min Scan# 13
Delta R.T. -0.024 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

Tgt Ion: 85 Resp: 466
Ion Ratio Lower Upper
85 100
87 33.7 16.4 49.2


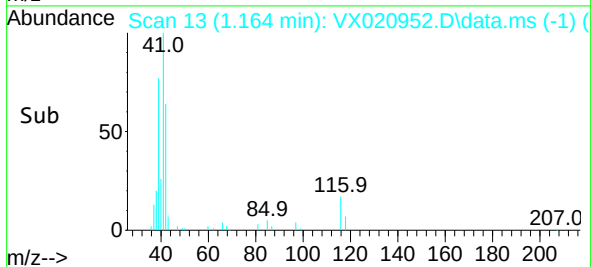

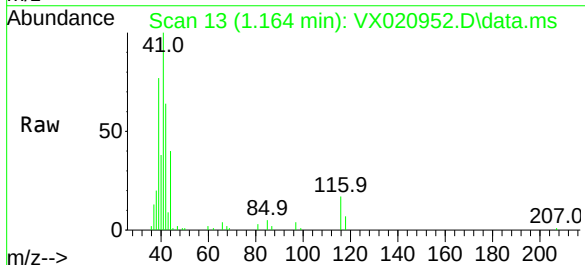


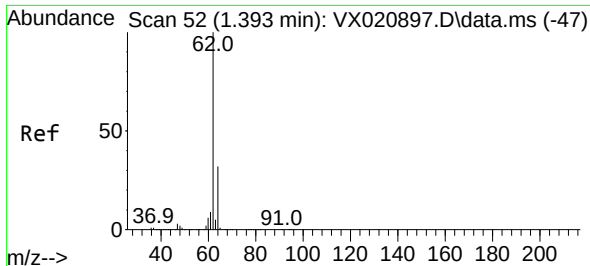

#4
 Vinyl Chloride
 Concen: 0.56 ug/l
 RT: 1.399 min Scan# 53
 Delta R.T. 0.006 min
 Lab File: VX020952.D
 Acq: 01 Mar 2021 22:14




Instrument :
 MSVOA_X
 ClientSampleId :
 GW807-41-46-022721


Tgt Ion: 62 Resp: 1532
 Ion Ratio Lower Upper
 62 100
 64 33.4 25.7 38.5

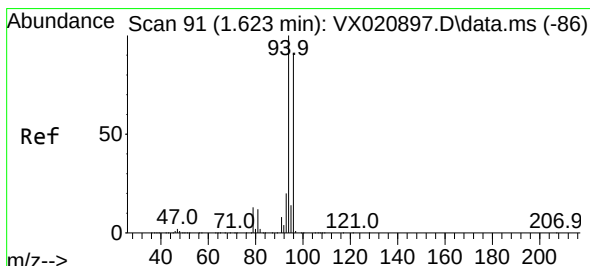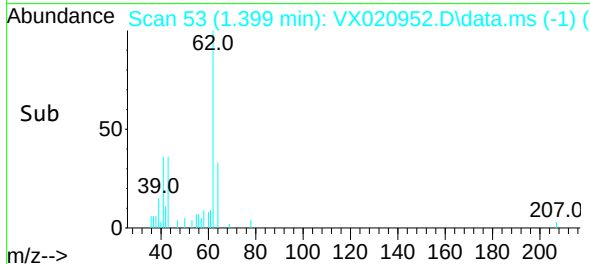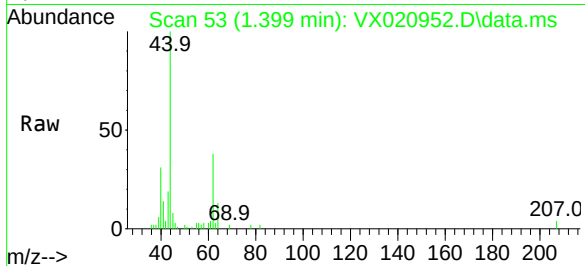

#5
 Bromomethane
 Concen: Below Cal
 RT: 1.640 min Scan# 94
 Delta R.T. 0.017 min
 Lab File: VX020952.D
 Acq: 01 Mar 2021 22:14

Tgt Ion: 94 Resp: 351
 Ion Ratio Lower Upper
 94 100
 96 107.1 76.4 114.6


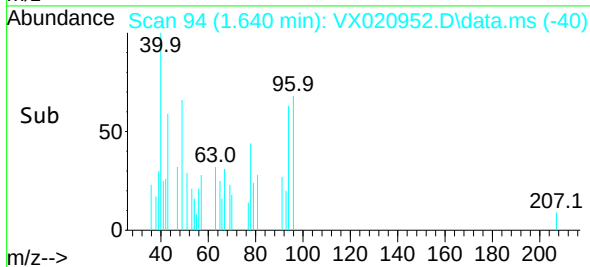

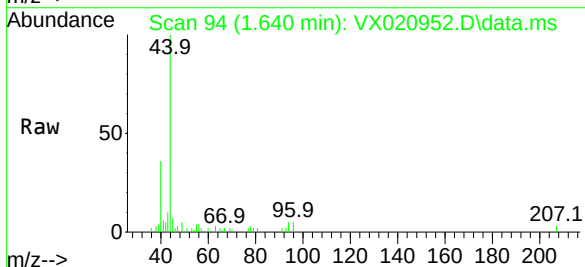




#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.22 ug/l
RT: 2.358 min Scan# 216
Delta R.T. -0.006 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14




Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721


Tgt Ion:101 Resp: 461
Ion Ratio Lower Upper
101 100
85 0.0 34.9 52.3#
151 0.0 61.4 92.2#

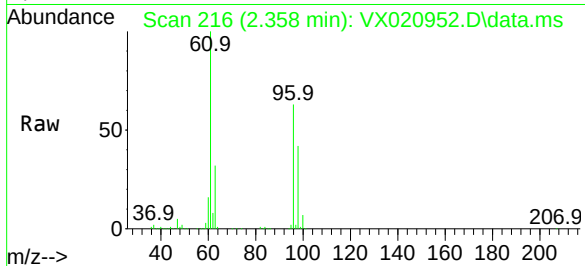

#11
Tert butyl alcohol
Concen: 4.03 ug/l
RT: 2.993 min Scan# 324
Delta R.T. -0.024 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14


Tgt Ion: 59 Resp: 2378
Ion Ratio Lower Upper
59 100
57 0.8 7.8 11.8#

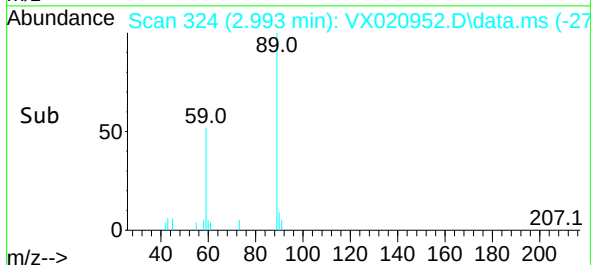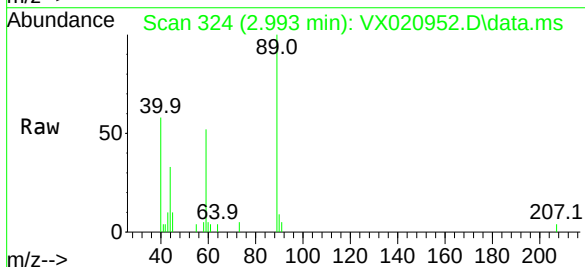






#12
 1,1-Dichloroethene
 Concen: 80.29 ug/l
 RT: 2.358 min Scan# 216
 Delta R.T. 0.006 min
 Lab File: VX020952.D
 Acq: 01 Mar 2021 22:14

Instrument :
 MSVOA_X
 ClientSampleId :
 GW807-41-46-022721



Tgt Ion: 96 Resp: 176187




Ion	Ratio	Lower	Upper
96	100		
61	157.8	124.6	187.0
98	66.8	50.6	76.0




#13
 Acrolein
 Concen: 1.04 ug/l
 RT: 2.275 min Scan# 202
 Delta R.T. -0.000 min
 Lab File: VX020952.D
 Acq: 01 Mar 2021 22:14

Tgt Ion: 56 Resp: 378

Ion	Ratio	Lower	Upper
56	100		
55	0.0	56.4	84.6#


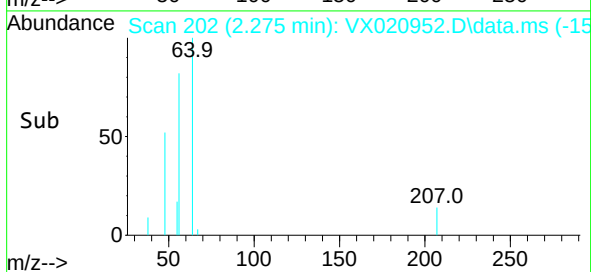






#16
Acetone
Concen: 4.88 ug/l
RT: 2.423 min Scan# 227
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14




Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721


Tgt Ion: 43 Resp: 5323
Ion Ratio Lower Upper
43 100
58 32.8 27.8 41.8

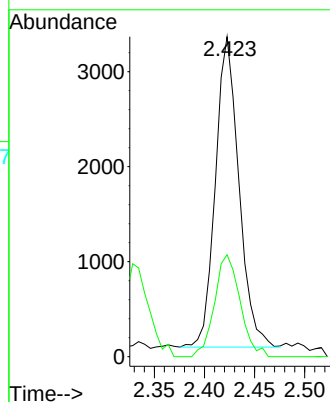

#17
Carbon Disulfide
Concen: 0.26 ug/l
RT: 2.552 min Scan# 249
Delta R.T. 0.006 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

Tgt Ion: 76 Resp: 1635
Ion Ratio Lower Upper
76 100
78 11.1 7.2 10.8#







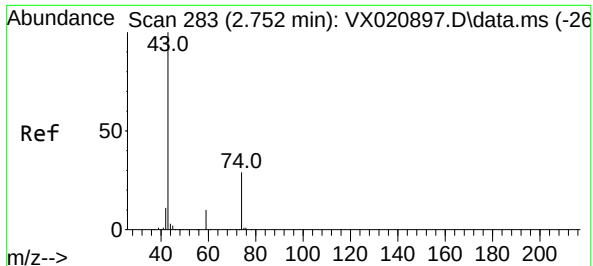

#18
Methyl Acetate
Concen: 0.29 ug/l
RT: 2.752 min Scan# 283
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14




Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721


Tgt Ion: 43 Resp: 744
Ion Ratio Lower Upper
43 100
74 13.6 21.9 32.9#

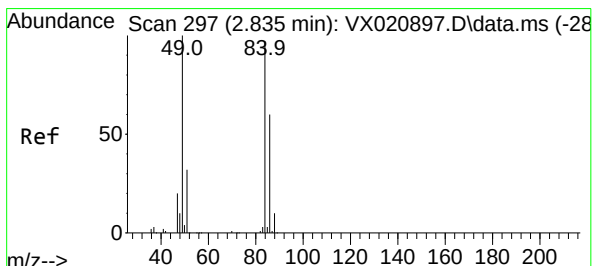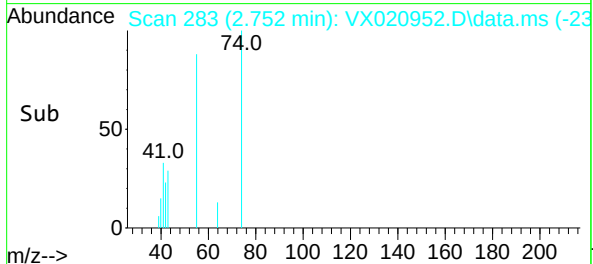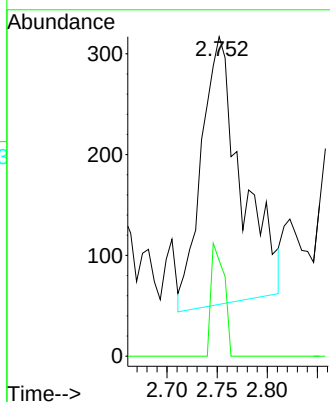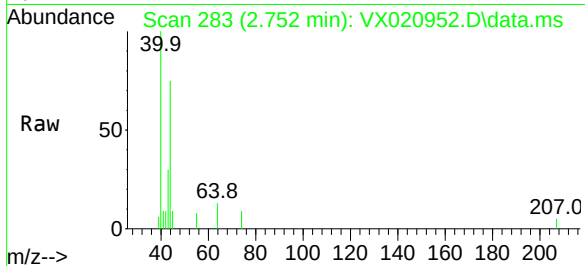

#20
Methylene Chloride
Concen: 0.37 ug/l
RT: 2.834 min Scan# 297
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

Tgt Ion: 84 Resp: 962
Ion Ratio Lower Upper
84 100
49 109.4 88.6 132.8
51 31.9 27.0 40.6
86 59.1 50.3 75.5


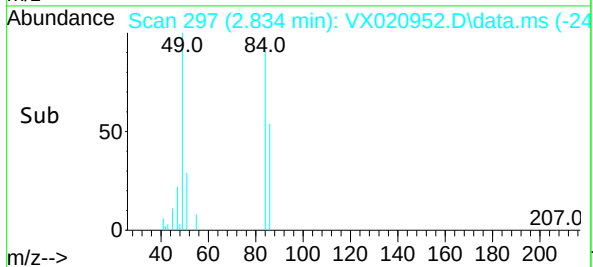

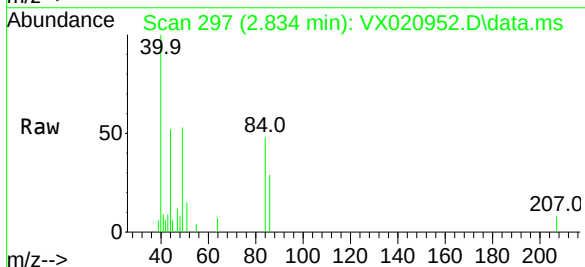


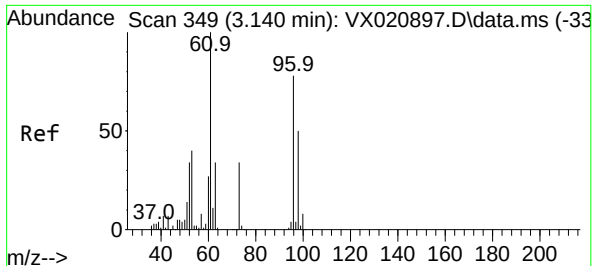

#21
trans-1,2-Dichloroethene
Concen: 6.24 ug/l
RT: 3.146 min Scan# 350
Delta R.T. 0.006 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14




Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721


Tgt Ion: 96 Resp: 15390
Ion Ratio Lower Upper
96 100
61 118.7 107.7 161.5
98 59.7 50.4 75.6

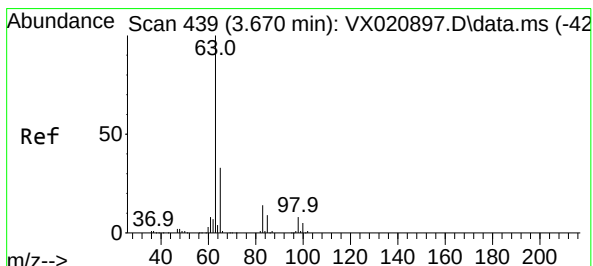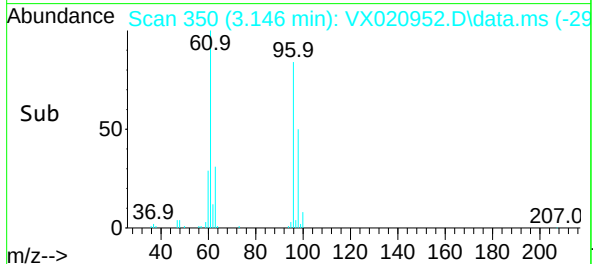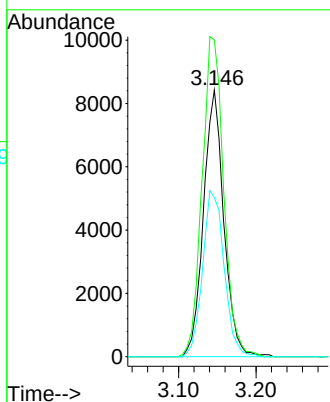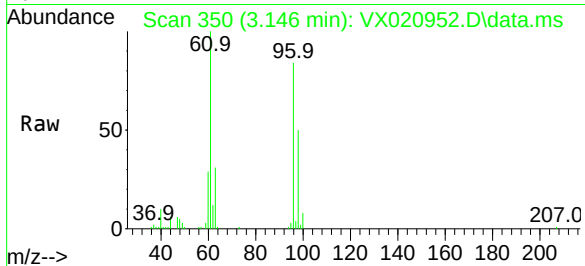

#24
1,1-Dichloroethane
Concen: 7.87 ug/l
RT: 3.670 min Scan# 439
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

Tgt Ion: 63 Resp: 33431
Ion Ratio Lower Upper
63 100
98 7.4 3.8 11.2
100 4.6 2.5 7.5


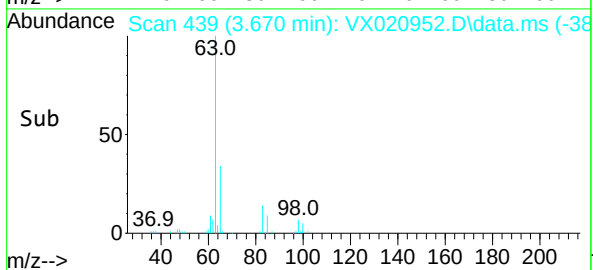

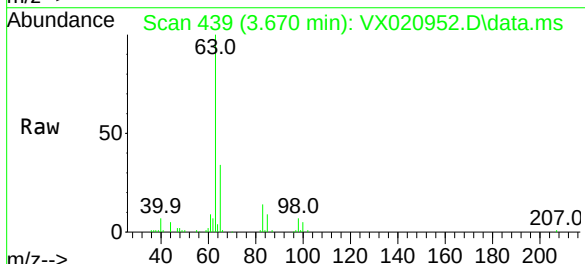




#25
2-Butanone
Concen: 0.94 ug/l
RT: 4.640 min Scan# 604
Delta R.T. 0.006 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14




Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721


Tgt Ion: 43 Resp: 1559
Ion Ratio Lower Upper
43 100
72 20.3 23.7 35.5#

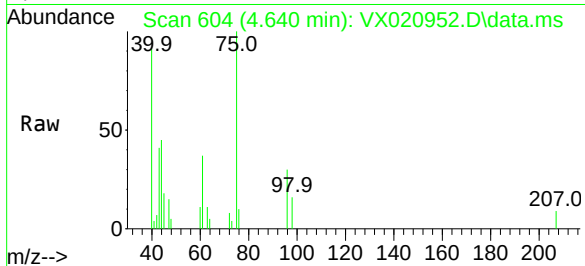

#27
cis-1,2-Dichloroethene
Concen: 59.16 ug/l
RT: 4.564 min Scan# 591
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

Tgt Ion: 96 Resp: 168009
Ion Ratio Lower Upper
96 100
61 116.3 0.0 285.6
98 64.1 0.0 129.6

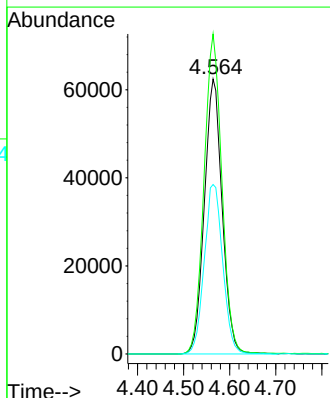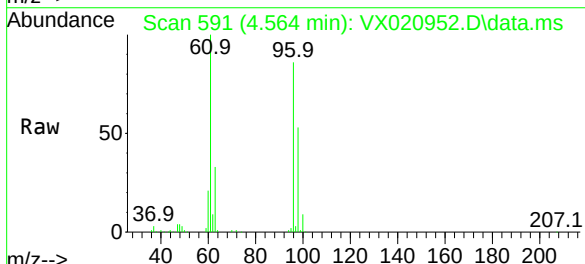



#29

Tetrahydrofuran

Concen: 0.59 ug/l

RT: 5.111 min Scan# 684

Delta R.T. 0.023 min

Lab File: VX020952.D


Acq: 01 Mar 2021 22:14

Instrument :




MSVOA_X

ClientSampleId :

GW807-41-46-022721



Tgt Ion:	42	Resp:	628
Ion	Ratio	Lower	Upper
42	100		
72	14.2	41.7	62.5#
71	32.6	38.4	57.6#



#30

Chloroform

Concen: 4.51 ug/l




RT: 5.170 min Scan# 694


Delta R.T. -0.006 min

Lab File: VX020952.D

Acq: 01 Mar 2021 22:14


Tgt Ion:	83	Resp:	19301
Ion	Ratio	Lower	Upper
83	100		
85	62.4	52.0	78.0

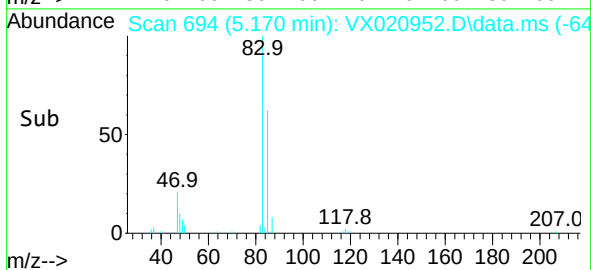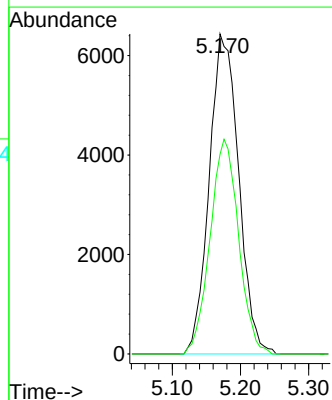






#31
Cyclohexane
Concen: 1.04 ug/l
RT: 5.623 min Scan# 771
Delta R.T. 0.076 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14


Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721





Tgt Ion: 56 Resp: 3991
Ion Ratio Lower Upper
56 100
69 166.2 25.3 37.9#
84 142.7 71.4 107.0#




#33
1,2-Dichloroethane-d4
Concen: 48.41 ug/l
RT: 6.029 min Scan# 840
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

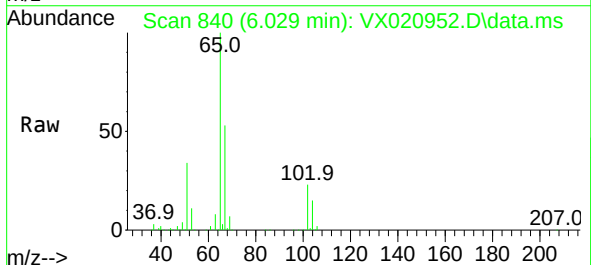


Tgt Ion: 65 Resp: 128185
Ion Ratio Lower Upper
65 100
67 53.1 0.0 105.4

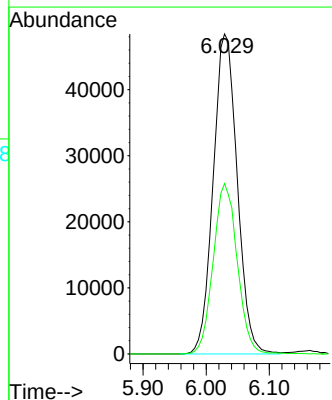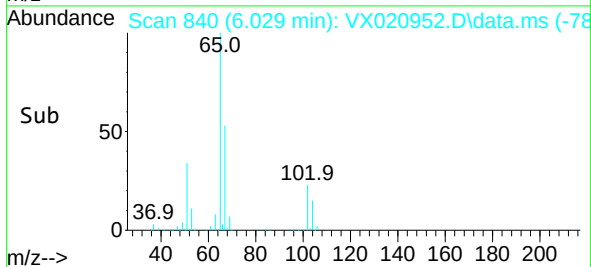






#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.829 min Scan# 976
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14


Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721

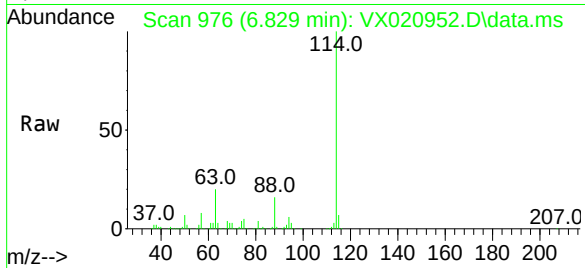



Tgt Ion:114 Resp: 363044
Ion Ratio Lower Upper
114 100
63 19.9 0.0 40.8
88 16.4 0.0 32.8

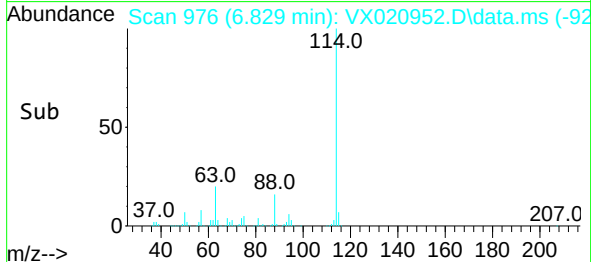


#35
Dibromofluoromethane
Concen: 50.64 ug/l
RT: 5.464 min Scan# 744
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

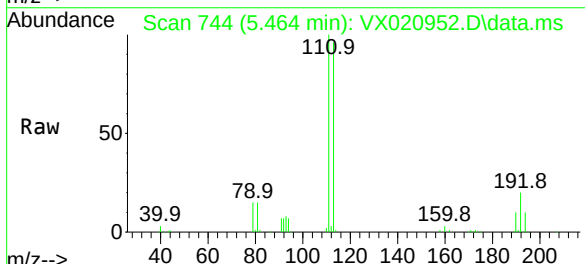


Tgt Ion:113 Resp: 111711
Ion Ratio Lower Upper
113 100
111 103.4 81.9 122.9
192 21.0 16.7 25.1

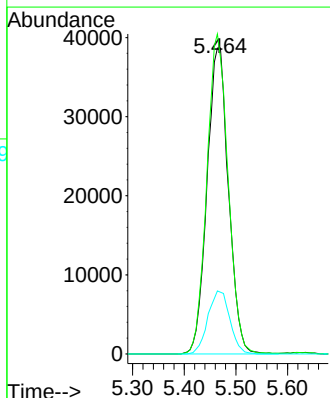






#36
1,1-Dichloropropene
Concen: 4.38 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.141 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14


Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721

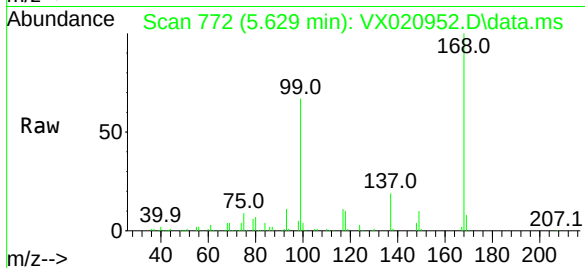



Tgt Ion: 75 Resp: 15098
Ion Ratio Lower Upper
75 100
110 8.7 18.1 54.4#
77 0.0 25.3 37.9#




#38
Carbon Tetrachloride
Concen: 5.63 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.130 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

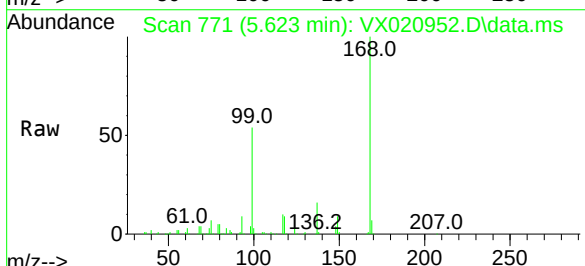

Tgt Ion: 117 Resp: 18810
Ion Ratio Lower Upper
117 100
119 4.4 76.2 114.2#
121 0.0 24.8 37.2#



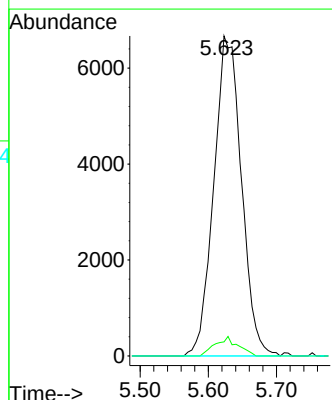
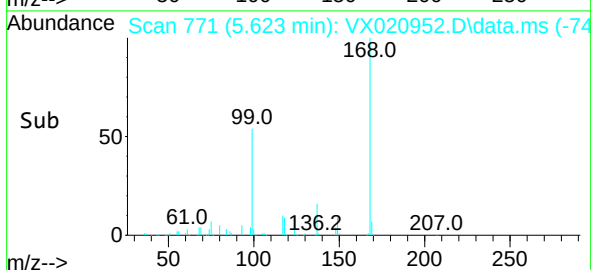




#40
Benzene
Concen: 0.46 ug/l
RT: 6.117 min Scan# 855
Delta R.T. 0.006 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14




Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721


Tgt Ion: 78 Resp: 4762
Ion Ratio Lower Upper
78 100
77 21.8 18.9 28.3



#42
1,2-Dichloroethane
Concen: 6.83 ug/l
RT: 6.158 min Scan# 862
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

Tgt Ion: 62 Resp: 23500
Ion Ratio Lower Upper
62 100
98 10.8 0.0 20.2

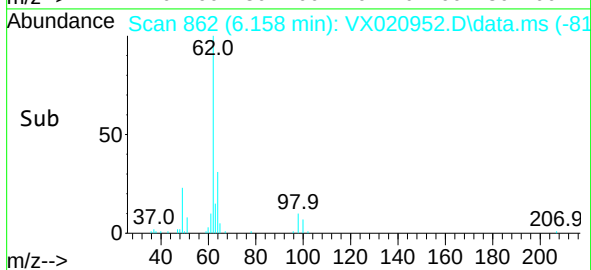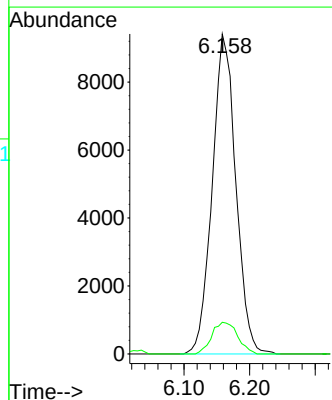

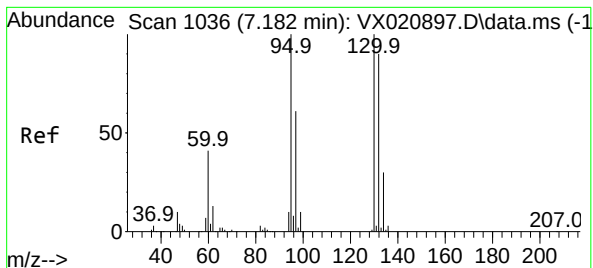

#44

Trichloroethene

Concen: 31.87 ug/l

RT: 7.188 min Scan# 1037

Delta R.T. 0.006 min

Lab File: VX020952.D





Acq: 01 Mar 2021 22:14

Tgt Ion:130 Resp: 86670

Ion Ratio Lower Upper

130 100

95 99.0 0.0 198.0

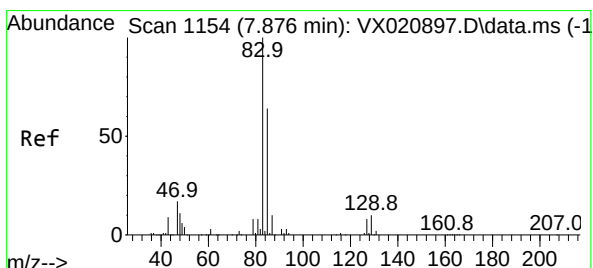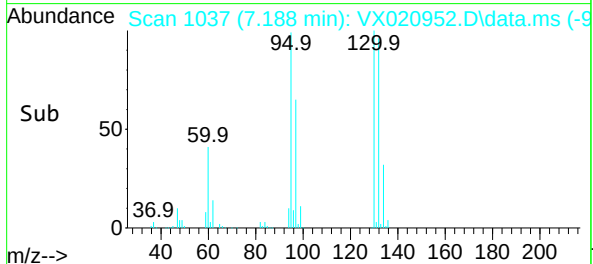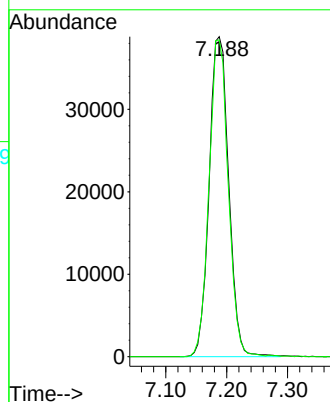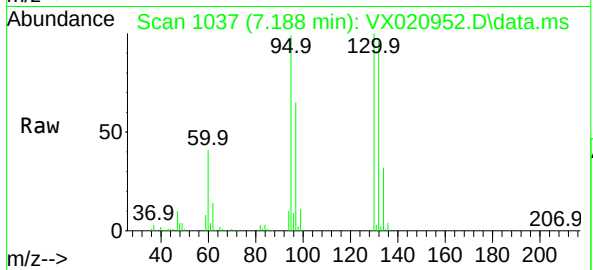

#47

Bromodichloromethane

Concen: 0.48 ug/l

RT: 7.876 min Scan# 1154

Delta R.T. -0.000 min

Lab File: VX020952.D

Acq: 01 Mar 2021 22:14




Tgt Ion: 83 Resp: 1741


Ion Ratio Lower Upper

83 100

85 55.7 51.4 77.0

127 8.2 6.8 10.2


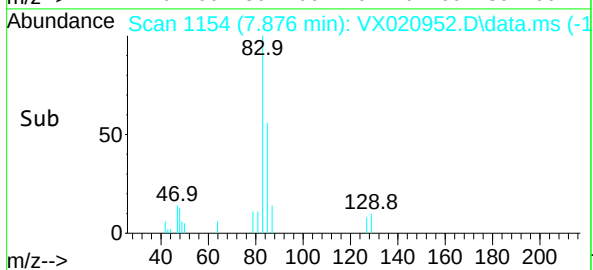
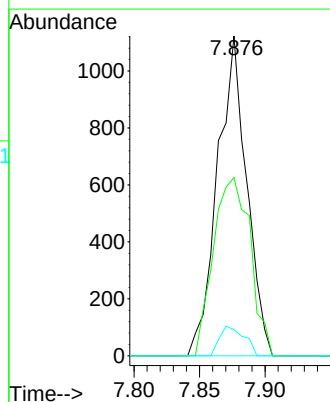
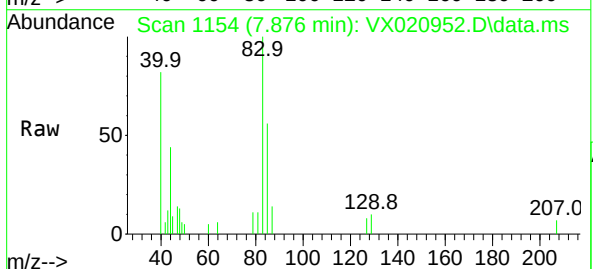


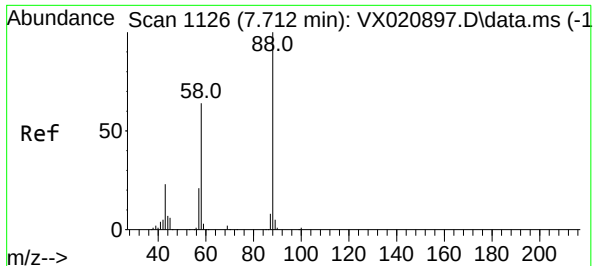

#49
1,4-Dioxane
Concen: 85.34 ug/l
RT: 7.723 min Scan# 1128
Delta R.T. 0.012 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14




Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721


Tgt Ion: 88 Resp: 5580
Ion Ratio Lower Upper
88 100
43 25.3 23.2 34.8
58 64.8 55.0 82.4

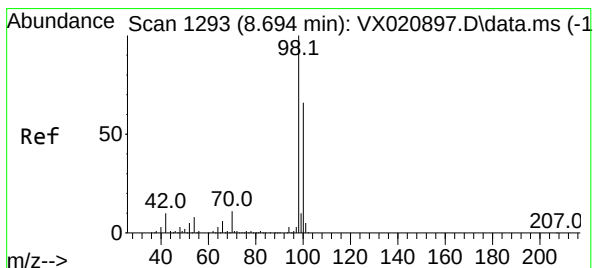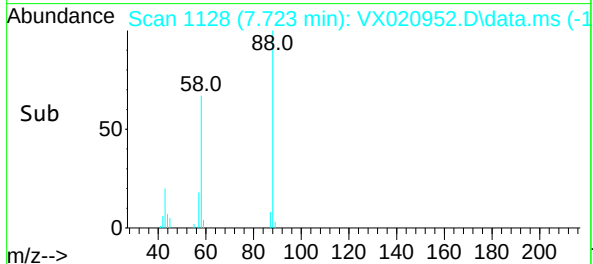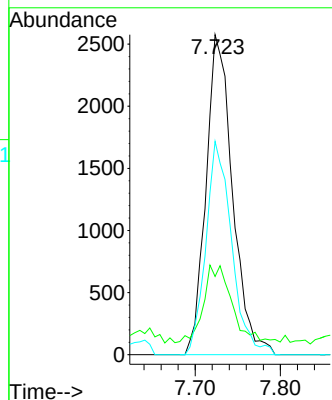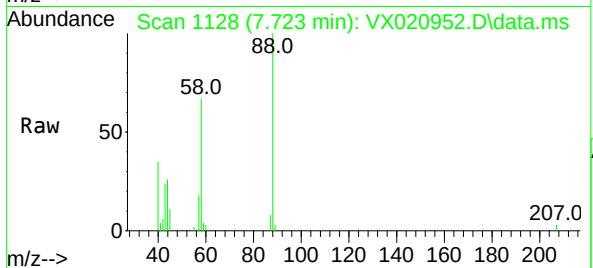

#50
Toluene-d8
Concen: 51.08 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

Tgt Ion: 98 Resp: 439314
Ion Ratio Lower Upper
98 100
100 68.0 51.9 77.9


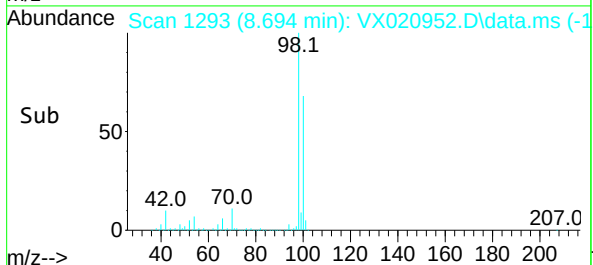
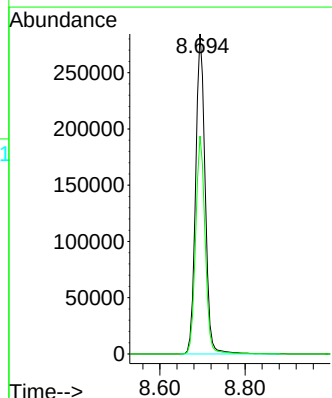
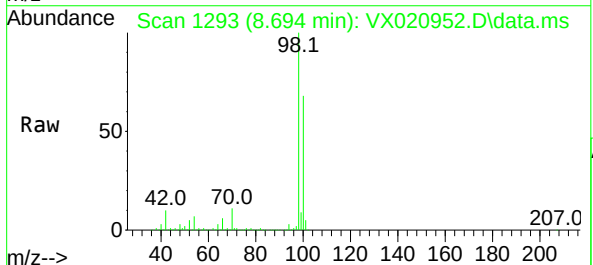




#51
4-Methyl-2-Pentanone
Concen: 0.31 ug/l
RT: 8.617 min Scan# 1280
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14




Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721


Tgt Ion: 43 Resp: 1005
Ion Ratio Lower Upper
43 100
58 11.5 35.4 53.0#



#62
4-Bromofluorobenzene
Concen: 51.30 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

Tgt Ion: 95 Resp: 163145
Ion Ratio Lower Upper
95 100
174 76.8 0.0 154.6
176 73.3 0.0 155.8


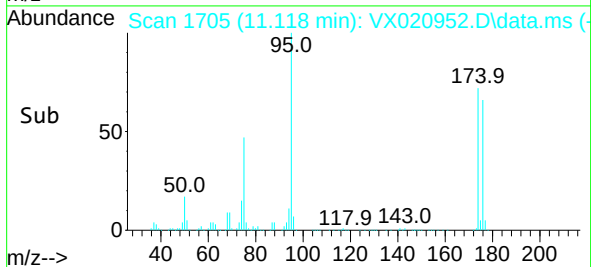

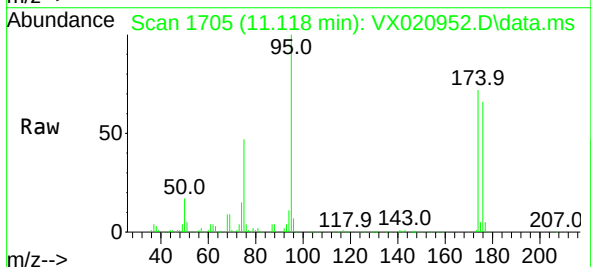




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. -0.000 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14




Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721


Tgt Ion:117 Resp: 343037
Ion Ratio Lower Upper
117 100
82 56.1 47.4 71.2
119 30.9 26.6 39.8

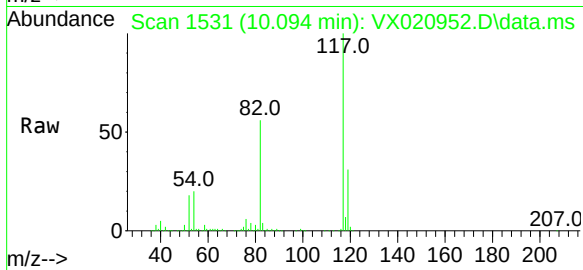

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. -0.006 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14


Tgt Ion:152 Resp: 144188
Ion Ratio Lower Upper
152 100
115 59.1 41.1 123.3
150 158.3 0.0 349.0

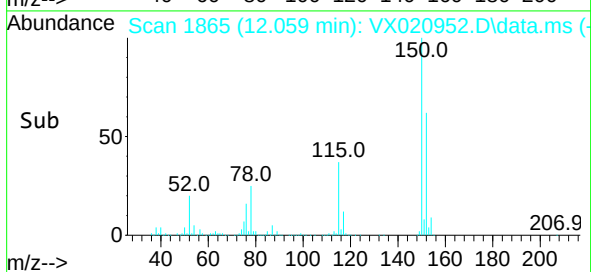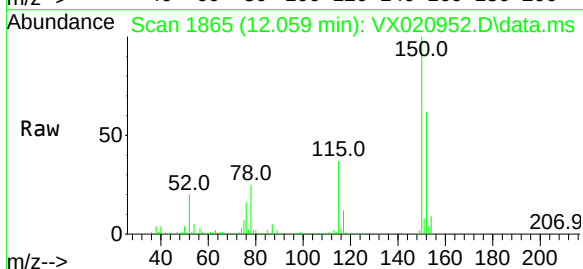






#74
N-amy1 acetate
Concen: 0.93 ug/l
RT: 10.894 min Scan# 1667
Delta R.T. 0.017 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14

Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721



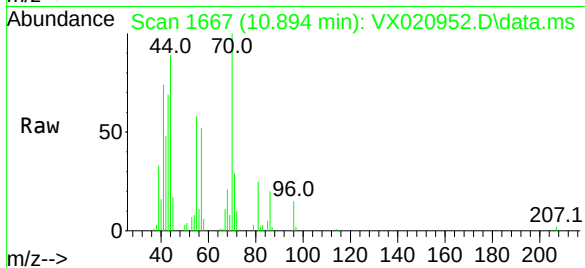



Tgt Ion:	43	Resp:	4279
Ion	Ratio	Lower	Upper
43	100		
70	129.0	39.0	58.6#
55	81.1	21.5	32.3#
61	0.0	22.1	33.1#

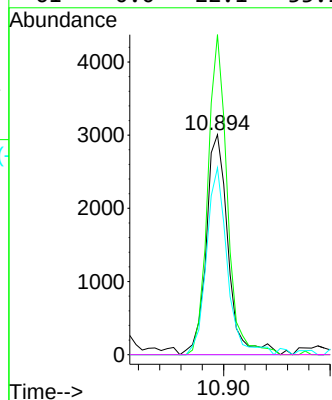

#76
1,2,3-Trichloropropane
Concen: 24.93 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.159 min
Lab File: VX020952.D
Acq: 01 Mar 2021 22:14


Tgt Ion:	75	Resp:	77331
Ion	Ratio	Lower	Upper
75	100		
77	1.3	19.1	57.5#

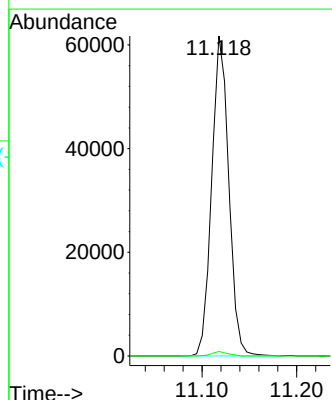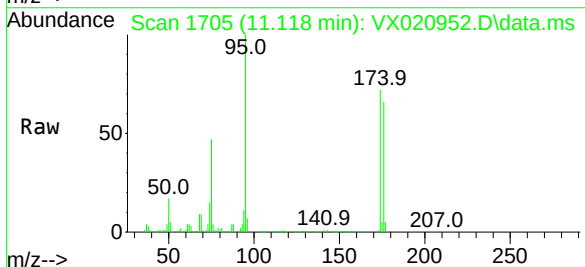

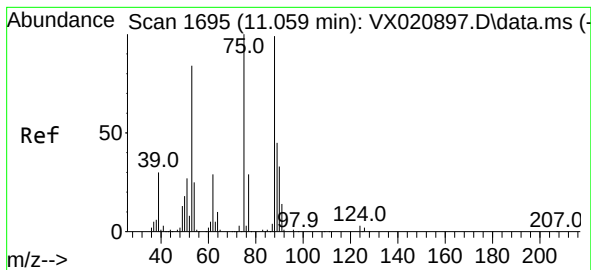

#81
 trans-1,4-Dichloro-2-butene
 Concen: 55.20 ug/l
 RT: 11.118 min Scan# 1705
 Delta R.T. 0.059 min
 Lab File: VX020952.D
 Acq: 01 Mar 2021 22:14

Instrument :
 MSVOA_X
 ClientSampleId :
 GW807-41-46-022721

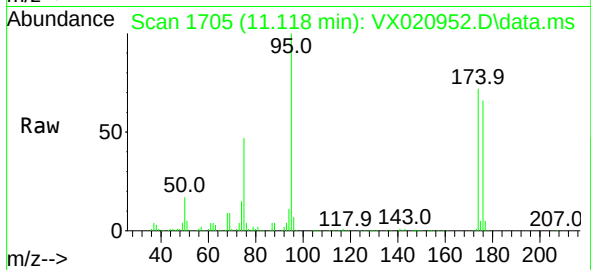

Tgt Ion: 75 Resp: 77331
 Ion Ratio Lower Upper
 75 100
 53 0.0 74.5 111.7#
 89 0.0 37.9 56.9#

