

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030221\
 Data File : VX020947.D
 Acq On : 01 Mar 2021 20:18
 Operator : JC/MD
 Sample : M1522-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-VPB-RW6-TB-20210224

Quant Time: Mar 02 00:32:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 24 13:50:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	204997	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	381355	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	365011	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.065	152	164101	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	133026	48.04	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	96.08%
35) Dibromofluoromethane	5.464	113	116220	50.16	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.32%
50) Toluene-d8	8.694	98	455749	50.45	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	100.90%
62) 4-Bromofluorobenzene	11.118	95	176661	52.88	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	105.76%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030221\
Data File : VX020947.D
Acq On : 01 Mar 2021 20:18
Operator : JC/MD
Sample : M1522-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-TB-20210224

Quant Time: Mar 02 00:32:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 24 13:50:55 2021
Response via : Initial Calibration




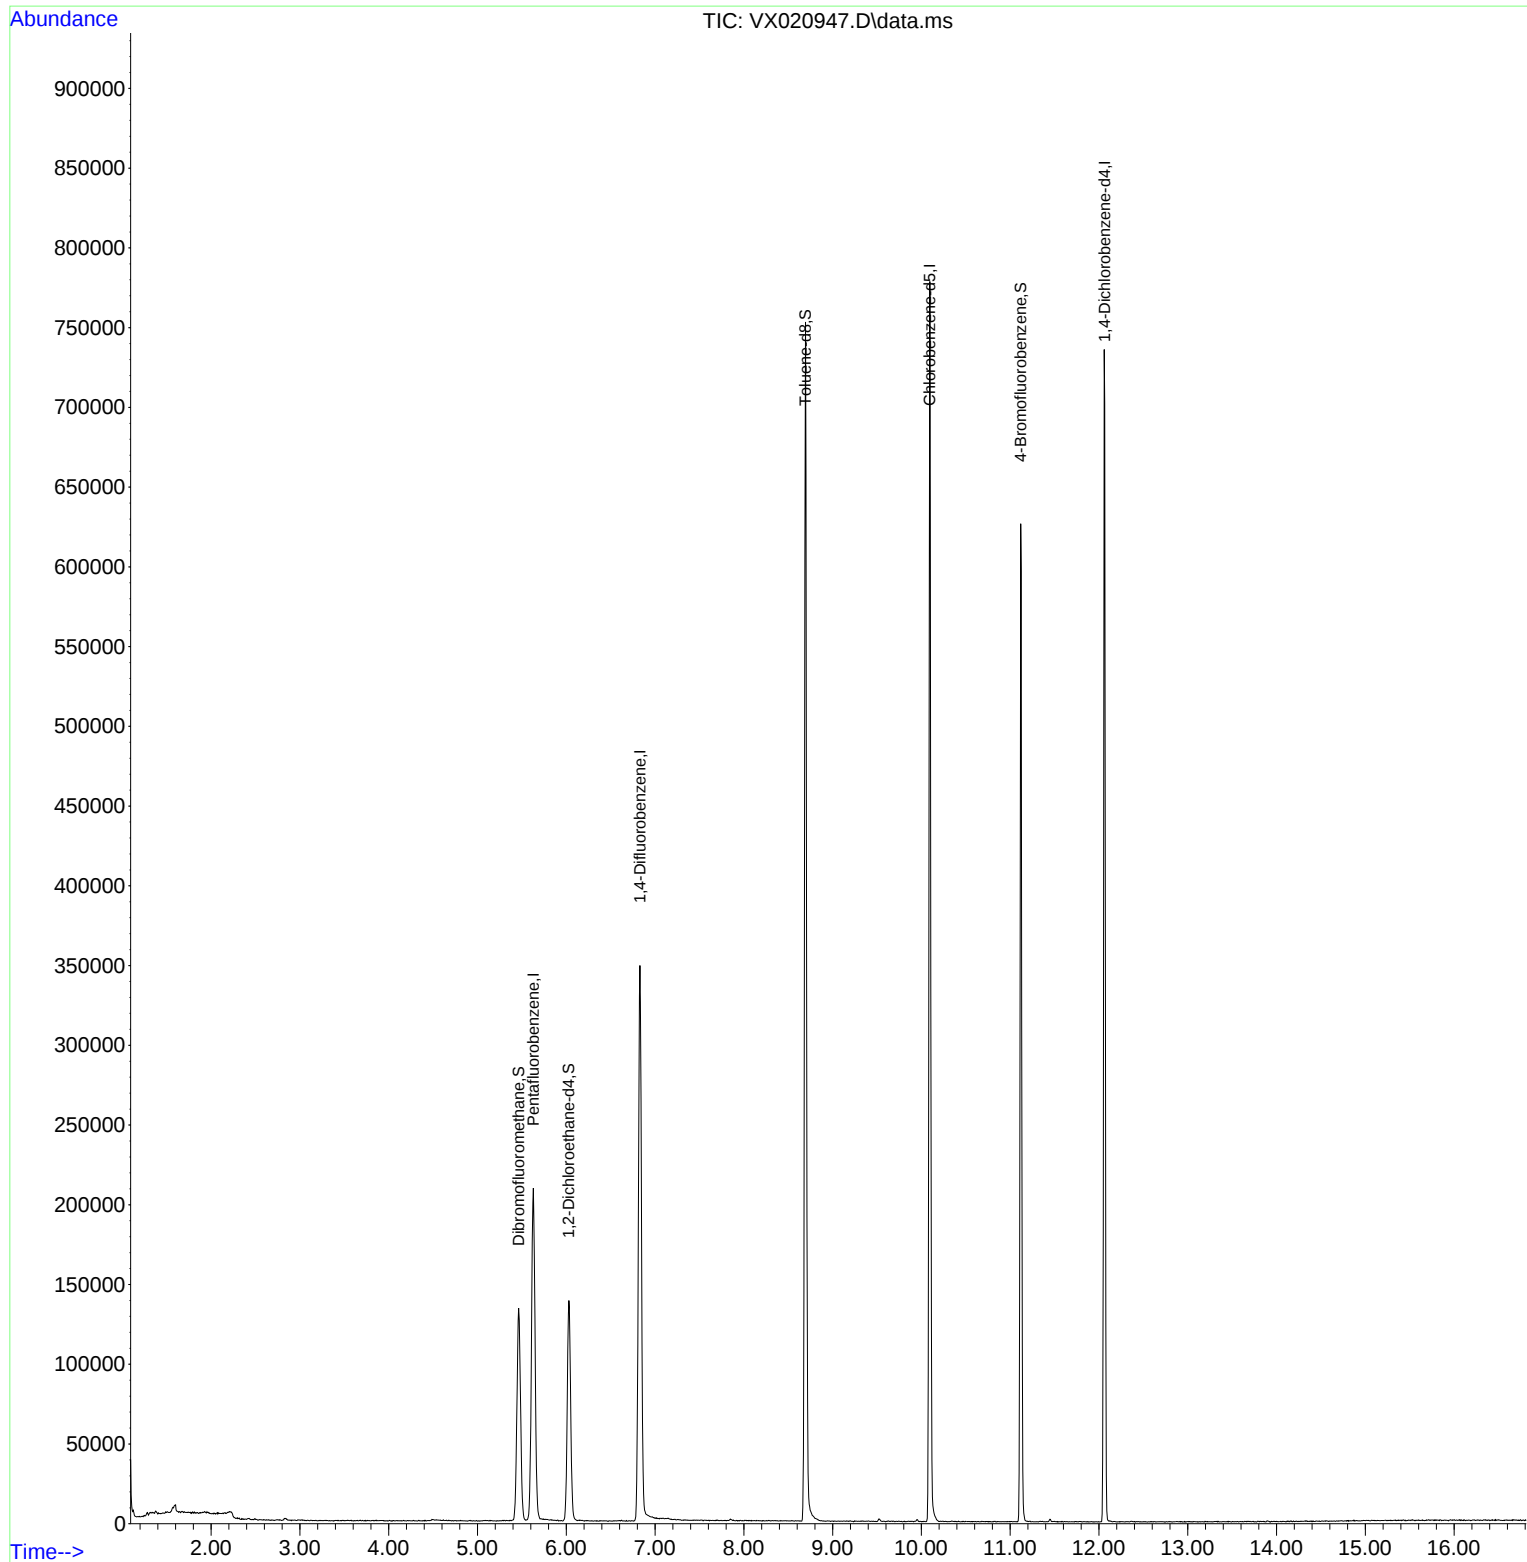




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 772
Delta R.T. 0.006 min
Lab File: VX020947.D
Acq: 01 Mar 2021 20:18




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-TB-20210224


Tgt Ion:168 Resp: 204997
Ion Ratio Lower Upper
168 100
99 53.7 45.8 68.6

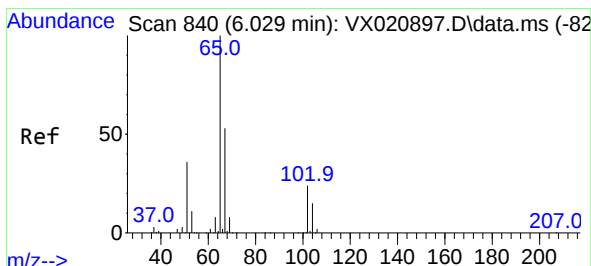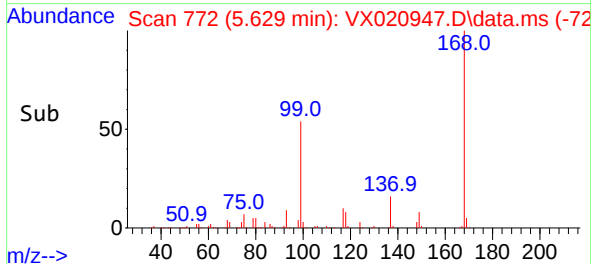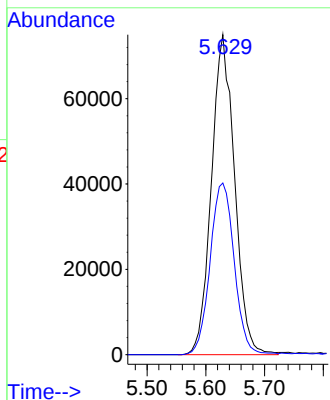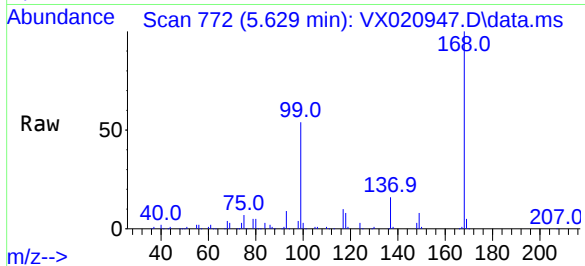

#33
1,2-Dichloroethane-d4
Concen: 48.04 ug/l
RT: 6.029 min Scan# 840
Delta R.T. -0.000 min
Lab File: VX020947.D
Acq: 01 Mar 2021 20:18


Tgt Ion: 65 Resp: 133026
Ion Ratio Lower Upper
65 100
67 52.3 0.0 105.4

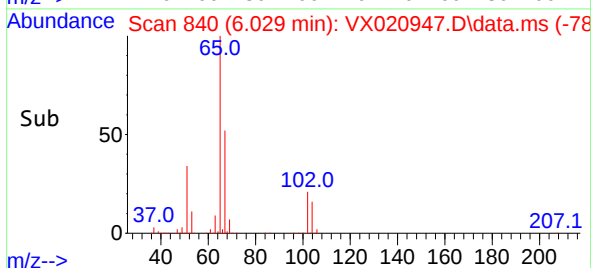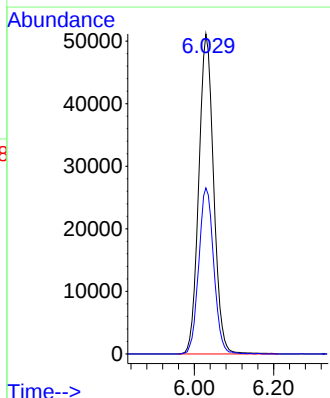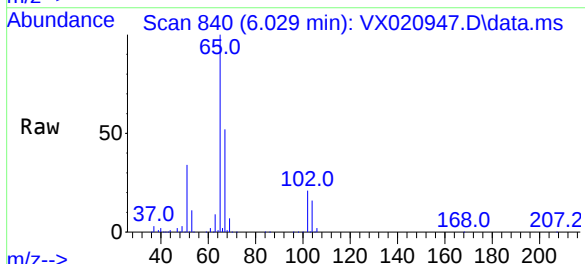



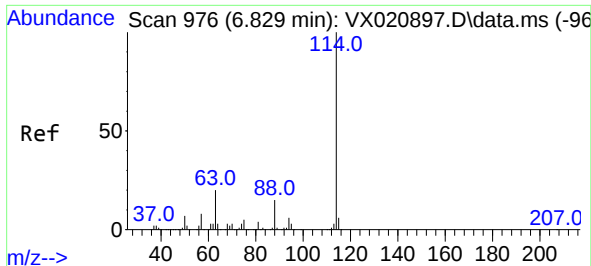


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.829 min Scan# 976
Delta R.T. -0.000 min
Lab File: VX020947.D
Acq: 01 Mar 2021 20:18


Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-TB-20210224

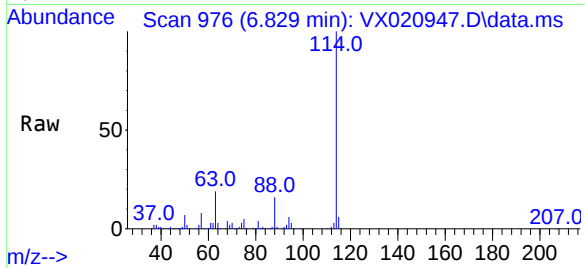



Tgt Ion:114 Resp: 381355
Ion Ratio Lower Upper
114 100
63 18.9 0.0 40.8
88 15.6 0.0 32.8

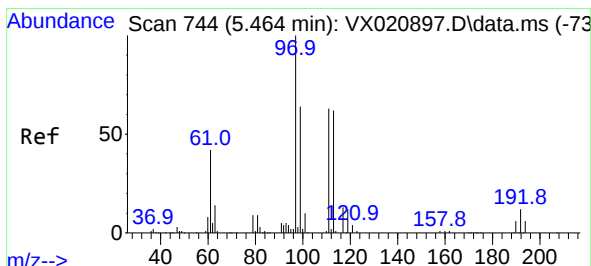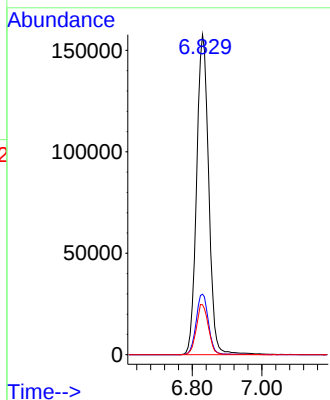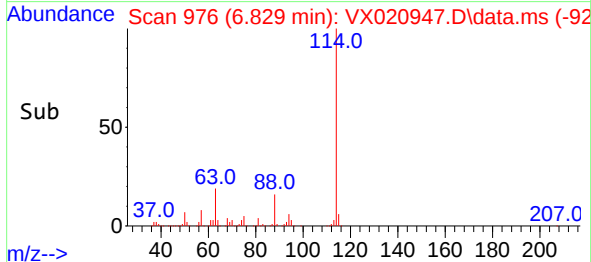


#35
Dibromofluoromethane
Concen: 50.16 ug/l
RT: 5.464 min Scan# 744
Delta R.T. -0.000 min
Lab File: VX020947.D
Acq: 01 Mar 2021 20:18

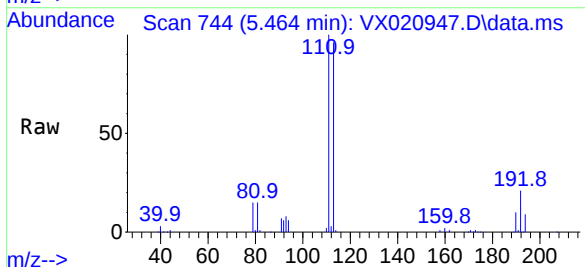

Tgt Ion:113 Resp: 116220
Ion Ratio Lower Upper
113 100
111 104.0 81.9 122.9
192 19.9 16.7 25.1



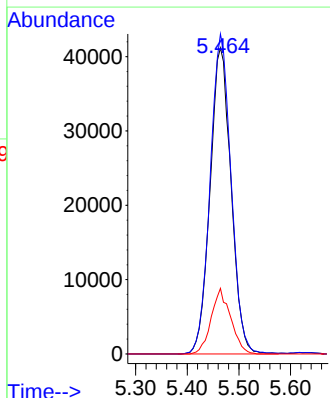
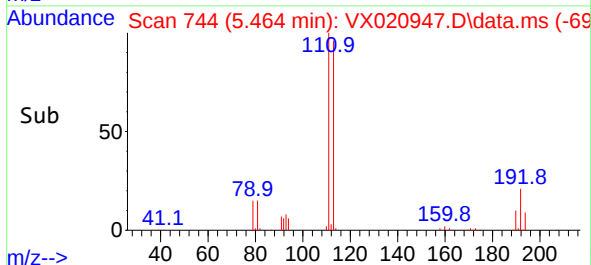


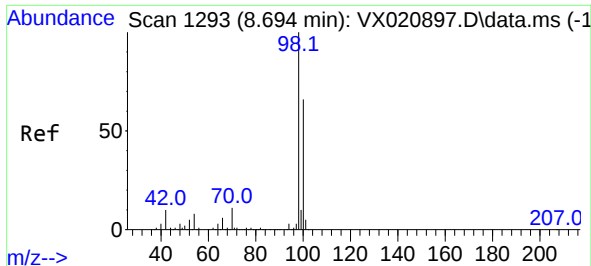

#50
Toluene-d8
Concen: 50.45 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. -0.000 min
Lab File: VX020947.D
Acq: 01 Mar 2021 20:18




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-TB-20210224


Tgt Ion: 98 Resp: 455749
Ion Ratio Lower Upper
98 100
100 67.9 51.9 77.9

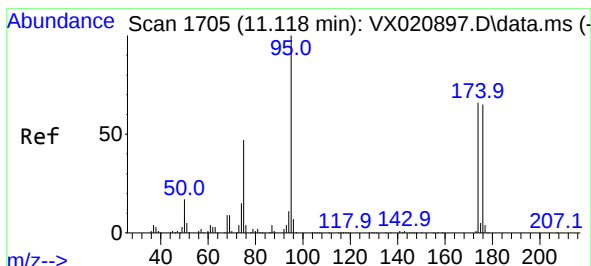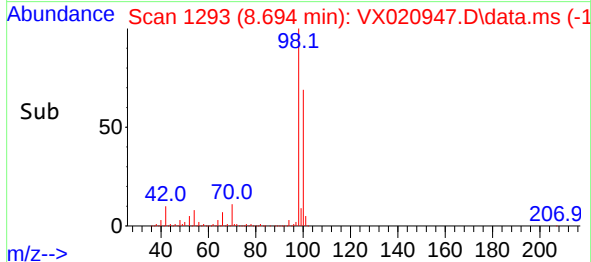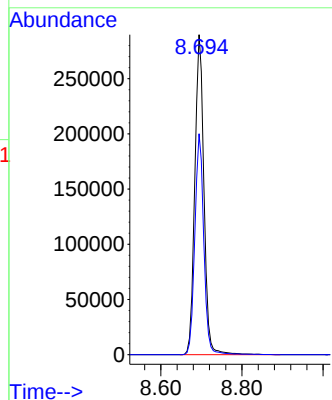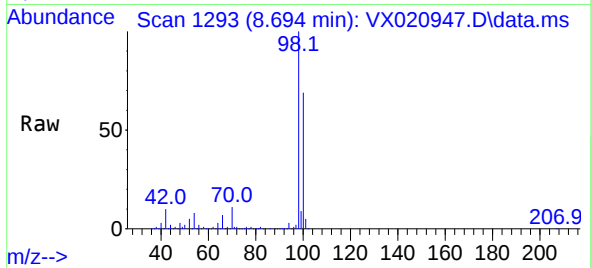

#62
4-Bromofluorobenzene
Concen: 52.88 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX020947.D
Acq: 01 Mar 2021 20:18

Tgt Ion: 95 Resp: 176661
Ion Ratio Lower Upper
95 100
174 75.6 0.0 154.6
176 74.6 0.0 155.8


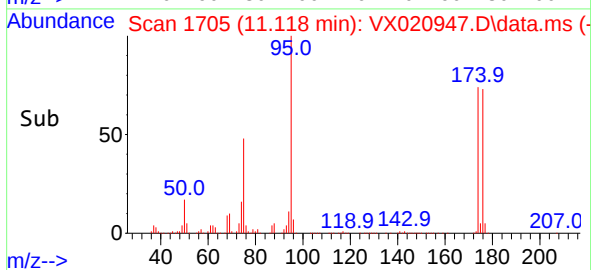
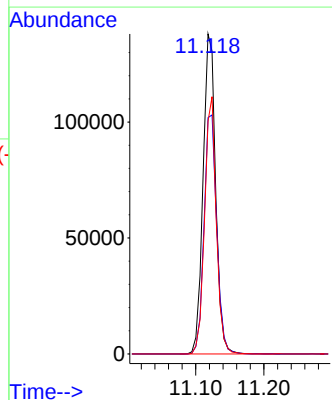
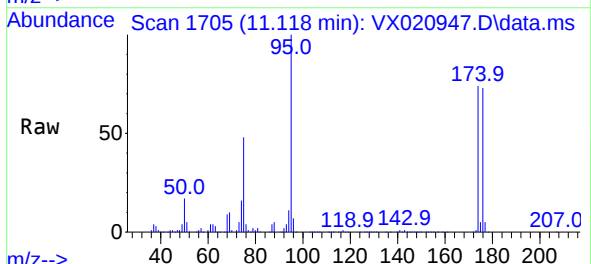


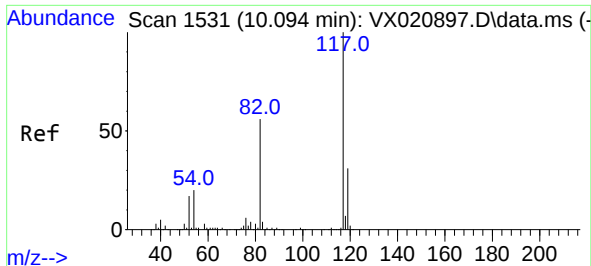

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. -0.000 min
Lab File: VX020947.D
Acq: 01 Mar 2021 20:18

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-TB-20210224

Tgt Ion:117 Resp: 365011
Ion Ratio Lower Upper
117 100
82 54.9 47.4 71.2
119 31.3 26.6 39.8

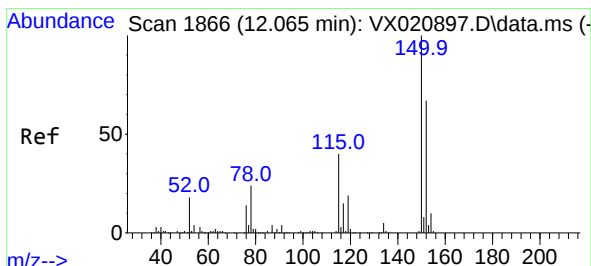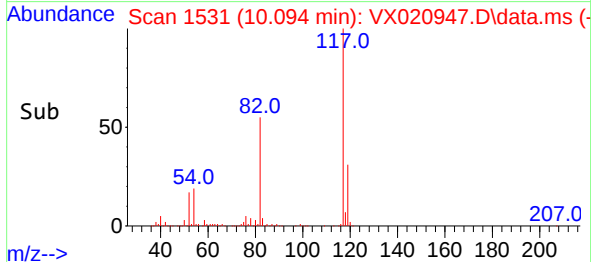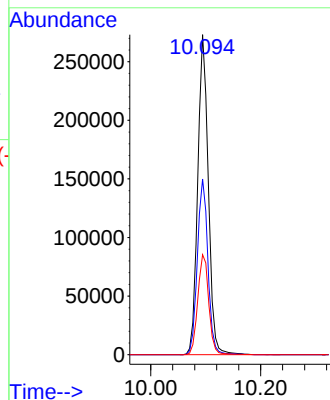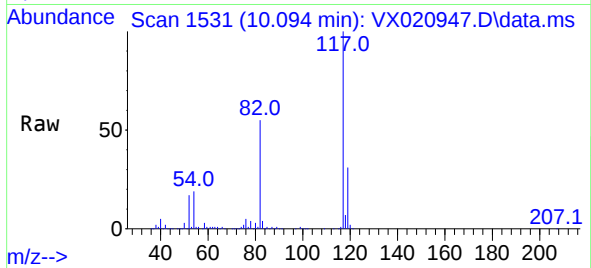

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.065 min Scan# 1866
Delta R.T. -0.000 min
Lab File: VX020947.D
Acq: 01 Mar 2021 20:18

Tgt Ion:152 Resp: 164101
Ion Ratio Lower Upper
152 100
115 59.3 41.1 123.3
150 150.2 0.0 349.0

