

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX030221\  
 Data File : VX020948.D  
 Acq On : 01 Mar 2021 20:42  
 Operator : JC/MD  
 Sample : M1535-06  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 TB-01-030121

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022421W.M

Title : SW846 8260

Signal : TIC: VX020948.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.617       | 81            | 90          | 97           | rBV6     | 3602           | 11106         | 1.00%           | 0.197%        |
| 2         | 5.464       | 731           | 744         | 760          | rBV      | 128527         | 364666        | 32.95%          | 6.476%        |
| 3         | 5.629       | 760           | 772         | 787          | rBV      | 196331         | 556081        | 50.25%          | 9.875%        |
| 4         | 6.029       | 828           | 840         | 854          | rBV      | 132775         | 348650        | 31.50%          | 6.191%        |
| 5         | 6.829       | 966           | 976         | 990          | rBV      | 343013         | 798532        | 72.15%          | 14.180%       |
| 6         | 8.694       | 1286          | 1293        | 1320         | rBV      | 701401         | 1106719       | 100.00%         | 19.653%       |
| 7         | 10.094      | 1525          | 1531        | 1547         | rBV      | 719254         | 957785        | 86.54%          | 17.008%       |
| 8         | 11.118      | 1699          | 1705        | 1715         | rBV      | 534474         | 687703        | 62.14%          | 12.212%       |
| 9         | 12.059      | 1860          | 1865        | 1875         | rVB      | 639123         | 800022        | 72.29%          | 14.207%       |




Sum of corrected areas: 5631264

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX030221\  
Data File : VX020948.D  
Acq On : 01 Mar 2021 20:42  
Operator : JC/MD  
Sample : M1535-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-01-030121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022421W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

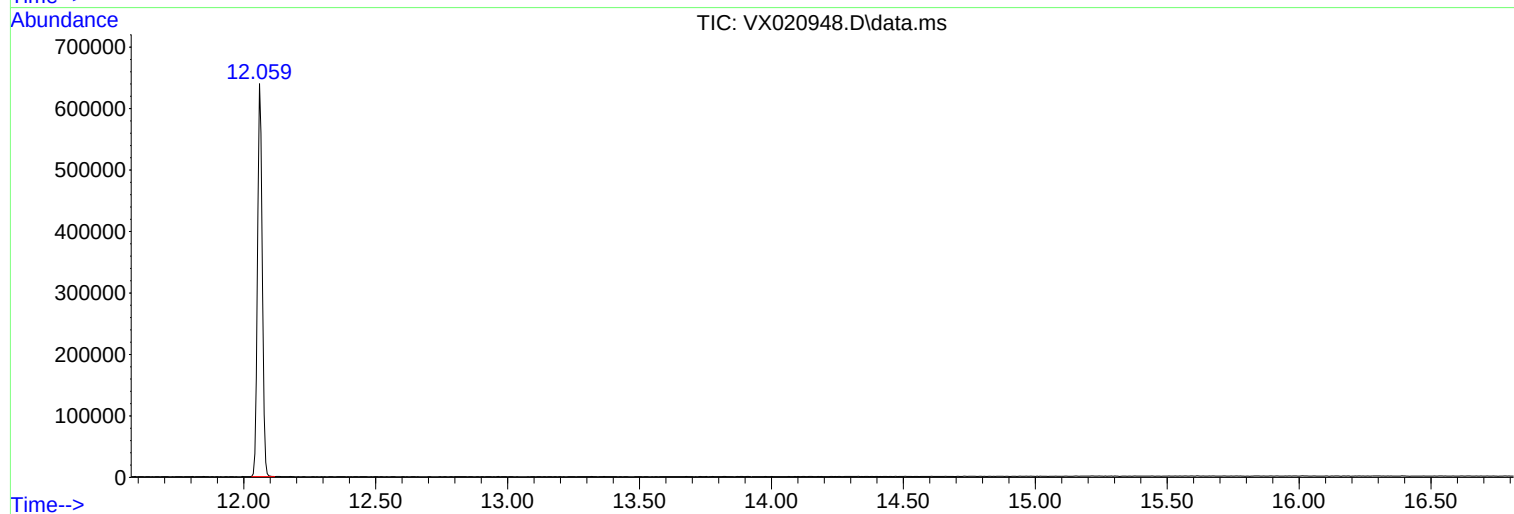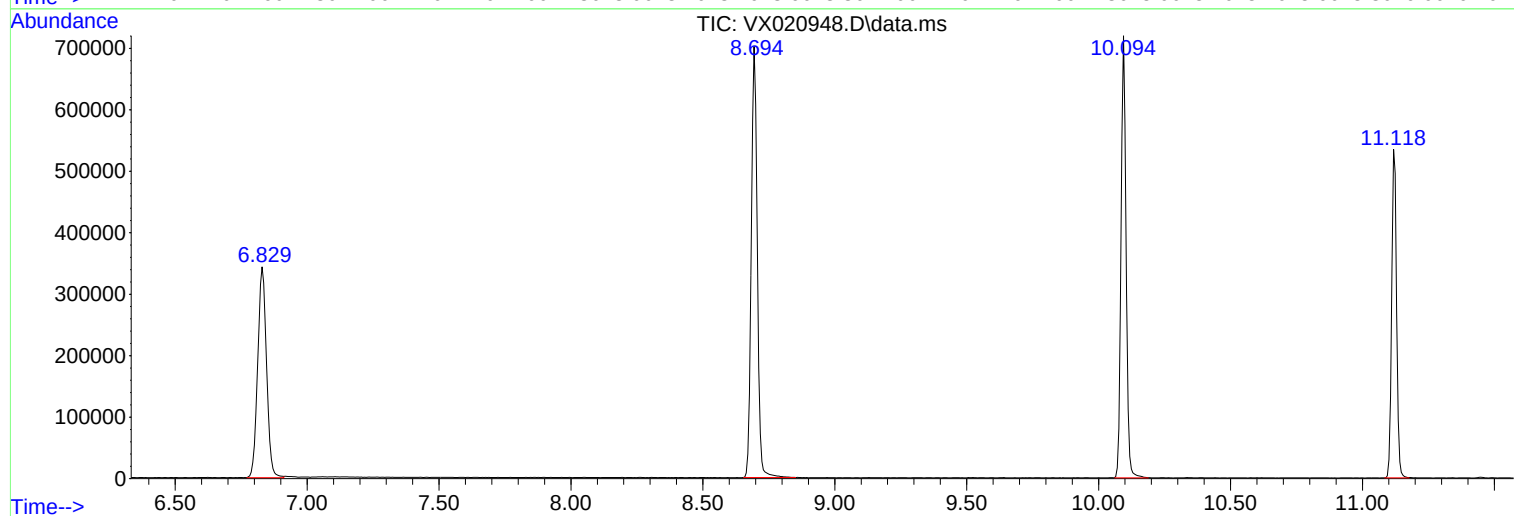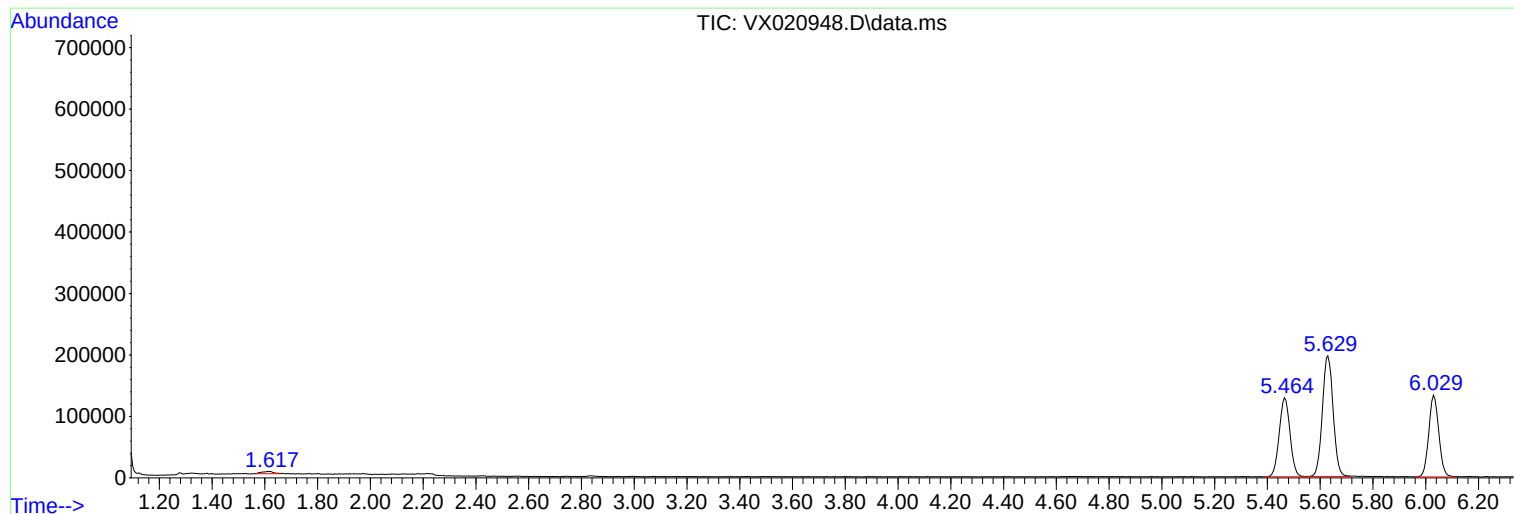

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX030221\  
Data File : VX020948.D  
Acq On : 01 Mar 2021 20:42  
Operator : JC/MD  
Sample : M1535-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-01-030121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022421W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX030221\  
Data File : VX020948.D  
Acq On : 01 Mar 2021 20:42  
Operator : JC/MD  
Sample : M1535-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB-01-030121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X022421W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----