

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030221\
 Data File : VX020952.D
 Acq On : 01 Mar 2021 22:14
 Operator : JC/MD
 Sample : M1535-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW807-41-46-022721

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M

Title : SW846 8260

Signal : TIC: VX020952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.164	9	13	19	rVB2	34264	36029	3.22%	0.446%
2	1.381	46	50	57	rBV2	9240	13915	1.24%	0.172%
3	2.358	208	216	225	rBV	507583	793608	70.89%	9.824%
4	2.593	251	256	268	rVB2	6746	17008	1.52%	0.211%
5	3.146	342	350	361	rBV	35279	68624	6.13%	0.849%
6	3.670	425	439	458	rBV	29966	77203	6.90%	0.956%
7	4.564	579	591	603	rBV	246536	671341	59.97%	8.311%
8	5.176	686	695	707	rVB3	15766	46020	4.11%	0.570%
9	5.464	732	744	759	rBV	126215	361469	32.29%	4.475%
10	5.623	761	771	785	rBV2	194433	558739	49.91%	6.917%
11	6.029	829	840	850	rBV	132463	352646	31.50%	4.365%
12	6.164	850	863	872	rVB2	21395	65882	5.89%	0.816%
13	6.829	965	976	998	rBV	334646	802436	71.68%	9.933%
14	7.188	1028	1037	1051	rBV	209397	455534	40.69%	5.639%
15	7.723	1121	1128	1137	rBV3	6297	13867	1.24%	0.172%
16	8.694	1286	1293	1302	rBV	726030	1119436	100.00%	13.858%
17	10.094	1525	1531	1549	rVB	734683	990281	88.46%	12.259%
18	10.894	1662	1667	1677	rBV	32105	41553	3.71%	0.514%
19	11.118	1699	1705	1719	rBV	575047	738609	65.98%	9.143%
20	12.059	1859	1865	1872	rBV	693651	853975	76.29%	10.571%




Sum of corrected areas: 8078175

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030221\
Data File : VX020952.D
Acq On : 01 Mar 2021 22:14
Operator : JC/MD
Sample : M1535-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

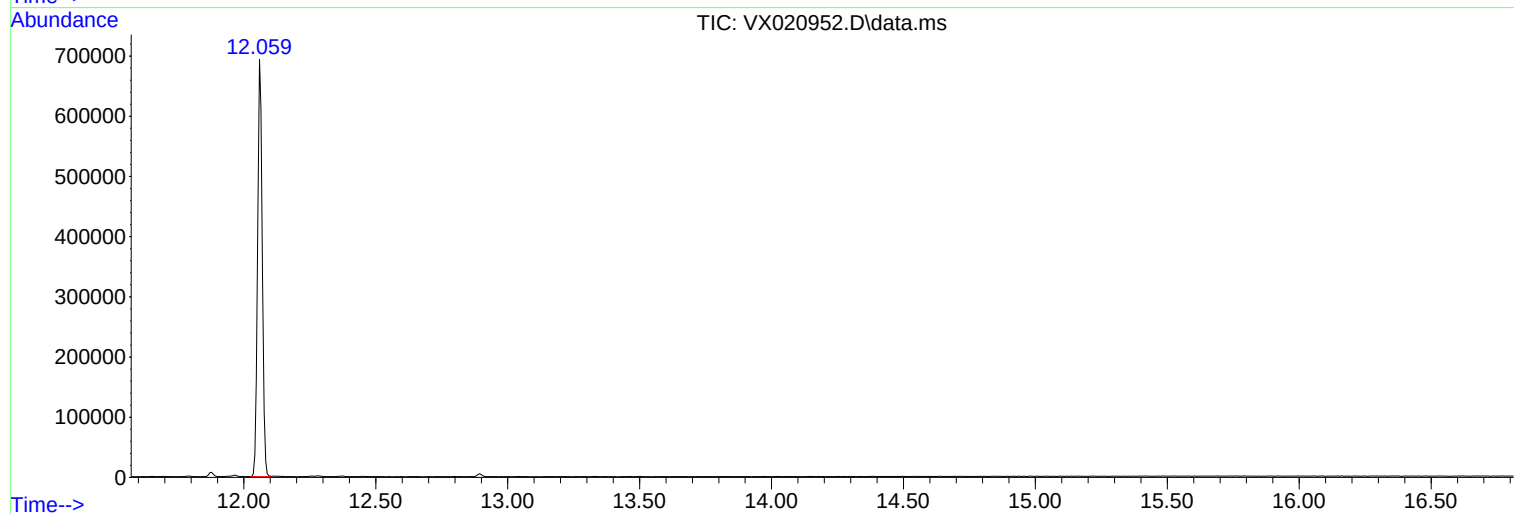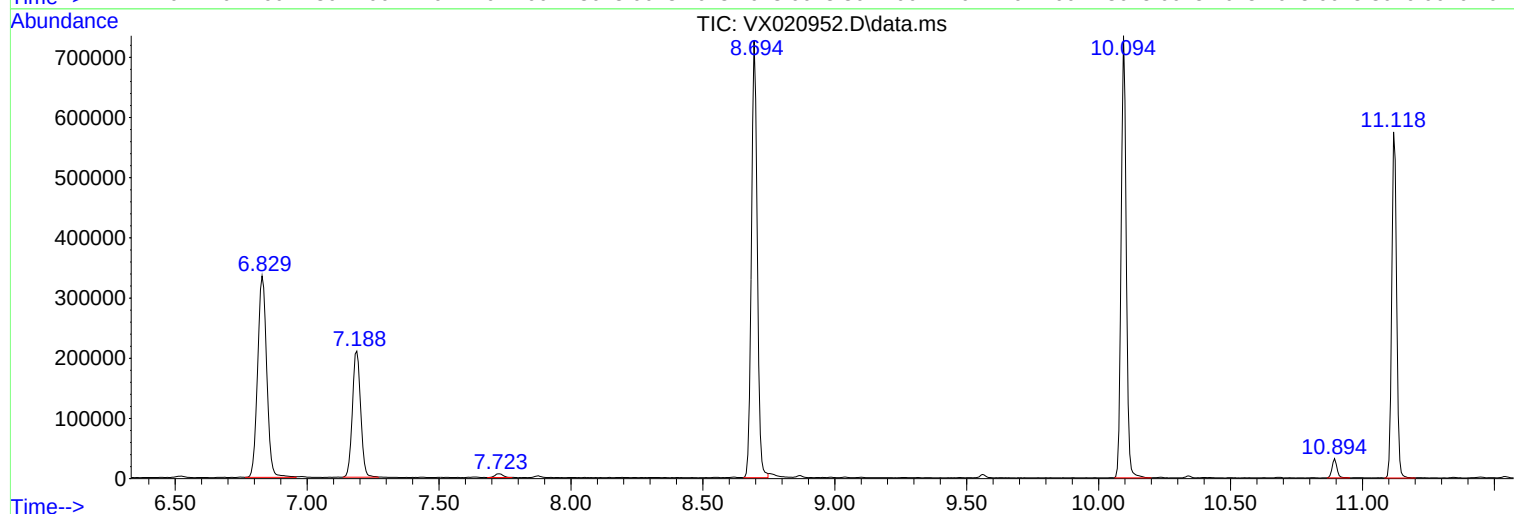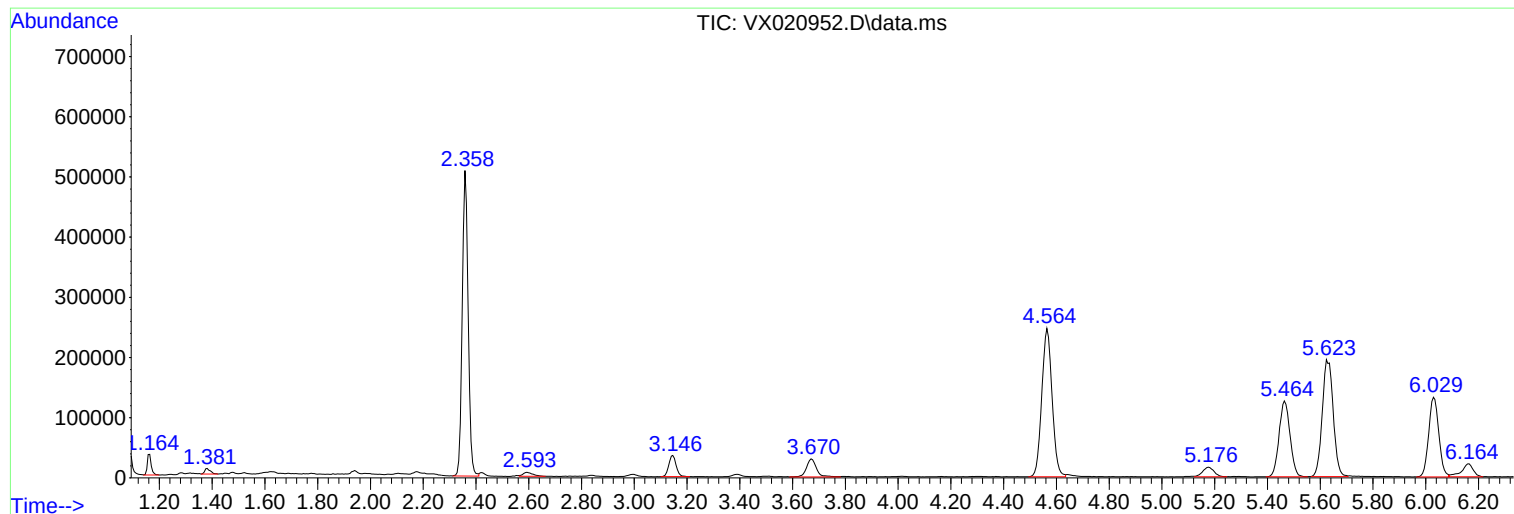

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030221\
Data File : VX020952.D
Acq On : 01 Mar 2021 22:14
Operator : JC/MD
Sample : M1535-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030221\
Data File : VX020952.D
Acq On : 01 Mar 2021 22:14
Operator : JC/MD
Sample : M1535-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW807-41-46-022721

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
