
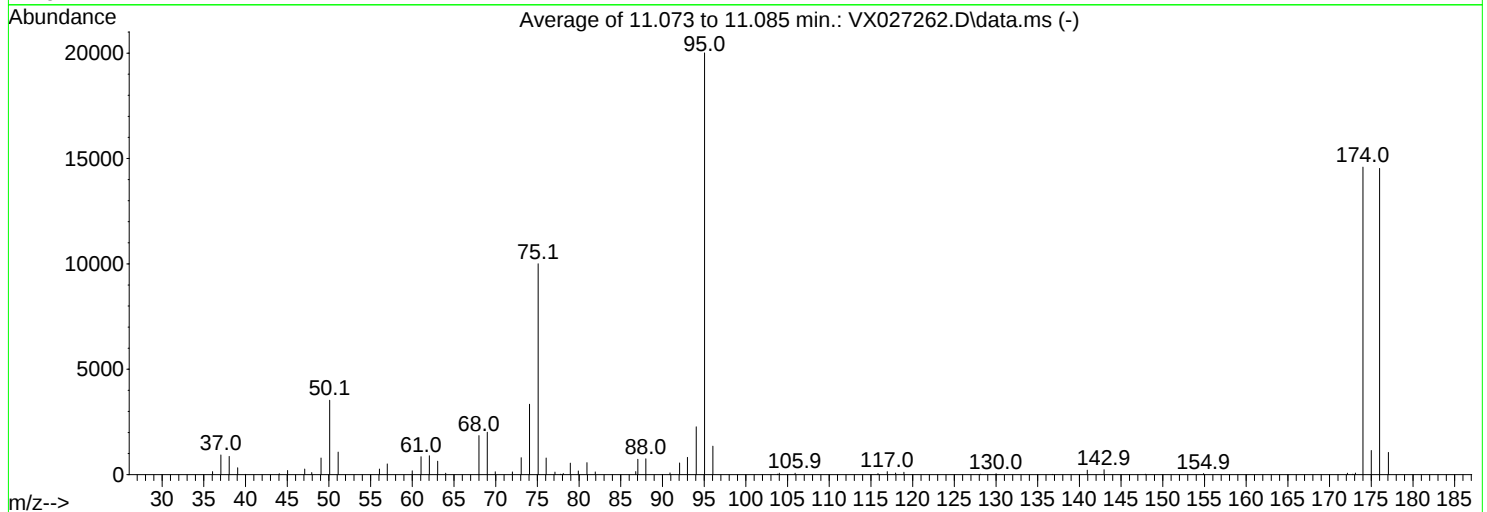


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030222\
 Data File : VX027262.D
 Acq On : 02 Mar 2022 11:10
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
 Title : SW846 8260
 Last Update : Wed Feb 23 13:06:57 2022

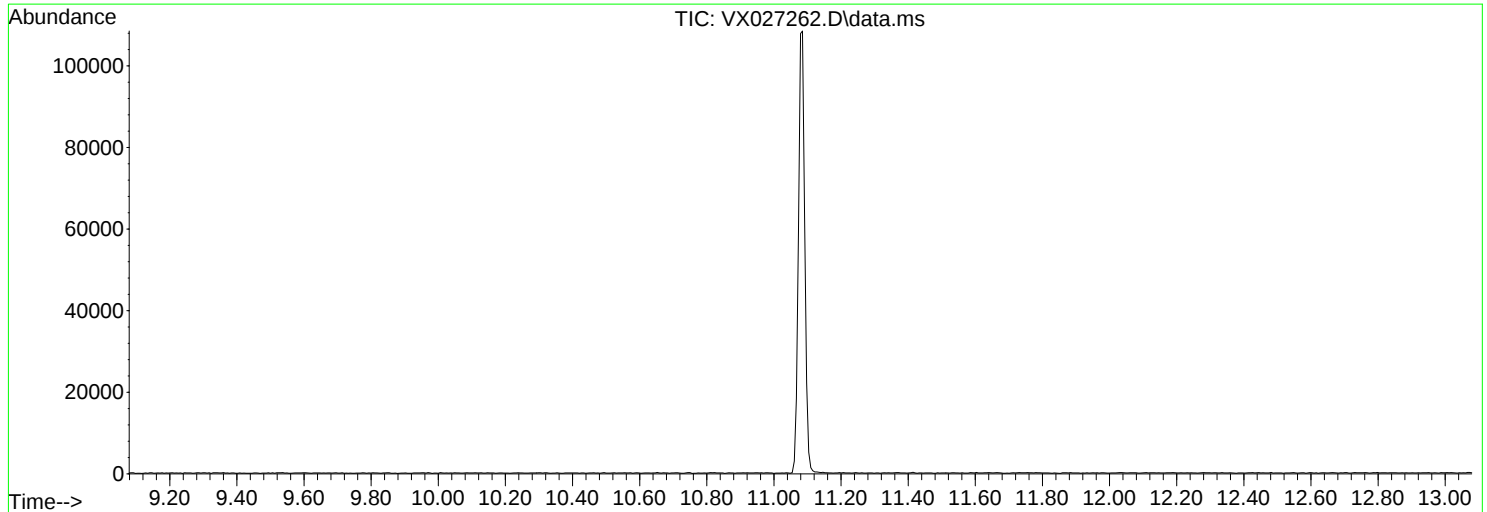

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	3528	PASS
75	95	30	60	50.0	10004	PASS
95	95	100	100	100.0	20013	PASS
96	95	5	9	6.8	1353	PASS
173	174	0.00	2	0.5	73	PASS
174	95	50	100	72.9	14588	PASS
175	174	5	9	7.9	1150	PASS
176	174	95	101	99.6	14528	PASS
177	176	5	9	7.3	1054	PASS