

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030223\
 Data File : VX034303.D
 Acq On : 02 Mar 2023 12:46
 Operator : JC/MD
 Sample : 01759-01 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DEP-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
 Title : SW846 8260

Signal : TIC: VX034303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	720	rBV	147300	433476	32.89%	6.220%
2	5.550	722	732	748	rVB	255818	723860	54.93%	10.387%
3	5.958	789	799	816	rBV	160683	435254	33.03%	6.246%
4	6.763	921	931	949	rBV	398622	949203	72.03%	13.621%
5	8.647	1231	1240	1258	rBV	841045	1317854	100.00%	18.911%
6	10.055	1465	1471	1487	rBV	795492	1073063	81.43%	15.398%
7	11.079	1634	1639	1651	rBV	592467	782847	59.40%	11.233%
8	12.024	1789	1794	1805	rVB	687133	883357	67.03%	12.676%
9	12.317	1838	1842	1849	rVV7	6116	13961	1.06%	0.200%
10	12.817	1919	1924	1927	rBV3	12189	21052	1.60%	0.302%
11	12.920	1931	1941	1946	rBV2	25201	47842	3.63%	0.687%
12	12.981	1946	1951	1955	rVV5	10213	16975	1.29%	0.244%
13	13.097	1965	1970	1974	rBV4	9895	17480	1.33%	0.251%
14	13.292	1999	2002	2008	rVB6	8447	14106	1.07%	0.202%
15	13.420	2017	2023	2032	rVB6	8228	28487	2.16%	0.409%
16	13.579	2046	2049	2053	rBV2	19081	26663	2.02%	0.383%
17	13.853	2089	2094	2098	rBV3	16765	26407	2.00%	0.379%
18	13.926	2098	2106	2111	rBV7	15327	28939	2.20%	0.415%
19	13.981	2111	2115	2124	rVB7	6964	18408	1.40%	0.264%
20	14.371	2175	2179	2184	rVB3	10038	13509	1.03%	0.194%
21	14.481	2193	2197	2202	rBV2	12713	20651	1.57%	0.296%
22	14.615	2215	2219	2225	rBV5	12370	21233	1.61%	0.305%
23	14.670	2225	2228	2232	rVB4	13527	18155	1.38%	0.261%
24	14.786	2243	2247	2251	rBV4	14603	22589	1.71%	0.324%
25	15.182	2307	2312	2315	rBV2	8190	13516	1.03%	0.194%


Sum of corrected areas: 6968887

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030223\
Data File : VX034303.D
Acq On : 02 Mar 2023 12:46
Operator : JC/MD
Sample : 01759-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DEP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

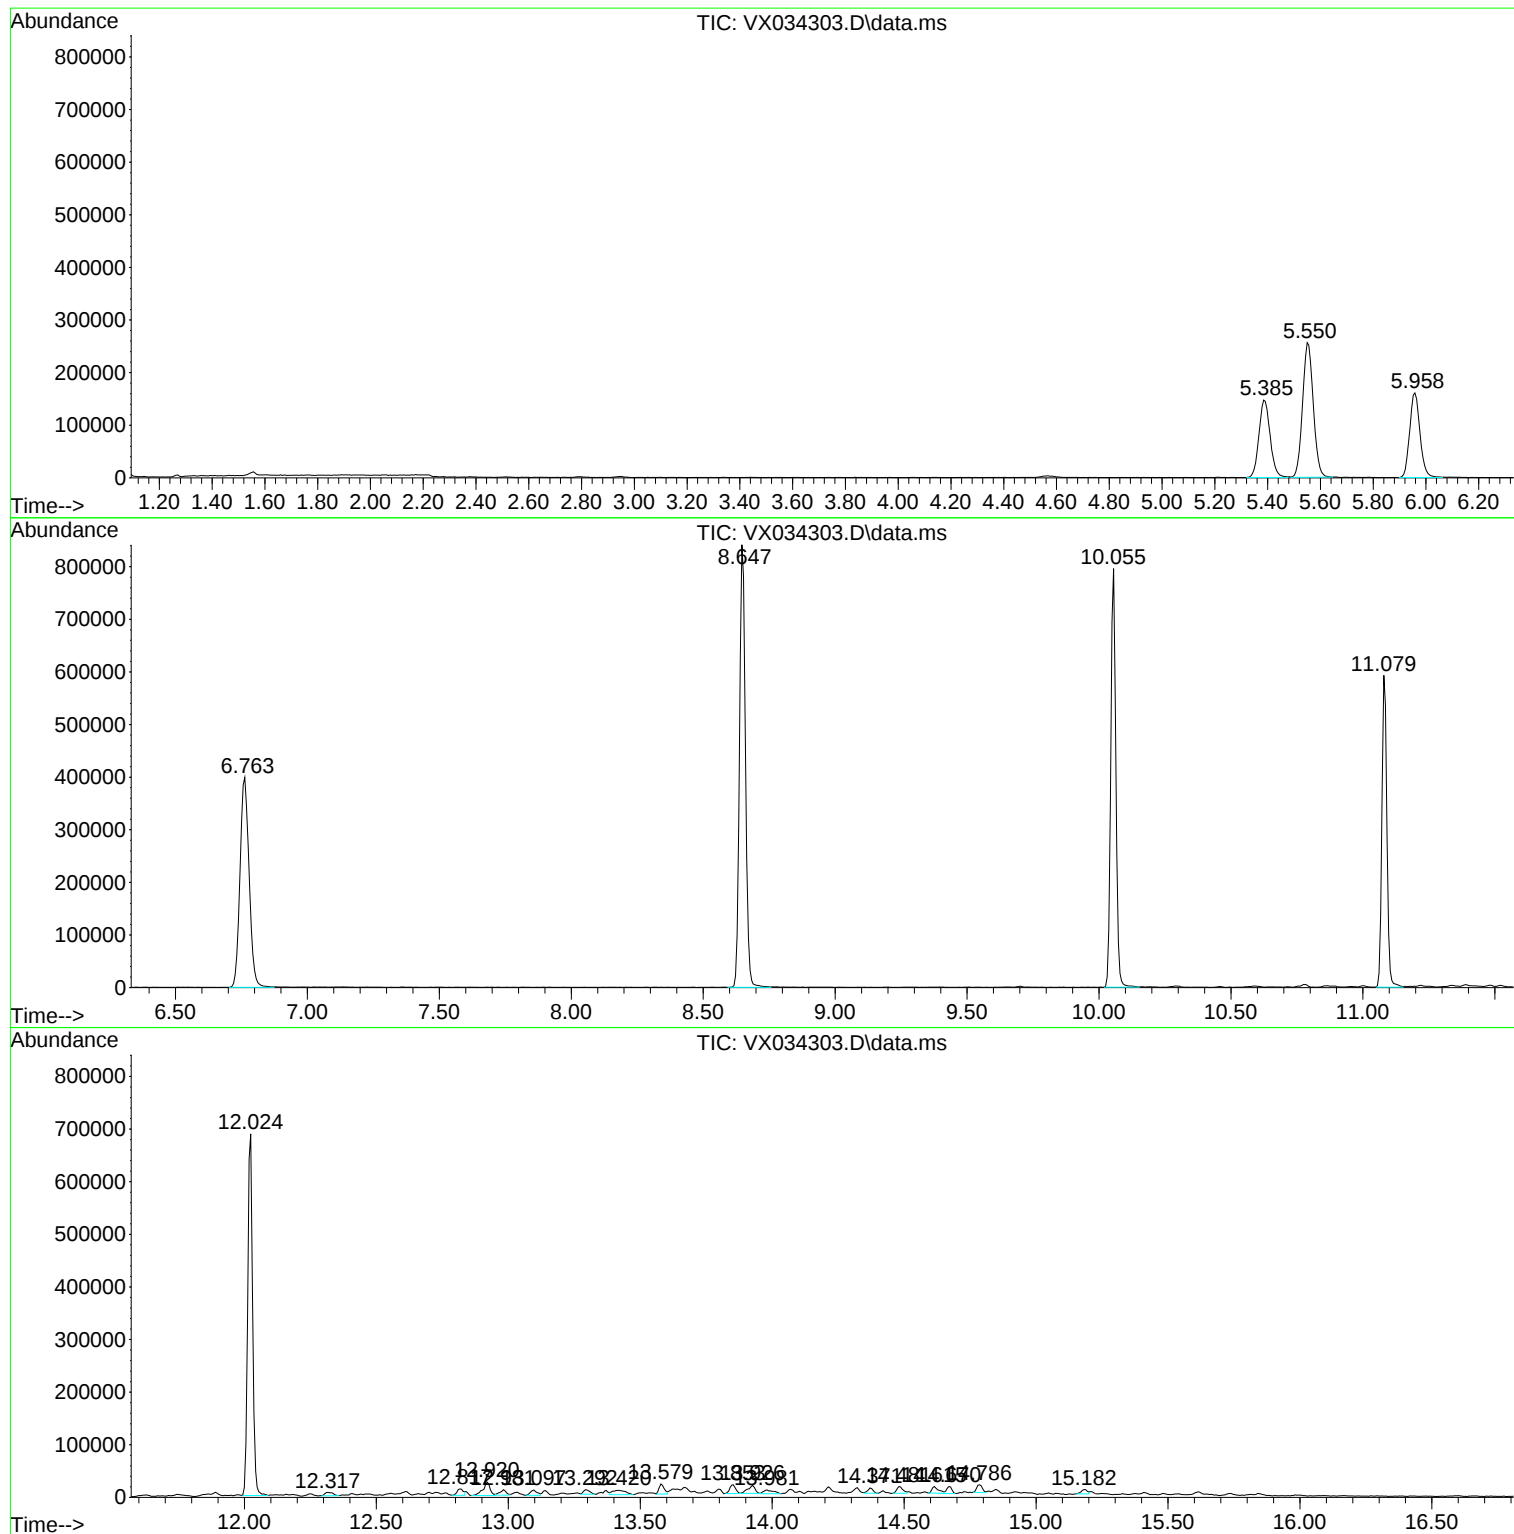

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030223\
Data File : VX034303.D
Acq On : 02 Mar 2023 12:46
Operator : JC/MD
Sample : 01759-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DEP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030223\
Data File : VX034303.D
Acq On : 02 Mar 2023 12:46
Operator : JC/MD
Sample : 01759-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DEP-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------