
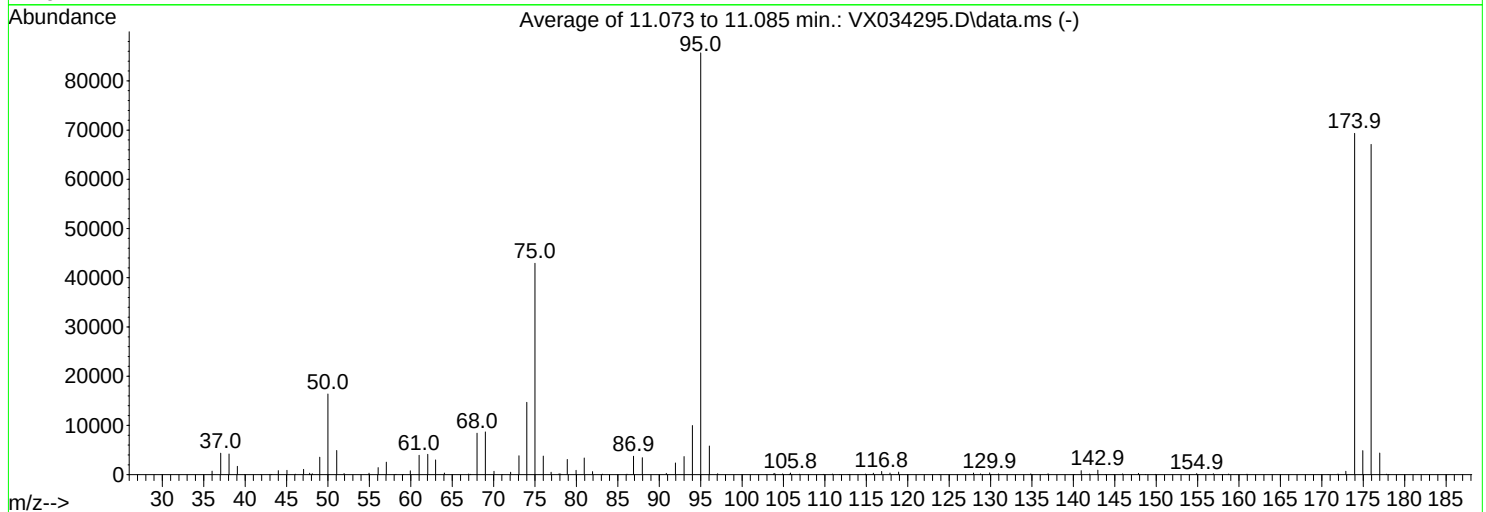


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030223\
Data File : VX034295.D
Acq On : 02 Mar 2023 08:39
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Title : SW846 8260
Last Update : Fri Feb 17 12:33:35 2023

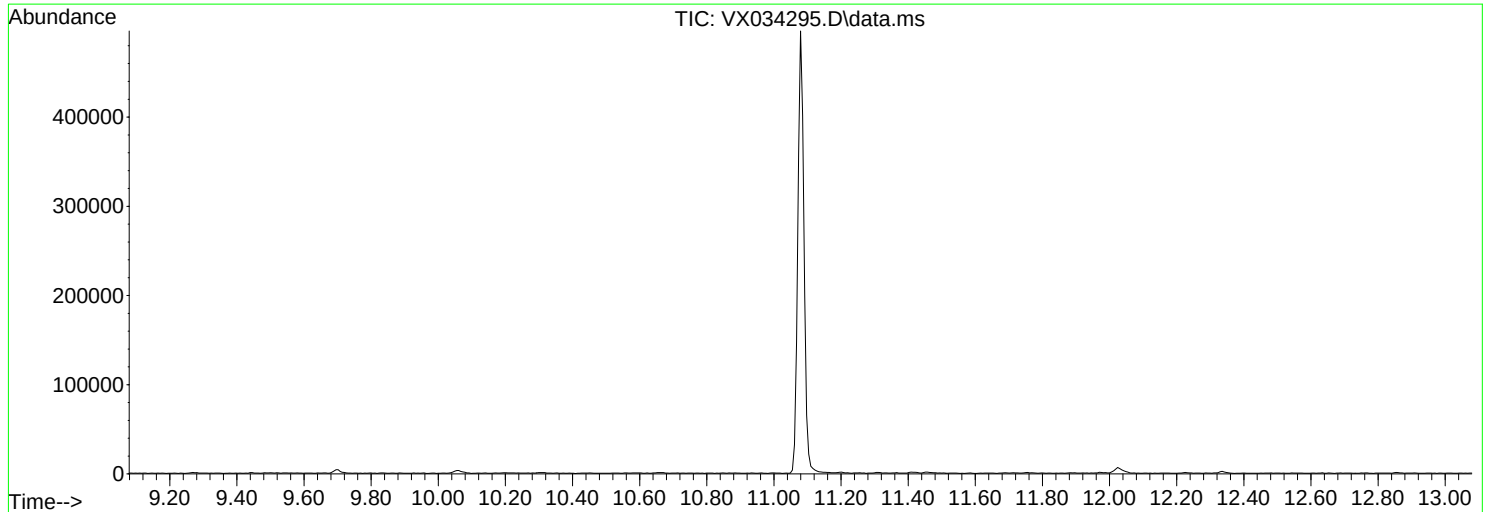

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	16373	PASS
75	95	30	60	50.1	42957	PASS
95	95	100	100	100.0	85691	PASS
96	95	5	9	6.8	5824	PASS
173	174	0.00	2	1.0	674	PASS
174	95	50	100	80.9	69355	PASS
175	174	5	9	7.1	4890	PASS
176	174	95	101	96.7	67096	PASS
177	176	5	9	6.5	4391	PASS