
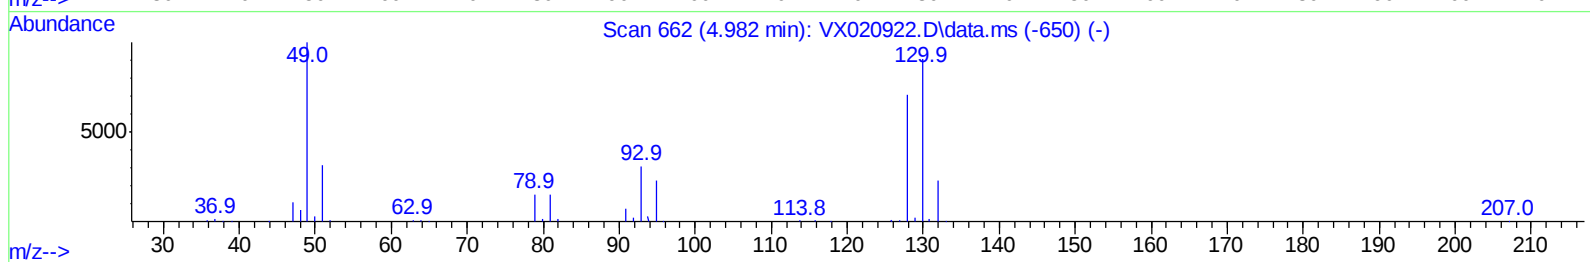
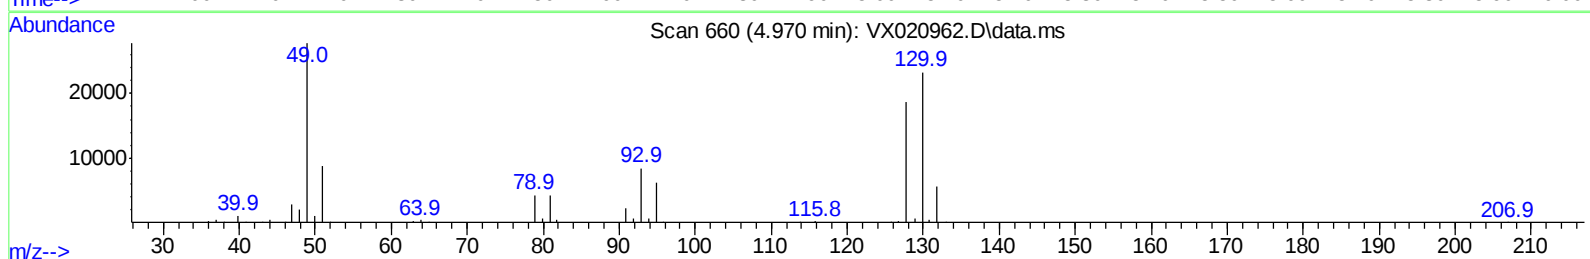


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
 Data File : VX020962.D
 Acq On : 02 Mar 2021 10:16
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 03 01:00:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 26 12:33:14 2021
 Response via : Initial Calibration

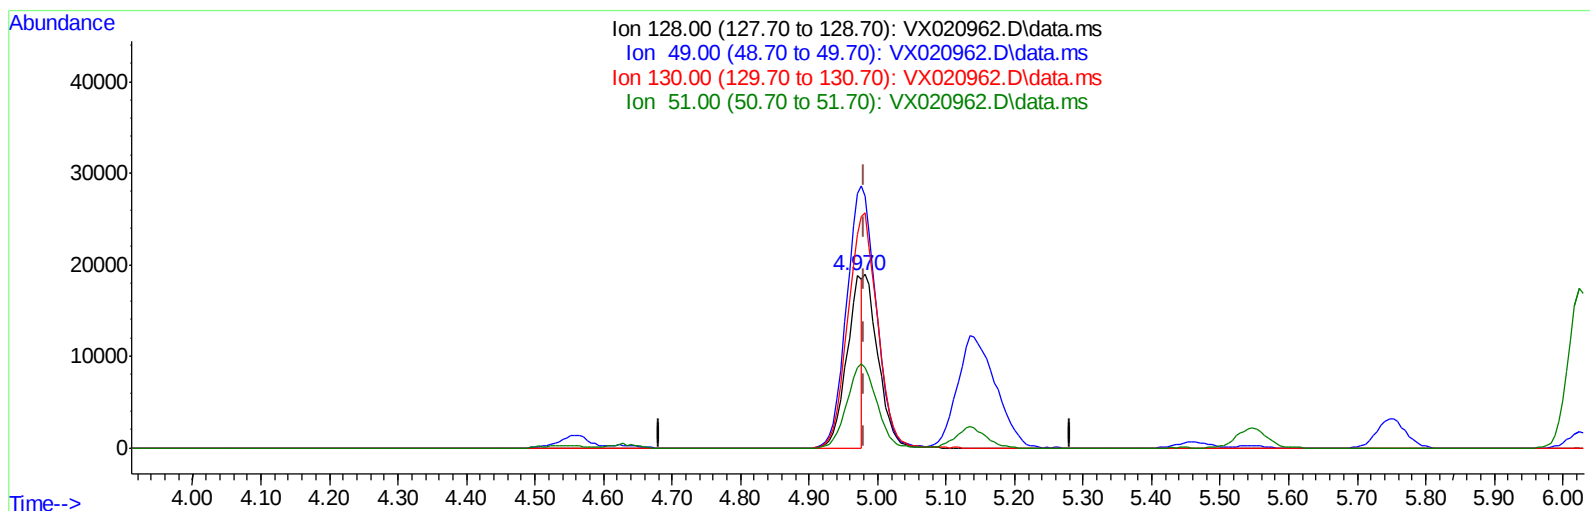

TIC: VX020962.D\data.ms

(23) Bromochloromethane (T)

4.970min (-0.011) 25.47 ug/L

response 30018

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	153.60	148.06
130.00	130.20	124.07
51.00	50.40	46.83