
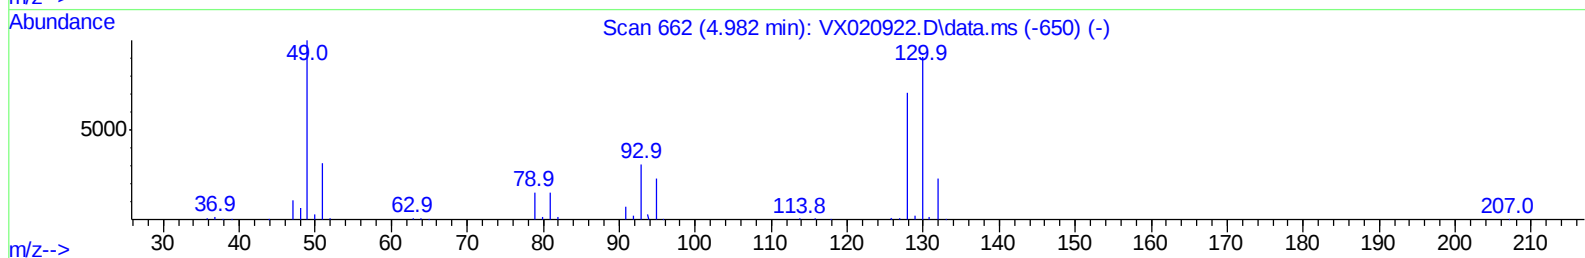
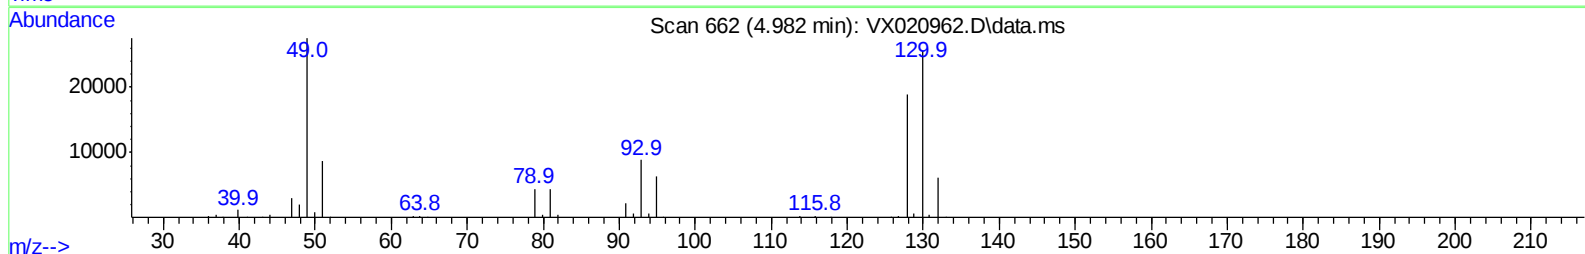


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
Data File : VX020962.D
Acq On : 02 Mar 2021 10:16
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 03 01:00:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 26 12:33:14 2021
Response via : Initial Calibration

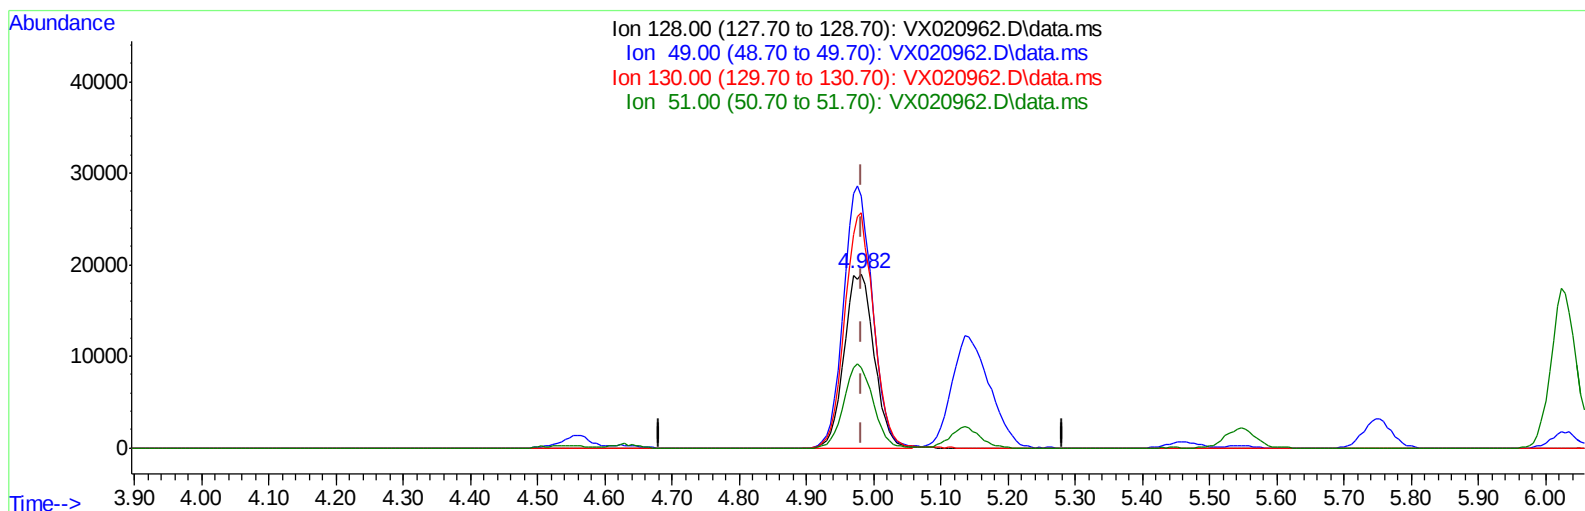

TIC: VX020962.D\data.ms

(23) Bromochloromethane (T)

4.982min (+ 0.000) 49.41 ug/L m

response 58236

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	153.60	144.95
130.00	130.20	134.89
51.00	50.40	45.81