

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
 Data File : VX020963.D
 Acq On : 02 Mar 2021 10:50
 Operator : JC/MD
 Sample : VX0303MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK107

Quant Time: Mar 03 01:05:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 03 01:05:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.823	114	295950	50.00	ug/L	0.00
28) Chlorobenzene-d5	10.094	117	268565	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.059	152	113785	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.387	65	91275	45.90	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.80%		
7) Chloroethane-d5	1.693	69	85284	51.61	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	103.22%		
11) 1,1-Dichloroethene-d2	2.346	63	136606	36.36	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	72.72%		
21) 2-Butanone-d5	4.523	46	138564	114.18	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	114.18%		
24) Chloroform-d	5.135	84	199796	53.64	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	107.28%		
26) 1,2-Dichloroethane-d4	6.029	65	128459	53.45	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	106.90%		
32) Benzene-d6	6.047	84	409560	51.54	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.08%		
36) 1,2-Dichloropropane-d6	7.364	67	128104	52.29	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	104.58%		
41) Toluene-d8	8.694	98	362985	50.89	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.78%		
43) trans-1,3-Dichloroprop...	8.988	79	63556	49.80	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	99.60%		
47) 2-Hexanone-d5	9.424	63	106700	107.35	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	107.35%		
56) 1,1,2,2-Tetrachloroeth...	11.230	84	155403	51.10	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	102.20%		
66) 1,2-Dichlorobenzene-d4	12.359	152	118024	54.19	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.38%		
Target Compounds					Qvalue	
35) Methylcyclohexane	7.370	83	31856	8.90	ug/L	# 19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
Data File : VX020963.D
Acq On : 02 Mar 2021 10:50
Operator : JC/MD
Sample : VX0303MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK107

Quant Time: Mar 03 01:05:49 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 03 01:05:22 2021
Response via : Initial Calibration

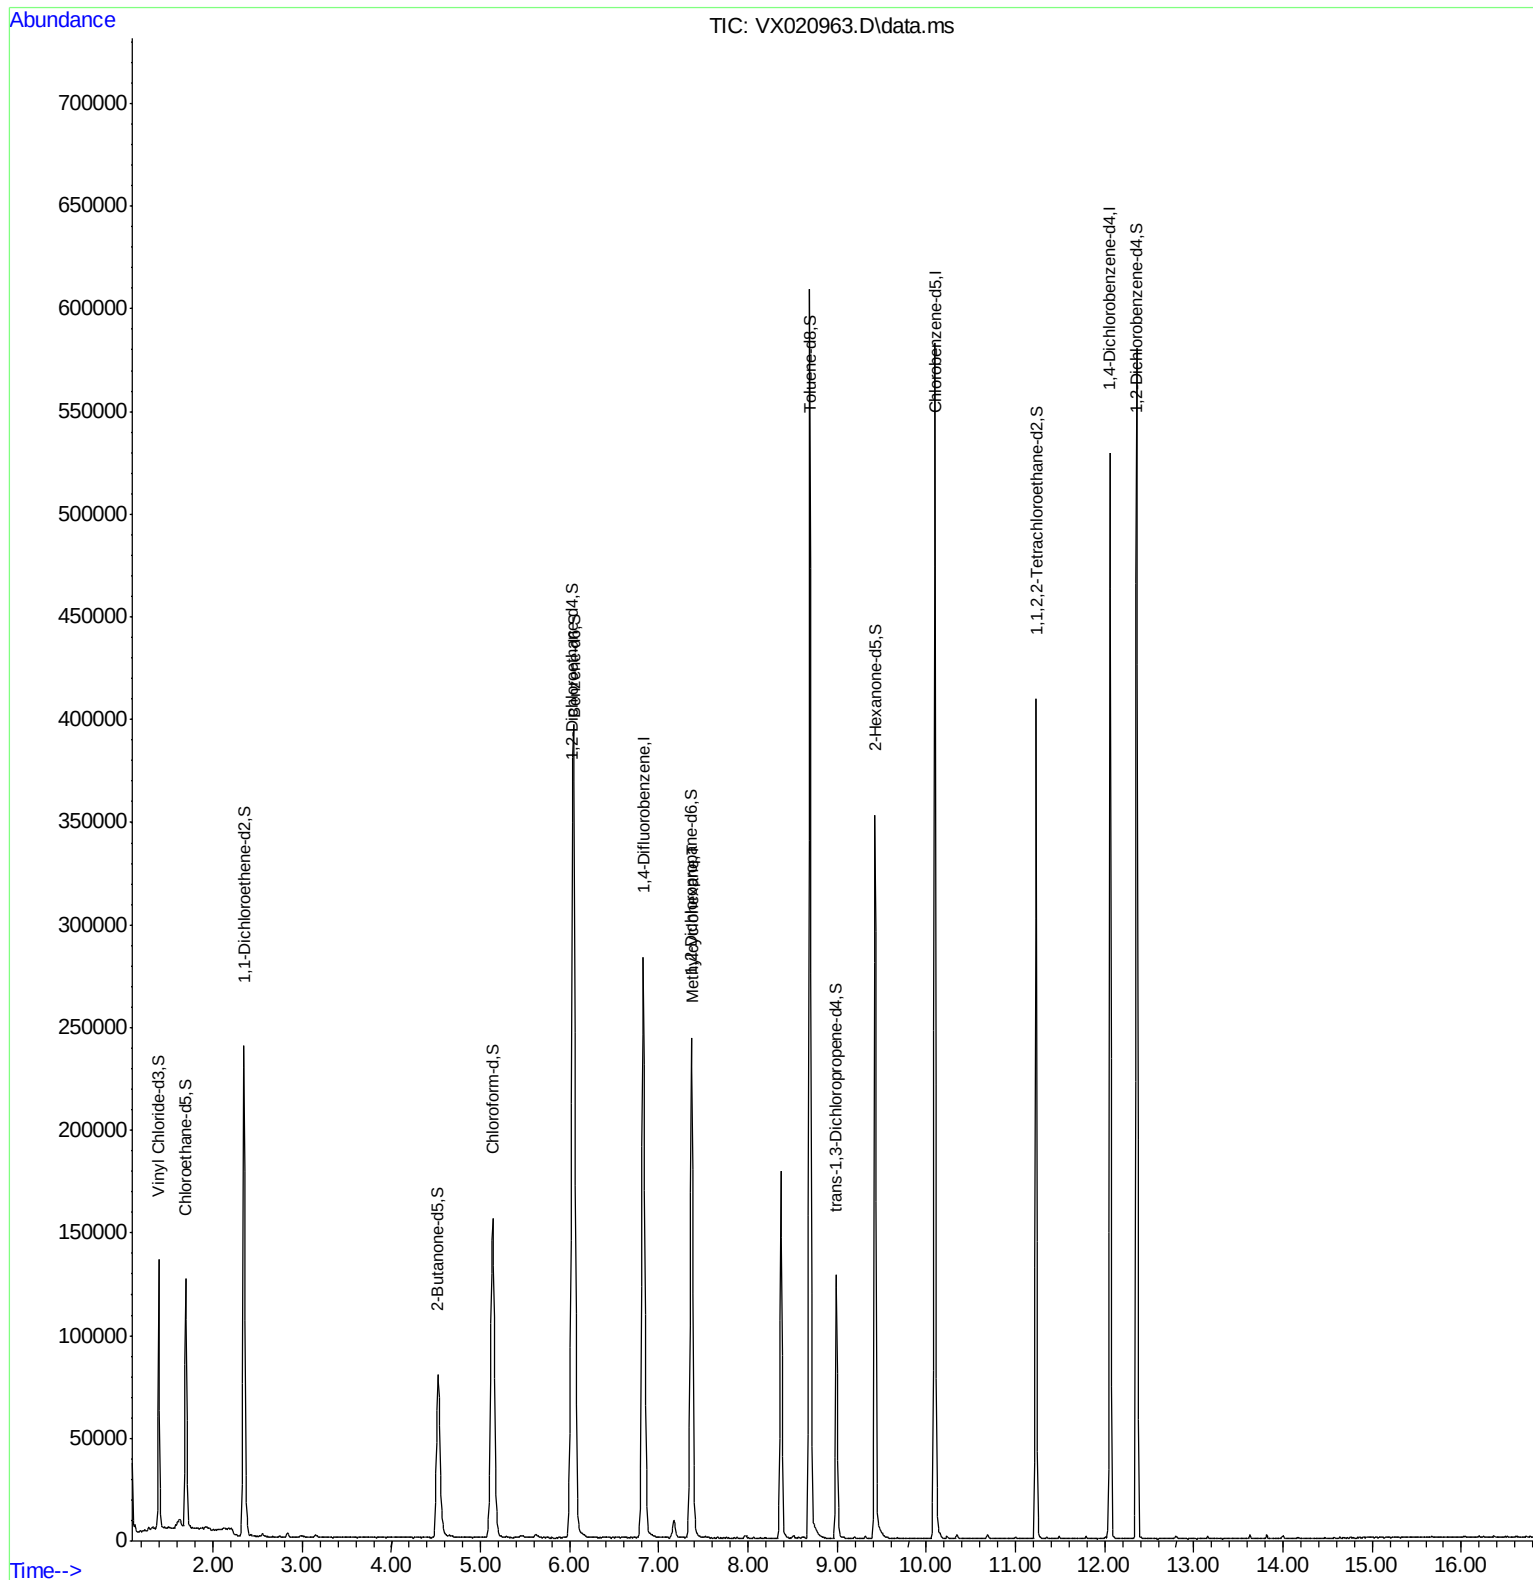

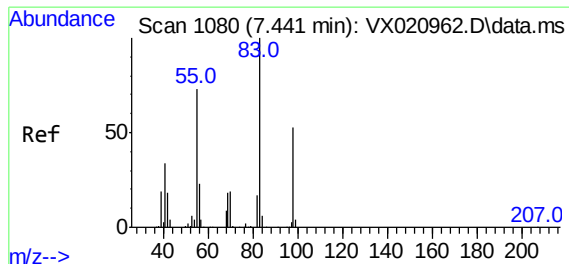

#35
Methylcyclohexane
Concen: 8.90 ug/L
RT: 7.370 min Scan# 1068
Delta R.T. -0.071 min
Lab File: VX020963.D
Acq: 02 Mar 2021 10:50

Instrument :
MSVOA_X
ClientSampleId :
VBLK107

Tgt Ion: 83 Resp: 31856

Ion	Ratio	Lower	Upper
83	100		
55	0.5	61.2	91.8#
98	1.8	38.7	58.1#

