

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
 Data File : VX020963.D
 Acq On : 02 Mar 2021 10:50
 Operator : JC/MD
 Sample : VX0303MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK107

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Title : VOC Analysis

Signal : TIC: VX020963.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.387	48	51	61	rVB	130623	142842	12.21%	1.694%
2	1.693	99	103	114	rVB	121713	151131	12.92%	1.792%
3	2.346	207	214	225	rBV	238146	396671	33.90%	4.704%
4	2.552	247	249	254	rVB2	1329	1317	0.11%	0.016%
5	2.834	293	297	303	rVB5	1868	3247	0.28%	0.039%
6	2.987	318	323	333	rBV8	821	2469	0.21%	0.029%
7	3.135	346	348	349	rBV	491	386	0.03%	0.005%
8	3.152	349	351	352	rVB	588	346	0.03%	0.004%
9	3.346	383	384	385	rBV	454	289	0.02%	0.003%
10	4.258	537	539	541	rBV	400	366	0.03%	0.004%
11	4.523	572	584	602	rBV	79635	236434	20.21%	2.804%
12	5.135	676	688	702	rBV	155245	463563	39.62%	5.497%
13	5.464	738	744	747	rBV3	875	1861	0.16%	0.022%
14	5.617	767	770	777	rVB6	1393	2709	0.23%	0.032%
15	5.794	799	800	804	rBV2	452	522	0.04%	0.006%
16	6.041	828	842	860	rBV2	396168	1170094	100.00%	13.874%
17	6.470	913	915	920	rBV3	271	518	0.04%	0.006%
18	6.523	920	924	925	rBV2	326	425	0.04%	0.005%
19	6.823	965	975	987	rBV	282920	665156	56.85%	7.887%
20	7.164	1026	1033	1042	rBV3	8432	18799	1.61%	0.223%
21	7.364	1058	1067	1085	rVV	243159	530359	45.33%	6.289%
22	7.523	1092	1094	1100	rVV3	904	1582	0.14%	0.019%
23	7.659	1114	1117	1119	rBV3	306	327	0.03%	0.004%
24	7.876	1152	1154	1156	rVB2	389	321	0.03%	0.004%
25	7.976	1165	1171	1177	rVB4	1352	2638	0.23%	0.031%
26	8.247	1214	1217	1219	rBV3	240	311	0.03%	0.004%
27	8.370	1231	1238	1252	rVV	178836	290482	24.83%	3.444%
28	8.512	1256	1262	1267	rBV3	1168	1913	0.16%	0.023%
29	8.618	1275	1280	1285	rBV5	585	1289	0.11%	0.015%
30	8.694	1285	1293	1318	rVV	608375	951554	81.32%	11.283%
31	8.918	1327	1331	1332	rBV	405	424	0.04%	0.005%
32	8.988	1337	1343	1355	rBV	128166	189328	16.18%	2.245%
33	9.118	1364	1365	1367	rBV	383	359	0.03%	0.004%
34	9.194	1374	1378	1382	rVB4	474	730	0.06%	0.009%
35	9.312	1395	1398	1403	rVB3	964	1333	0.11%	0.016%
36	9.424	1411	1417	1439	rVV	352167	508421	43.45%	6.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
 Data File : VX020963.D
 Acq On : 02 Mar 2021 10:50
 Operator : JC/MD
 Sample : VX0303MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK107

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Title : VOC Analysis

37	9.565	1439	1441	1444	rVB3	581	424	0.04%	0.005%
38	9.641	1453	1454	1459	rVB3	422	592	0.05%	0.007%
39	9.677	1459	1460	1463	rBV	484	312	0.03%	0.004%
40	9.759	1473	1474	1476	rBV	382	264	0.02%	0.003%
41	10.094	1525	1531	1546	rVV	582401	772325	66.01%	9.158%
42	10.188	1546	1547	1552	rVV3	354	529	0.05%	0.006%
43	10.230	1552	1554	1560	rVB3	1532	1787	0.15%	0.021%
44	10.283	1560	1563	1565	rBV2	278	392	0.03%	0.005%
45	10.341	1569	1573	1578	rVV3	1760	2403	0.21%	0.028%
46	10.565	1608	1611	1612	rVB2	318	277	0.02%	0.003%
47	10.583	1612	1614	1616	rBV	295	302	0.03%	0.004%
48	10.688	1626	1632	1637	rVB5	1814	3303	0.28%	0.039%
49	10.853	1659	1660	1664	rVB4	398	411	0.04%	0.005%
50	10.888	1664	1666	1669	rBV	368	292	0.02%	0.003%
51	10.924	1669	1672	1676	rVB2	253	335	0.03%	0.004%
52	10.953	1676	1677	1681	rBV2	225	264	0.02%	0.003%
53	11.000	1681	1685	1689	rBV2	961	1328	0.11%	0.016%
54	11.118	1701	1705	1709	rVB4	605	878	0.08%	0.010%
55	11.230	1718	1724	1731	rBV	409216	497020	42.48%	5.893%
56	11.283	1731	1733	1734	rVB2	511	317	0.03%	0.004%
57	11.353	1741	1745	1748	rVB	530	728	0.06%	0.009%
58	11.489	1764	1768	1773	rBV2	1172	1314	0.11%	0.016%
59	11.747	1807	1812	1815	rVB2	461	539	0.05%	0.006%
60	11.789	1815	1819	1823	rVB3	1249	1755	0.15%	0.021%
61	11.936	1841	1844	1846	rBV3	243	317	0.03%	0.004%
62	12.006	1852	1856	1860	rBV2	1088	1398	0.12%	0.017%
63	12.059	1860	1865	1875	rVV	528574	660027	56.41%	7.826%
64	12.159	1880	1882	1886	rVB2	343	325	0.03%	0.004%
65	12.359	1910	1916	1923	rVV	579677	721163	61.63%	8.551%
66	12.542	1940	1947	1949	rBV2	235	418	0.04%	0.005%
67	12.559	1949	1950	1955	rVB3	218	355	0.03%	0.004%
68	12.795	1986	1990	1995	rBV2	1632	2274	0.19%	0.027%
69	12.883	2002	2005	2007	rVV3	281	296	0.03%	0.004%
70	12.906	2007	2009	2013	rVB2	329	439	0.04%	0.005%
71	13.018	2025	2028	2030	rVB2	259	287	0.02%	0.003%
72	13.036	2030	2031	2033	rBV	337	274	0.02%	0.003%
73	13.153	2048	2051	2054	rVB4	1340	1562	0.13%	0.019%
74	13.195	2056	2058	2060	rBV2	283	292	0.02%	0.003%
75	13.348	2083	2084	2087	rBV2	259	261	0.02%	0.003%
76	13.501	2107	2110	2112	rBV3	263	277	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
 Data File : VX020963.D
 Acq On : 02 Mar 2021 10:50
 Operator : JC/MD
 Sample : VX0303MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK107

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
 Title : VOC Analysis

77	13.630	2128	2132	2137	rVB3	1848	2157	0.18%	0.026%
78	13.759	2151	2154	2157	rBV3	366	537	0.05%	0.006%
79	13.818	2159	2164	2169	rVB2	1950	2306	0.20%	0.027%
80	13.865	2169	2172	2174	rVB2	312	279	0.02%	0.003%
81	13.895	2174	2177	2180	rBV3	258	348	0.03%	0.004%
82	14.001	2191	2195	2200	rVB4	1419	1858	0.16%	0.022%
83	14.112	2210	2214	2216	rBV2	274	329	0.03%	0.004%
84	14.159	2216	2222	2224	rBV4	457	702	0.06%	0.008%
85	14.430	2267	2268	2272	rBV	235	266	0.02%	0.003%
86	14.465	2272	2274	2277	rBV	377	394	0.03%	0.005%
87	14.536	2282	2286	2288	rBV2	278	364	0.03%	0.004%
88	14.636	2301	2303	2308	rVV2	416	648	0.06%	0.008%
89	15.001	2364	2365	2369	rVB3	413	264	0.02%	0.003%
90	15.048	2369	2373	2376	rVB4	438	488	0.04%	0.006%
91	15.142	2388	2389	2391	rBV	446	386	0.03%	0.005%
92	15.189	2395	2397	2400	rVB3	383	318	0.03%	0.004%
93	15.218	2400	2402	2405	rBV2	469	600	0.05%	0.007%
94	15.318	2418	2419	2422	rBV3	395	364	0.03%	0.004%
95	15.395	2430	2432	2435	rVB2	455	346	0.03%	0.004%
96	15.607	2464	2468	2469	rBV3	528	613	0.05%	0.007%
97	15.701	2482	2484	2485	rBV2	380	301	0.03%	0.004%
98	16.024	2537	2539	2540	rBV2	430	317	0.03%	0.004%
99	16.360	2595	2596	2599	rVB3	587	472	0.04%	0.006%
100	16.513	2620	2622	2625	rBV4	412	286	0.02%	0.003%




Sum of corrected areas: 8433515

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
Data File : VX020963.D
Acq On : 02 Mar 2021 10:50
Operator : JC/MD
Sample : VX0303MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

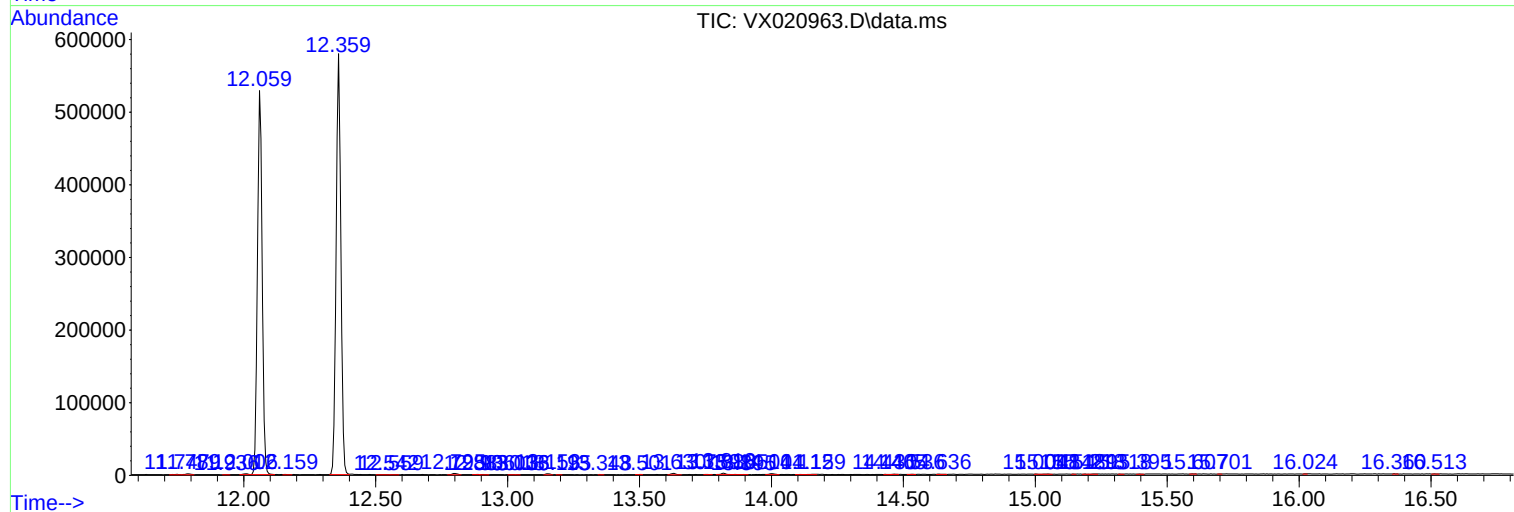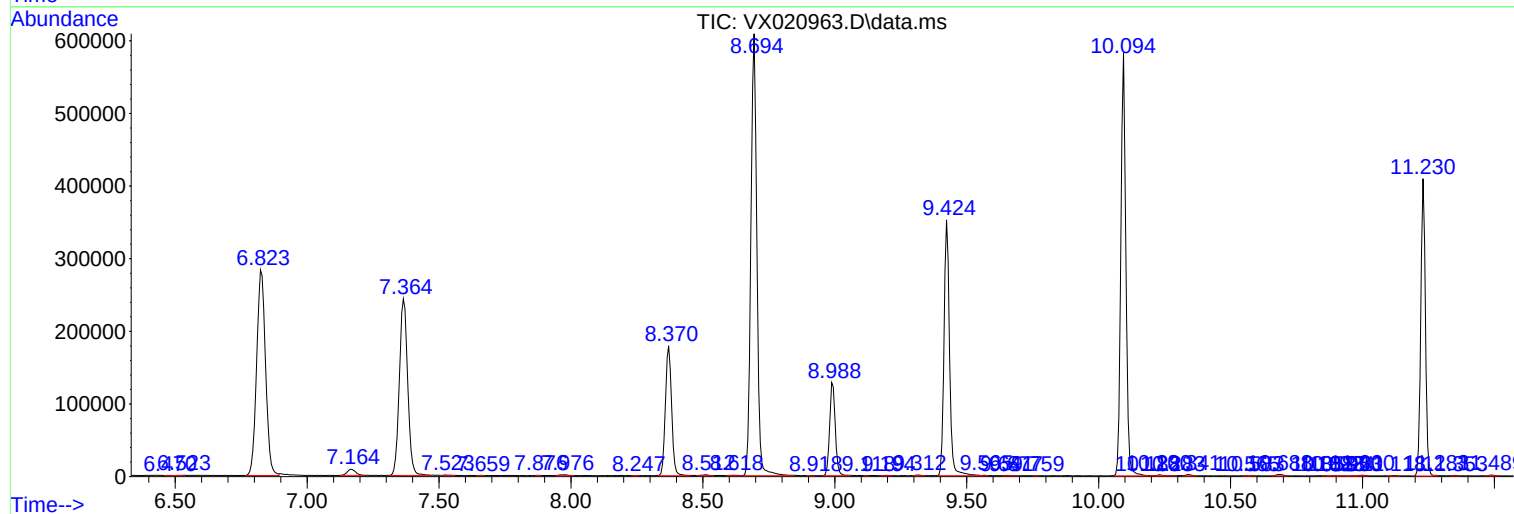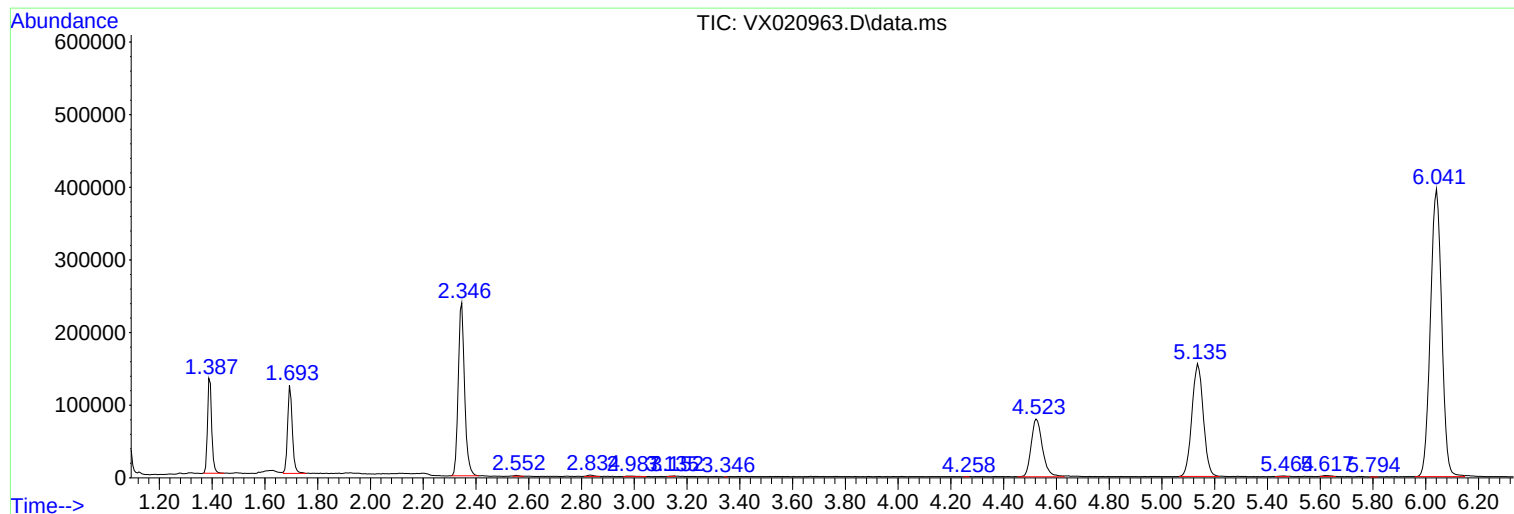

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
Data File : VX020963.D
Acq On : 02 Mar 2021 10:50
Operator : JC/MD
Sample : VX0303MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
Data File : VX020963.D
Acq On : 02 Mar 2021 10:50
Operator : JC/MD
Sample : VX0303MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK107

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML022621WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc