


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030321\
 Data File : VX020961.D
 Acq On : 02 Mar 2021 09:48
 Operator : JC/MD
 Sample : BFB69
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB69

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM022621WMA.M
 Title : VOC Analysis
 Last Update : Wed Mar 03 01:05:22 2021

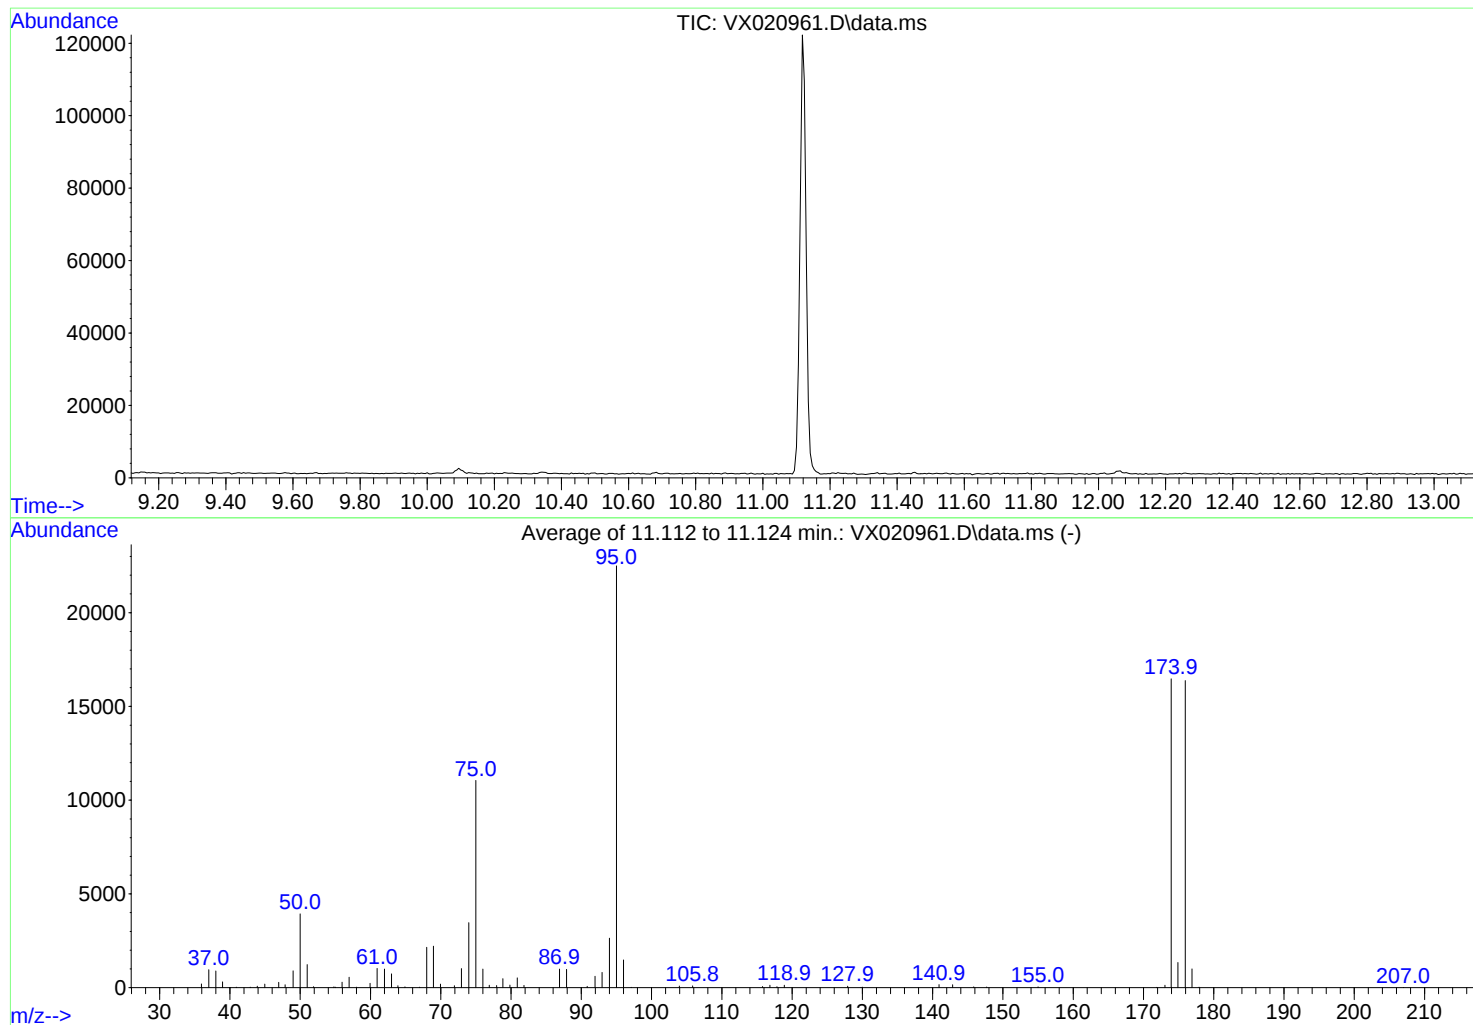

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1699

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	3939	PASS
75	95	30	80	49.1	11050	PASS
95	95	100	100	100.0	22499	PASS
96	95	5	9	6.6	1474	PASS
173	174	0.00	2	0.8	131	PASS
174	95	50	120	73.2	16469	PASS
175	174	5	9	8.1	1341	PASS
176	174	95	101	99.5	16379	PASS
177	176	5	9	6.1	1000	PASS

m/z	Abundance
35.90	160.0
37.00	875.0
38.00	795.0
38.90	271.0
39.90	441.0
40.90	67.0
42.90	81.0
43.90	734.0
44.90	165.0
47.00	329.0
47.80	130.0
49.00	823.0
50.00	3491.0
51.00	968.0
54.80	65.0
55.90	229.0
56.90	440.0
59.90	230.0
60.90	891.0
62.00	938.0
63.00	638.0
63.90	65.0
68.00	1856.0
68.90	1661.0
69.90	142.0
71.90	103.0
73.00	889.0
74.00	2885.0
75.00	9342.0
76.00	922.0
76.90	135.0
78.00	96.0
78.80	418.0
79.90	107.0
80.90	418.0
81.80	116.0
86.90	811.0
87.90	665.0
90.90	52.0
91.90	486.0
92.90	660.0
94.00	2010.0
95.00	18032.0
96.00	1359.0
104.00	56.0
105.90	64.0
116.90	110.0
118.90	87.0
127.80	55.0
140.90	117.0
142.80	97.0
173.10	92.0
173.90	11127.0
174.90	1025.0
176.00	9906.0
176.90	585.0
207.00	71.0

Instrument :
MSVOA_X
ClientSampleId :
BFB69

m/z	Abundance
36.00	269.0
37.00	1097.0
38.00	1012.0
39.00	328.0
40.00	475.0
42.90	59.0
43.90	691.0
44.90	207.0
46.90	258.0
47.90	146.0
49.00	1037.0
50.00	4666.0
51.00	1505.0
51.90	57.0
55.00	81.0
56.00	374.0
57.00	720.0
58.00	65.0
60.00	215.0
60.90	1181.0
62.00	1119.0
63.00	911.0
63.90	114.0
64.90	73.0
68.00	2424.0
69.00	2780.0
69.90	218.0
72.00	119.0
72.90	1169.0
74.00	4147.0
75.00	12655.0
76.00	1076.0
76.90	150.0
77.90	129.0
78.90	575.0
79.90	154.0
80.90	619.0
81.80	135.0
86.90	1101.0
87.90	1132.0
90.90	89.0
92.00	677.0
93.00	933.0
94.00	3197.0
95.00	27560.0
96.00	1615.0
97.10	60.0
103.90	90.0
105.90	101.0
115.80	81.0
116.80	143.0
117.90	77.0
118.90	194.0
127.90	106.0
129.80	61.0
140.90	195.0
142.90	162.0
145.80	77.0
147.70	50.0
155.00	64.0
172.90	150.0
174.00	18848.0
174.90	1617.0
175.90	19576.0
176.90	1160.0
177.90	69.0
207.00	73.0

Instrument :
MSVOA_X
ClientSampleId :
BFB69

m/z	Abundance
35.90	160.0
37.00	884.0
38.00	853.0
39.00	330.0
39.90	468.0
42.90	102.0
43.90	683.0
45.00	182.0
47.00	262.0
47.90	189.0
49.00	818.0
50.00	3660.0
51.00	1221.0
51.90	105.0
54.80	77.0
55.90	267.0
56.90	501.0
60.00	253.0
61.00	994.0
62.00	916.0
63.00	662.0
63.90	130.0
64.90	67.0
67.00	78.0
68.00	2169.0
69.00	2202.0
70.00	207.0
72.00	94.0
73.00	985.0
74.00	3361.0
75.00	11153.0
76.00	970.0
76.90	98.0
77.90	103.0
78.90	432.0
79.80	156.0
80.90	531.0
81.90	112.0
86.90	1068.0
87.90	1116.0
90.80	69.0
92.00	659.0
93.00	839.0
94.00	2706.0
95.00	21904.0
96.00	1447.0
103.90	101.0
105.80	111.0
115.80	92.0
116.90	131.0
117.80	69.0
118.90	112.0
128.00	61.0
130.00	91.0
140.90	165.0
142.90	201.0
145.90	56.0
147.70	54.0
155.00	68.0
171.90	55.0
173.10	152.0
173.90	19432.0
174.90	1381.0
175.90	19656.0
176.90	1255.0
207.00	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB69

Scan 1699 (11.082 min): VX020961.D\data.ms
BFB69

m/z	Abundance
39.00	457.0
43.00	52.0
44.00	622.0
207.00	61.0

Instrument :
MSVOA_X
ClientSampleId :
BFB69