

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030323\
 Data File : VX034314.D
 Acq On : 03 Mar 2023 11:50
 Operator : JC/MD
 Sample : 01740-05
 Misc : 10.33g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TOTAL-VOC-8-GRAB-8

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
 Title : SW846 8260

Signal : TIC: VX034314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	67	83	86	rBV8	16509	71645	5.38%	0.989%
2	2.940	297	304	313	rVB2	6047	14062	1.06%	0.194%
3	5.385	692	705	720	rBV	145628	421991	31.66%	5.825%
4	5.544	720	731	748	rVB	242476	707732	53.11%	9.768%
5	5.952	788	798	813	rBV2	161723	433433	32.52%	5.982%
6	6.757	917	930	946	rBV	399562	952291	71.46%	13.144%
7	8.647	1233	1240	1254	rBV	855667	1332689	100.00%	18.394%
8	10.055	1465	1471	1485	rBV	807235	1108515	83.18%	15.300%
9	11.085	1634	1640	1651	rBV	639434	872321	65.46%	12.040%
10	11.219	1653	1662	1671	rVB6	9715	20976	1.57%	0.290%
11	11.634	1721	1730	1734	rBV7	5678	13627	1.02%	0.188%
12	11.713	1740	1743	1746	rBV	13424	15420	1.16%	0.213%
13	11.841	1759	1764	1767	rBV4	8285	13606	1.02%	0.188%
14	11.939	1776	1780	1784	rVV3	9972	15733	1.18%	0.217%
15	12.024	1789	1794	1801	rBV	860789	1089009	81.72%	15.031%
16	12.250	1825	1831	1836	rBV9	9298	19186	1.44%	0.265%
17	12.311	1836	1841	1848	rVB7	18690	39559	2.97%	0.546%
18	12.469	1864	1867	1874	rVB7	7683	13783	1.03%	0.190%
19	12.555	1874	1881	1883	rBV5	7717	17713	1.33%	0.244%
20	12.817	1920	1924	1932	rVB8	10445	20117	1.51%	0.278%
21	12.920	1938	1941	1946	rVV	13704	17808	1.34%	0.246%
22	12.981	1946	1951	1955	rVB6	8941	16125	1.21%	0.223%
23	13.292	1998	2002	2008	rVB4	11054	17724	1.33%	0.245%




Sum of corrected areas: 7245065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030323\
Data File : VX034314.D
Acq On : 03 Mar 2023 11:50
Operator : JC/MD
Sample : 01740-05
Misc : 10.33g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTAL-VOC-8-GRAB-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

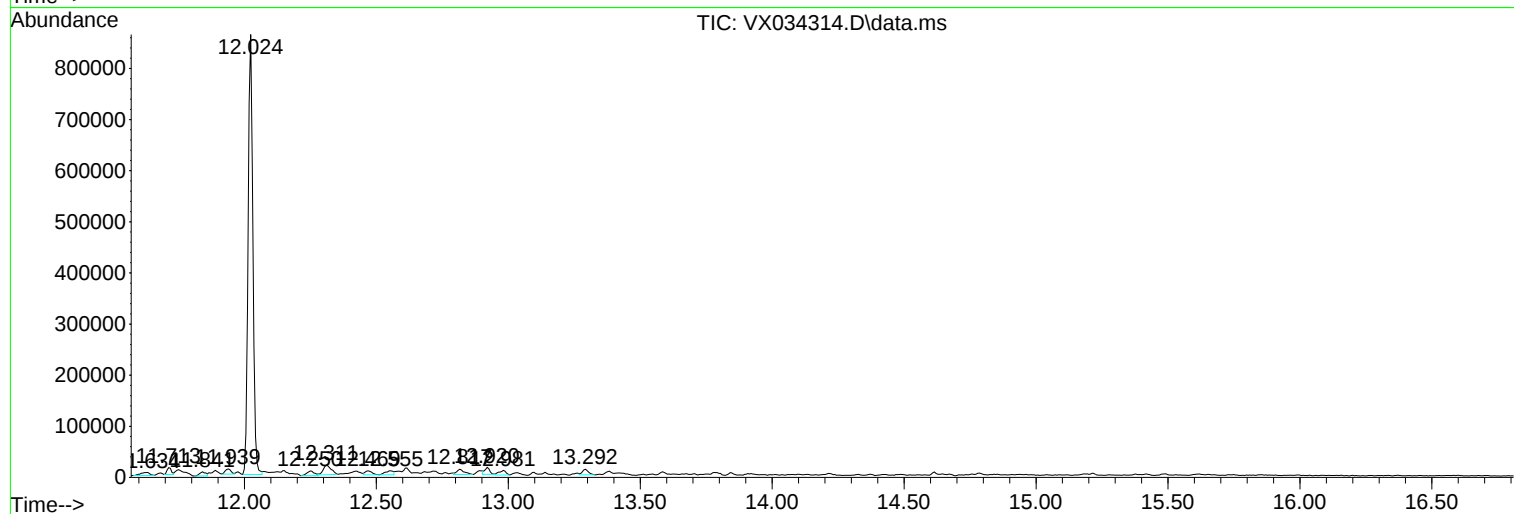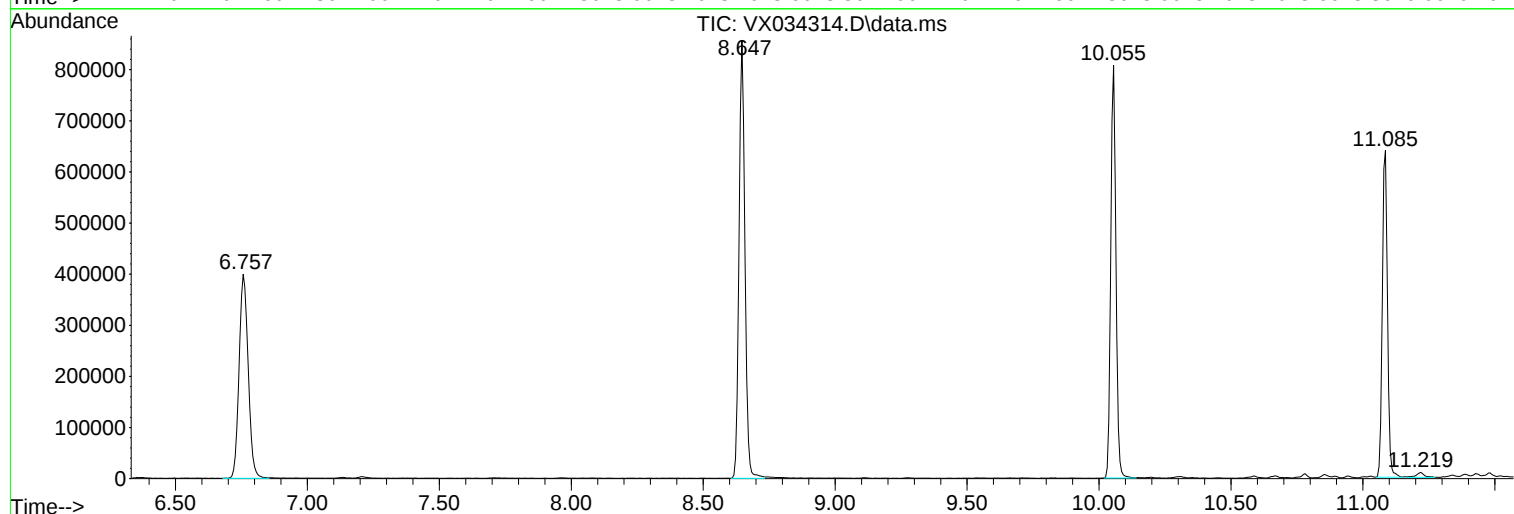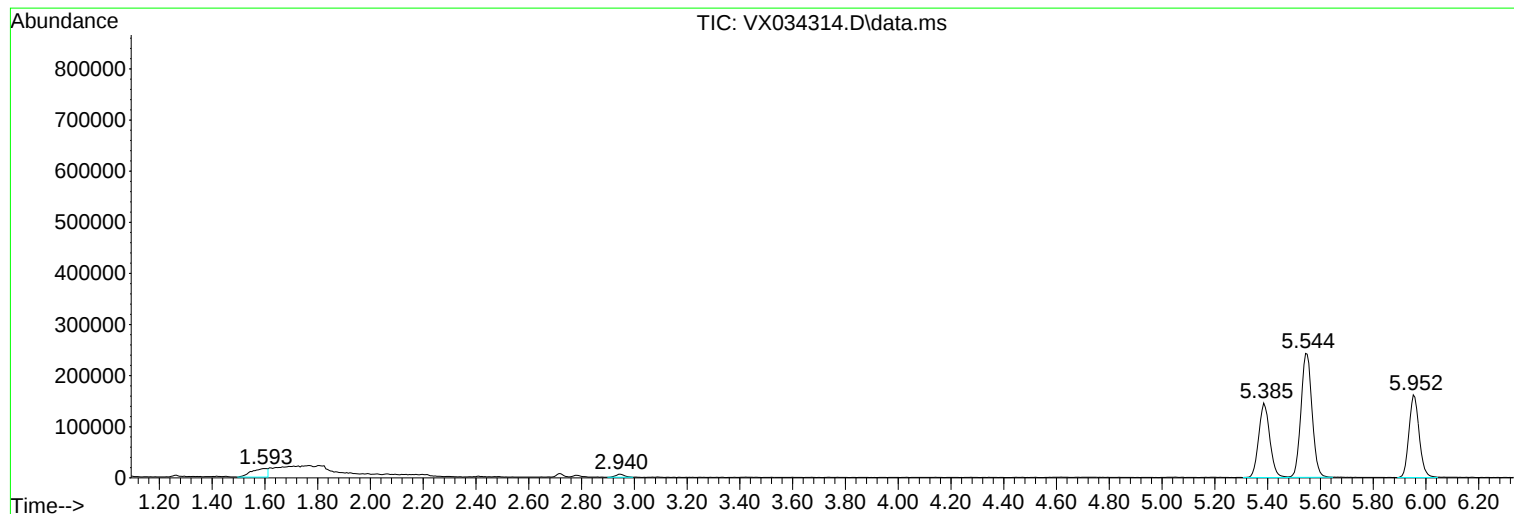

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030323\
Data File : VX034314.D
Acq On : 03 Mar 2023 11:50
Operator : JC/MD
Sample : 01740-05
Misc : 10.33g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTAL-VOC-8-GRAB-8










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.593 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.593	5.06 ug/l	71645	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Bis(2-chloroethyl) sulfone	190	C4H8Cl2O2S	000471-03-4	23
2			Propanoic acid, 2-chloro-	108	C3H5ClO2	000598-78-7	17
3			Phosgene	98	CCl2O	000075-44-5	9
4			Carbonic acid, 6-chlorohexyl pro...	222	C10H19ClO3	1000331-38-8	9
5			Acetic acid, chloro-, ethyl ester	122	C4H7ClO2	000105-39-5	9

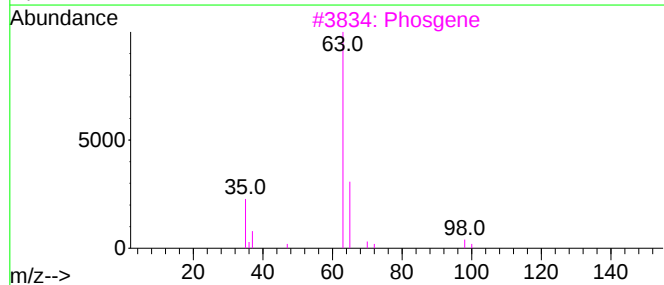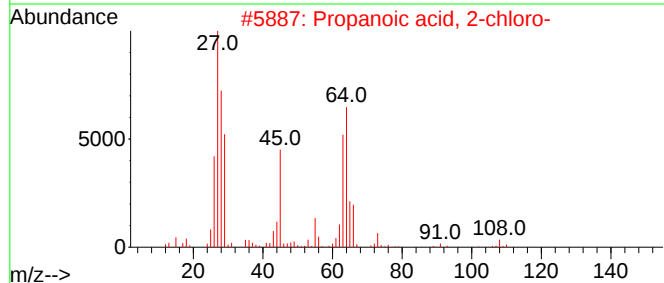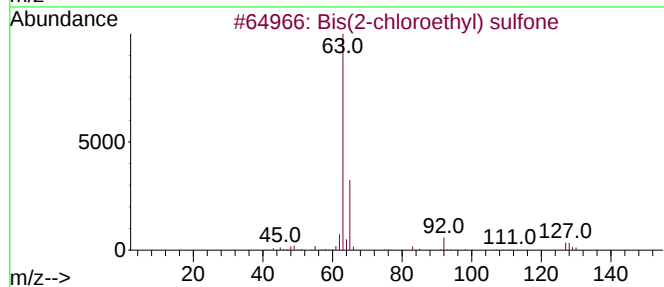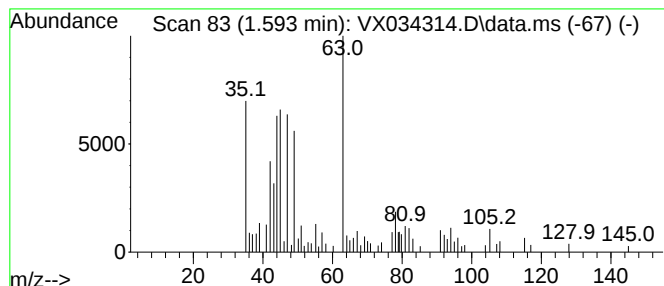

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030323\
Data File : VX034314.D
Acq On : 03 Mar 2023 11:50
Operator : JC/MD
Sample : 01740-05
Misc : 10.33g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTAL-VOC-8-GRAB-8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.593	1.593	5.1	ug/l	71645	1	5.550	707732	50.0