

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
 Data File : VX045101.D
 Acq On : 03 Mar 2025 09:16
 Operator : JC/MD
 Sample : VX0303MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0303MBL01

Quant Time: Mar 04 05:18:05 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.538	168	85856	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.751	114	167842	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	154084	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	68602	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	69138	50.626	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	101.260%
35) Dibromofluoromethane	5.379	113	57640	51.358	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.720%
50) Toluene-d8	8.641	98	209430	51.472	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.940%
62) 4-Bromofluorobenzene	11.079	95	72357	53.666	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	107.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
Data File : VX045101.D
Acq On : 03 Mar 2025 09:16
Operator : JC/MD
Sample : VX0303MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0303MBL01

Quant Time: Mar 04 05:18:05 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration




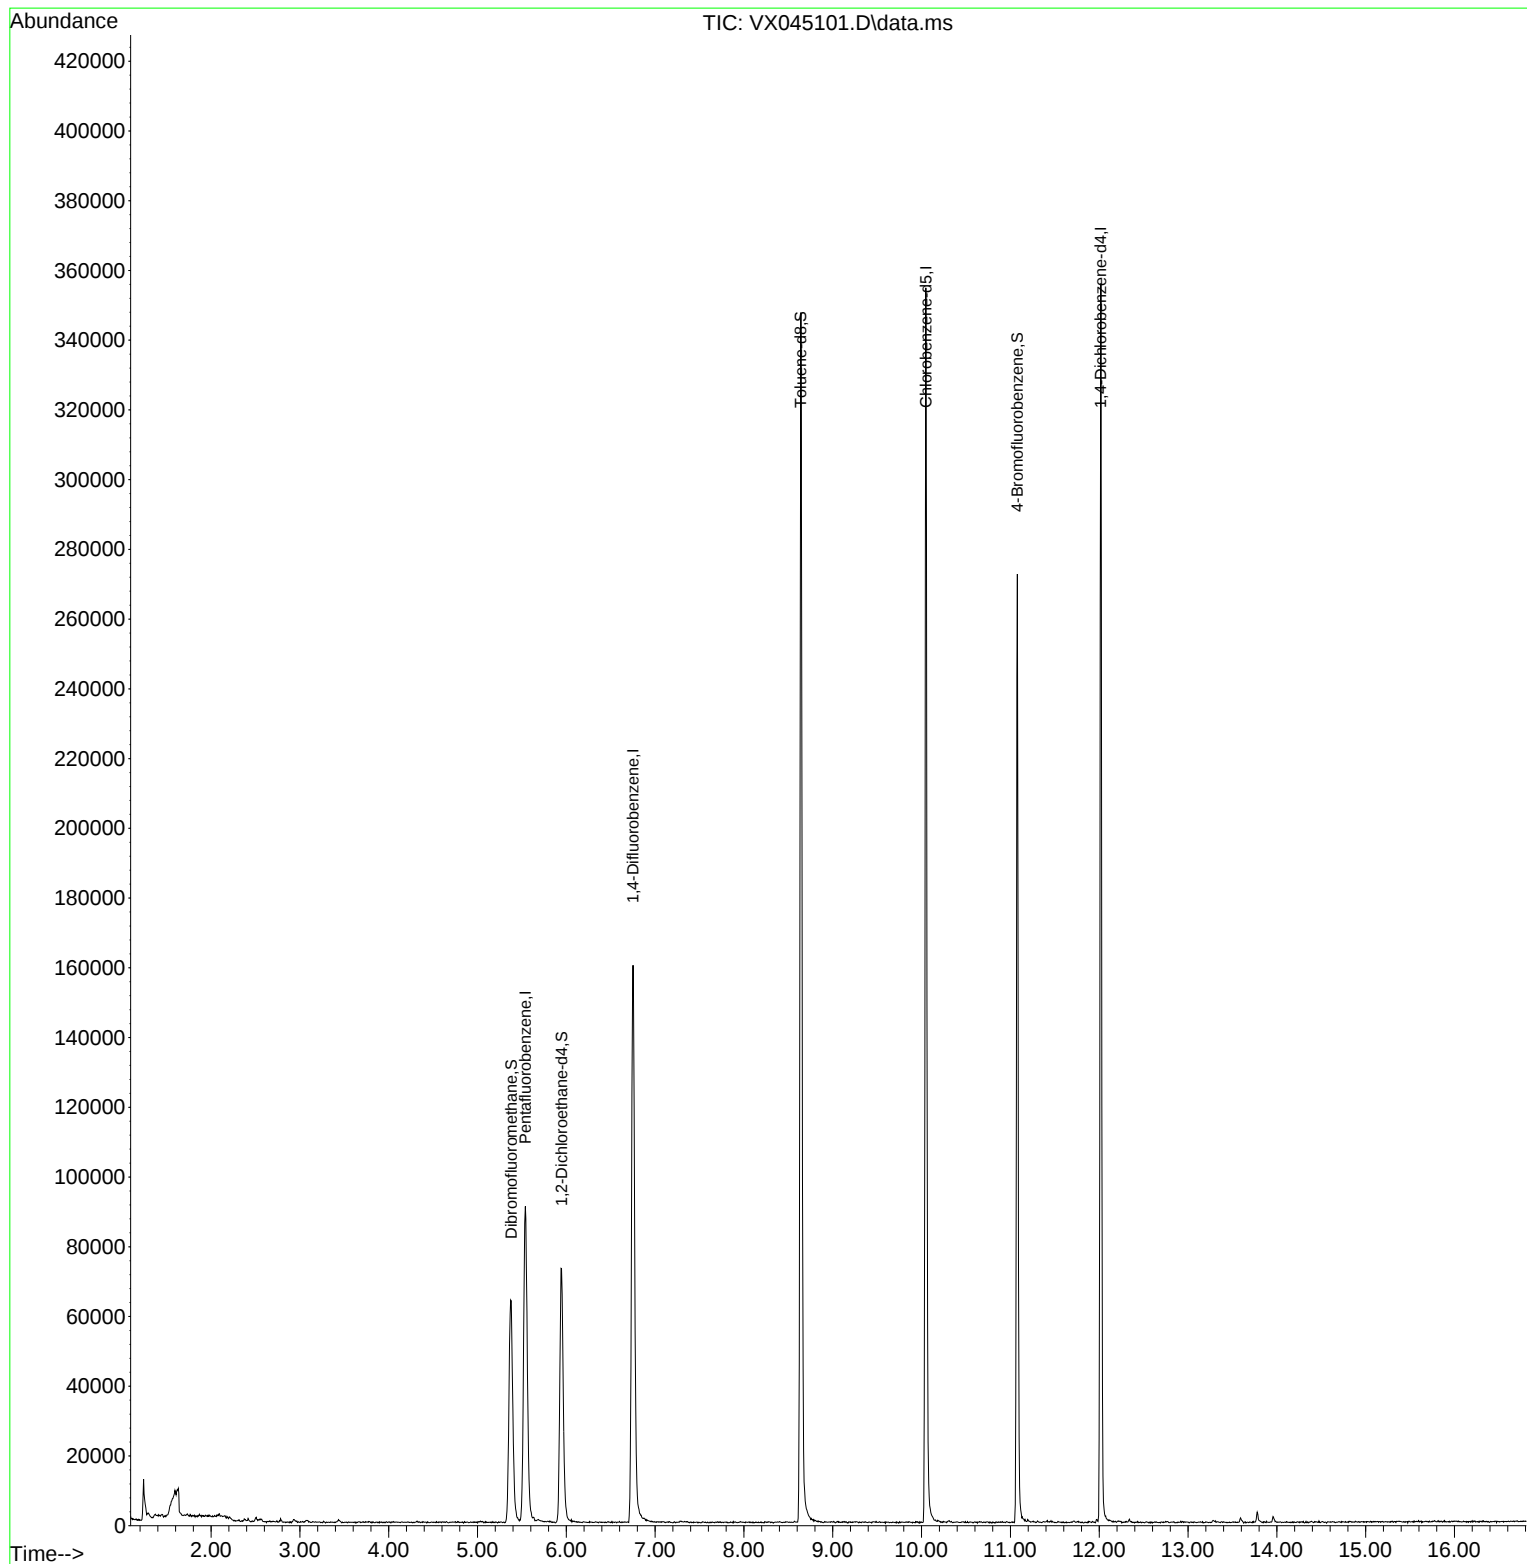


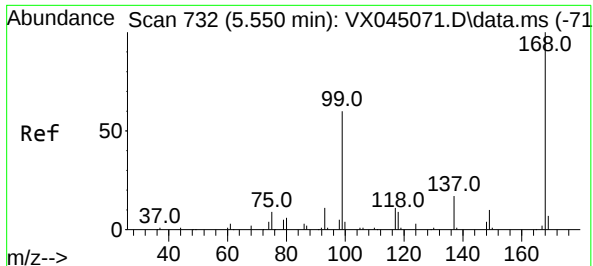

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.012 min
Lab File: VX045101.D
Acq: 03 Mar 2025 09:16




Instrument :
MSVOA_X
ClientSampleId :
VX0303MBL01


Tgt Ion:168 Resp: 85856
Ion Ratio Lower Upper
168 100
99 58.0 48.2 72.4

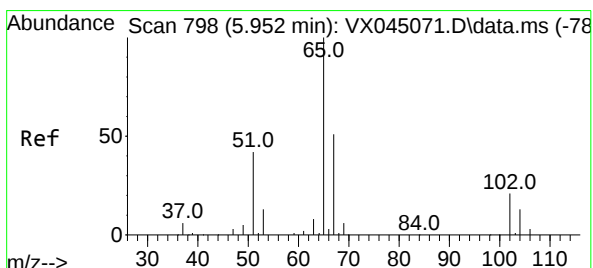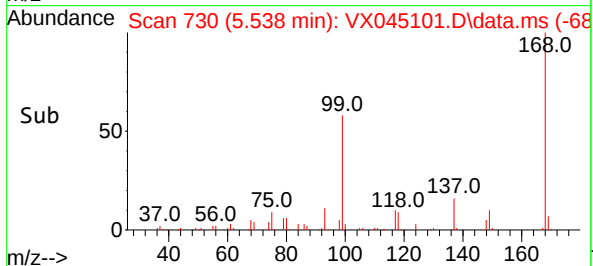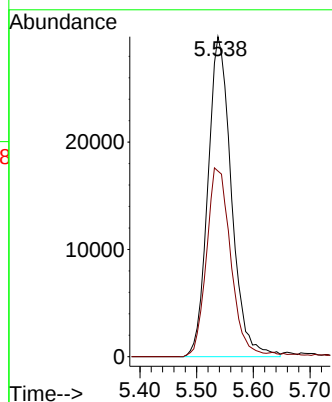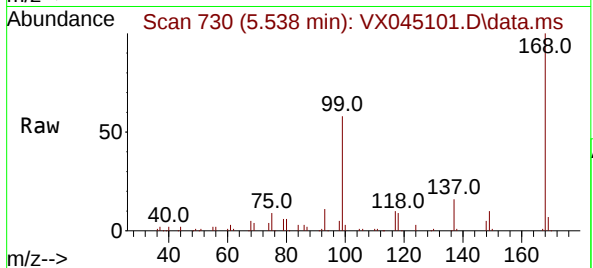

#33
1,2-Dichloroethane-d4
Concen: 50.626 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX045101.D
Acq: 03 Mar 2025 09:16

Tgt Ion: 65 Resp: 69138
Ion Ratio Lower Upper
65 100
67 53.1 0.0 106.2


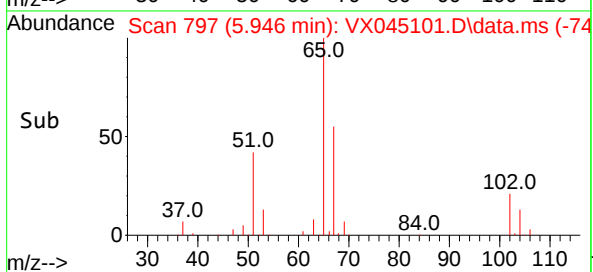
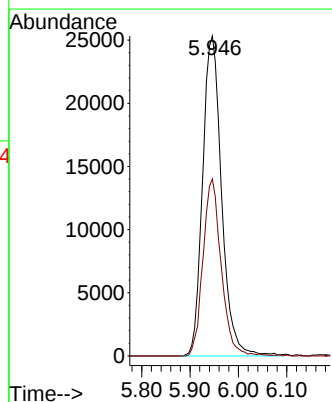
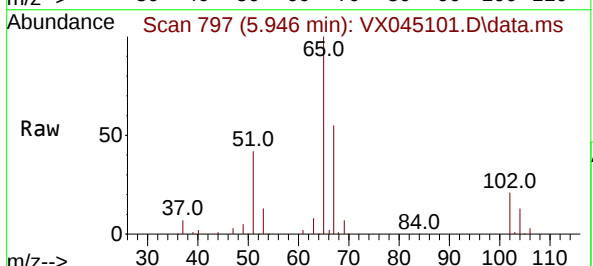


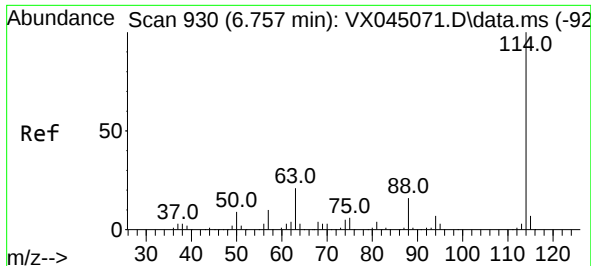

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX045101.D
Acq: 03 Mar 2025 09:16




Instrument :
MSVOA_X
ClientSampleId :
VX0303MBL01


Tgt Ion:114 Resp: 167842
Ion Ratio Lower Upper
114 100
63 21.5 0.0 41.8
88 16.3 0.0 32.8

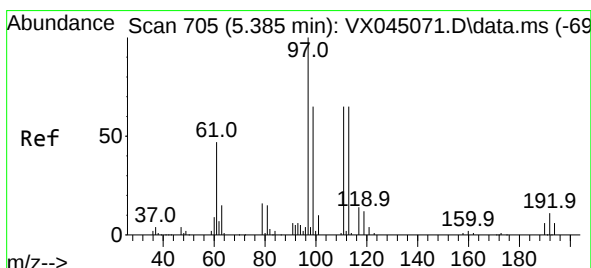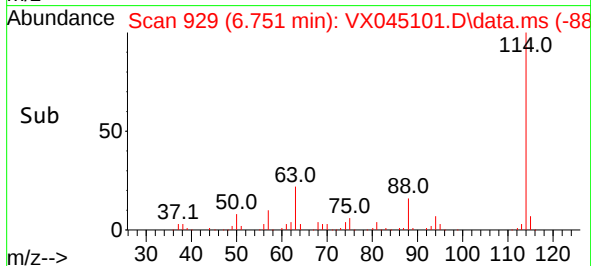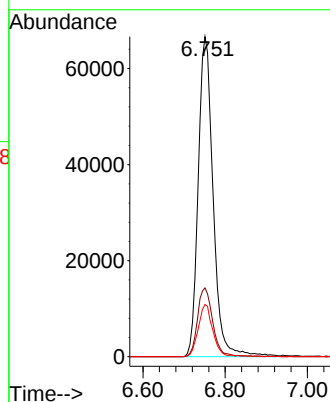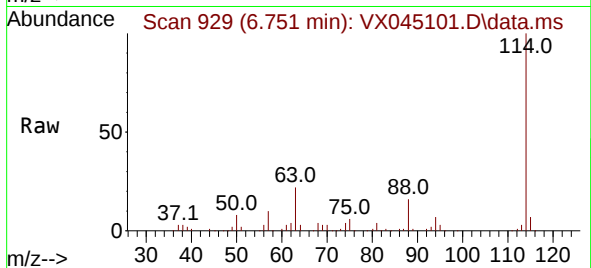

#35
Dibromofluoromethane
Concen: 51.358 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX045101.D
Acq: 03 Mar 2025 09:16

Tgt Ion:113 Resp: 57640
Ion Ratio Lower Upper
113 100
111 102.7 81.8 122.6
192 18.0 14.3 21.5


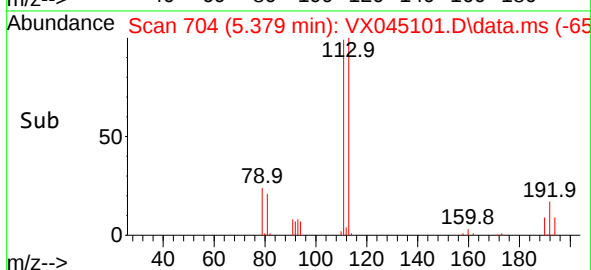
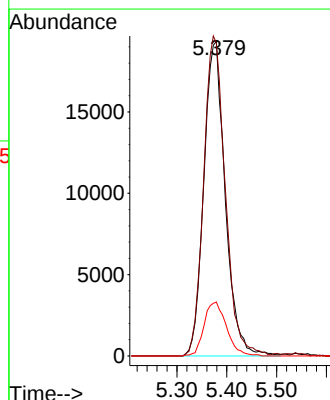
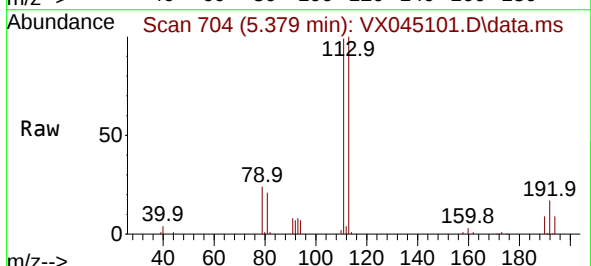


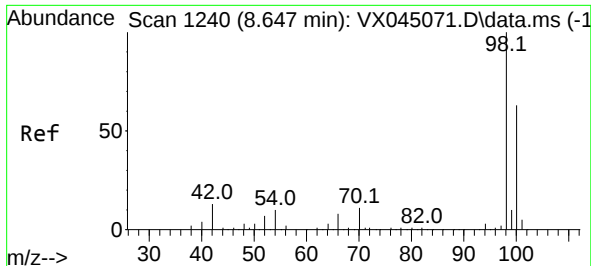

#50
Toluene-d8
Concen: 51.472 ug/l
RT: 8.641 min Scan# 1239
Delta R.T. -0.006 min
Lab File: VX045101.D
Acq: 03 Mar 2025 09:16




Instrument :
MSVOA_X
ClientSampleId :
VX0303MBL01


Tgt Ion: 98 Resp: 209430
Ion Ratio Lower Upper
98 100
100 65.3 52.0 78.0

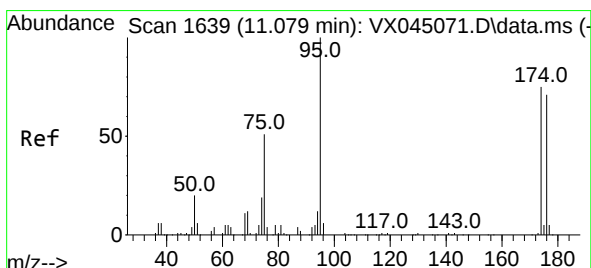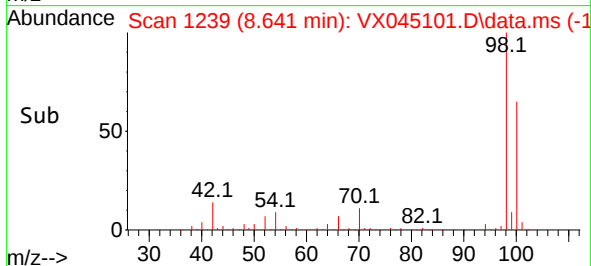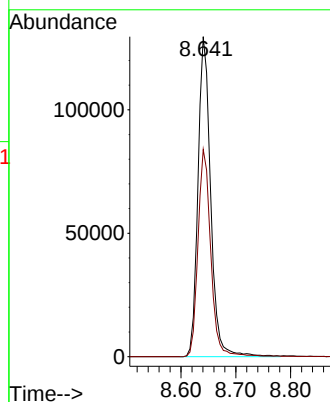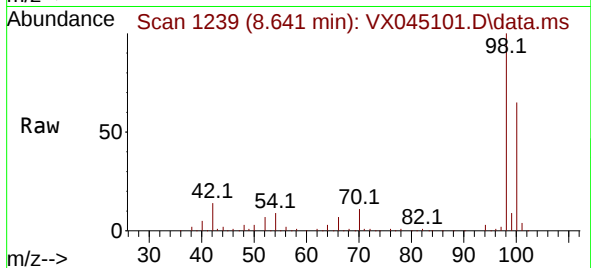

#62
4-Bromofluorobenzene
Concen: 53.666 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045101.D
Acq: 03 Mar 2025 09:16

Tgt Ion: 95 Resp: 72357
Ion Ratio Lower Upper
95 100
174 74.6 0.0 148.2
176 72.5 0.0 141.4


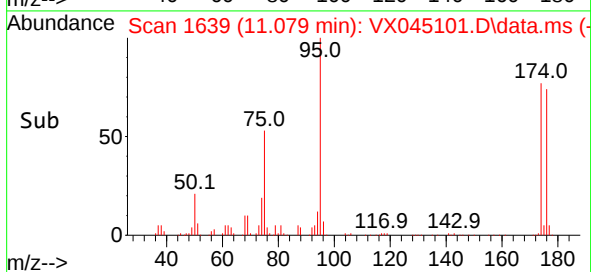
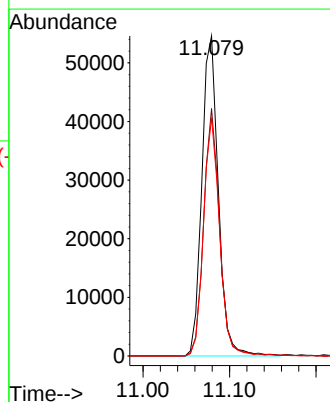
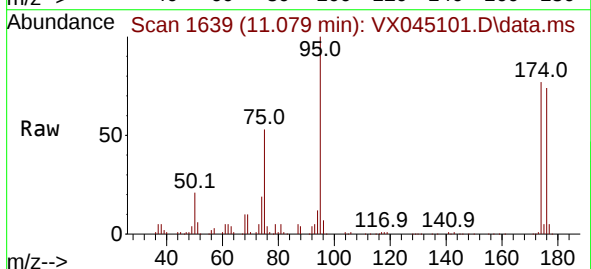


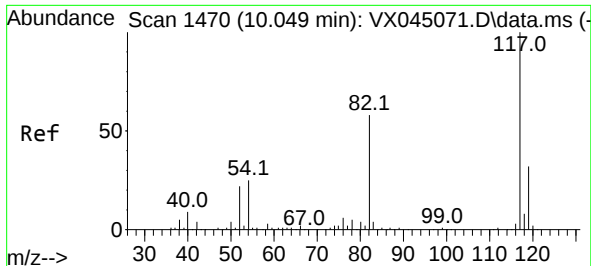

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX045101.D
Acq: 03 Mar 2025 09:16

Instrument :
MSVOA_X
ClientSampleId :
VX0303MBL01

Tgt Ion:117 Resp: 154084
Ion Ratio Lower Upper
117 100
82 56.8 46.3 69.5
119 32.2 25.7 38.5

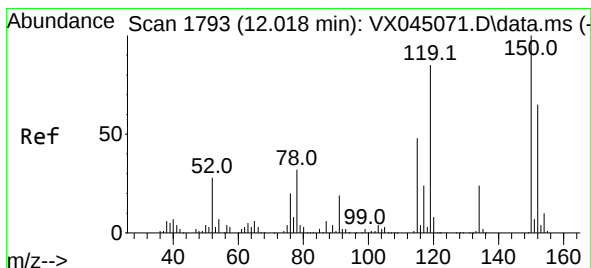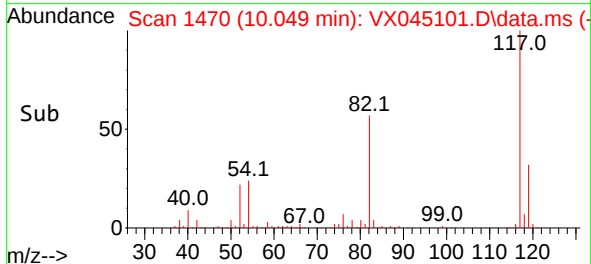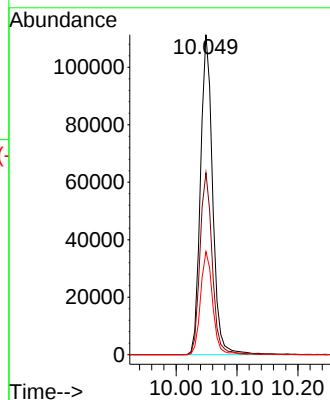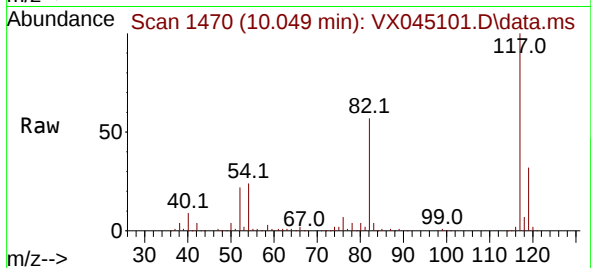

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045101.D
Acq: 03 Mar 2025 09:16

Tgt Ion:152 Resp: 68602
Ion Ratio Lower Upper
152 100
115 62.3 44.2 132.6
150 157.6 0.0 349.0

