

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
 Data File : VX045115.D
 Acq On : 03 Mar 2025 16:03
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Mar 04 05:25:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	75306	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	150223	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	138820	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	58431	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	62144	51.880	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 103.760%	
35) Dibromofluoromethane	5.379	113	51287	51.057	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.120%	
50) Toluene-d8	8.647	98	186352	51.172	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.340%	
62) 4-Bromofluorobenzene	11.079	95	63905	52.957	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 105.920%	
Target Compounds						
44) Trichloroethene	7.123	130	2464	2.412	ug/l	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
Data File : VX045115.D
Acq On : 03 Mar 2025 16:03
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Mar 04 05:25:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration




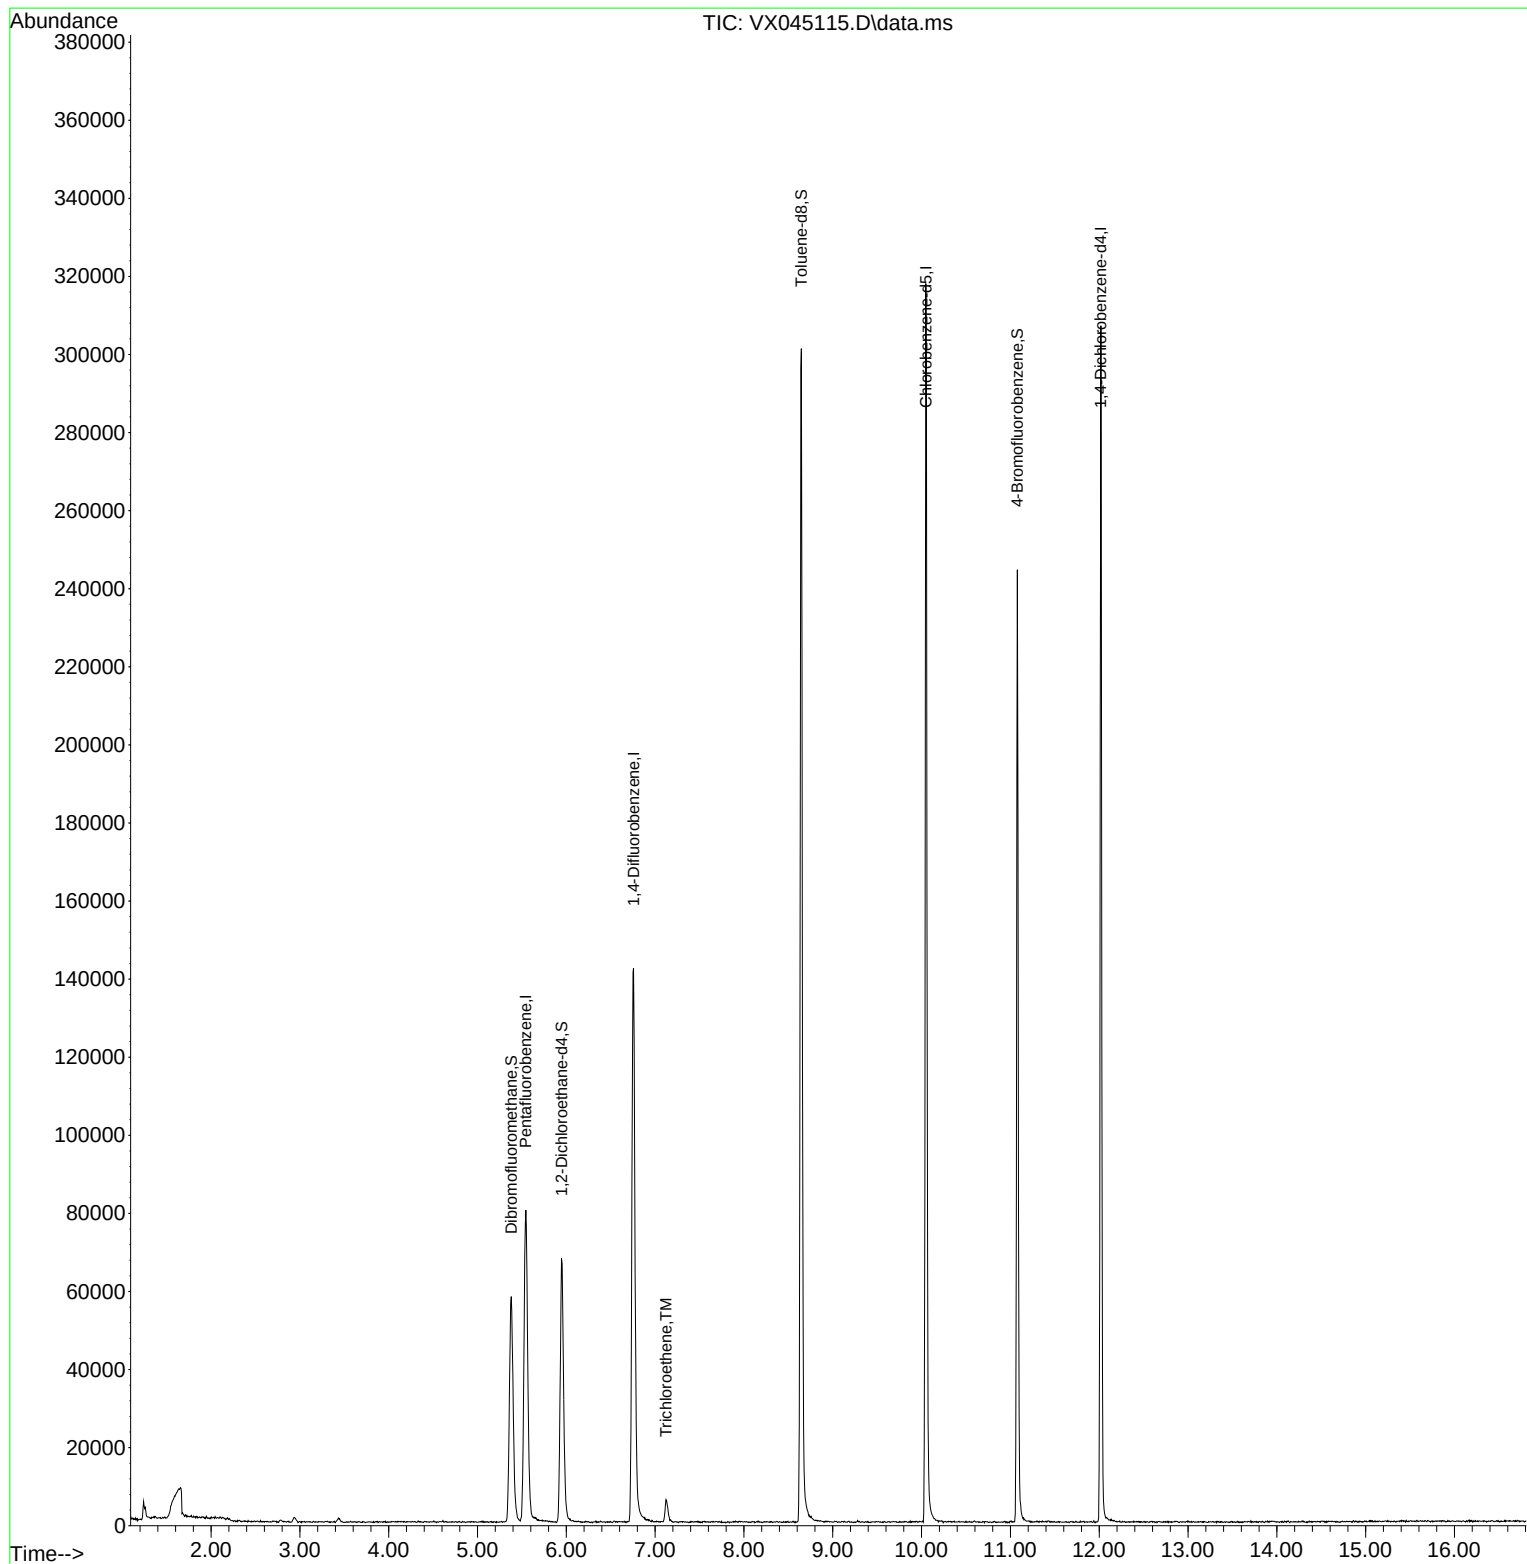


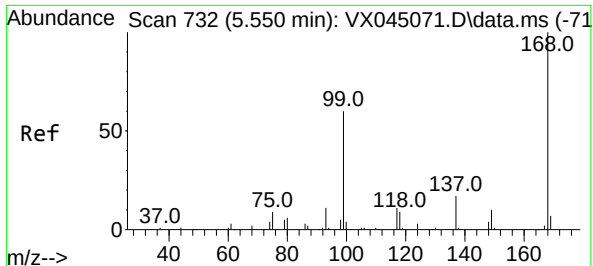

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX045115.D
Acq: 03 Mar 2025 16:03




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 75306
Ion Ratio Lower Upper
168 100
99 59.9 48.2 72.4

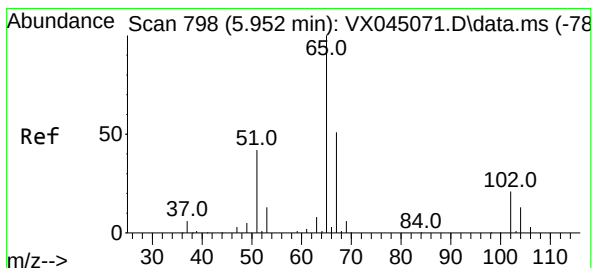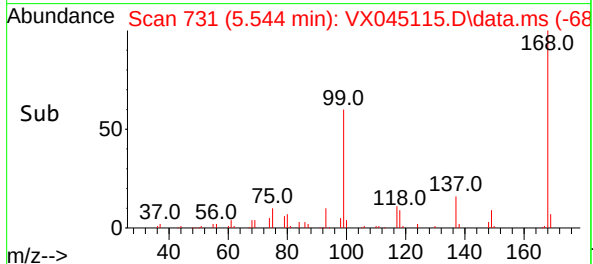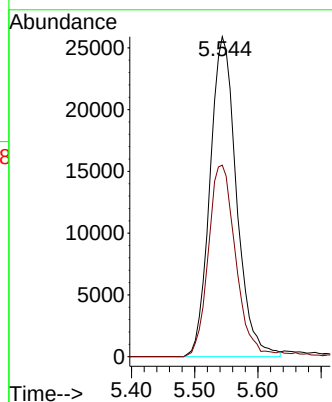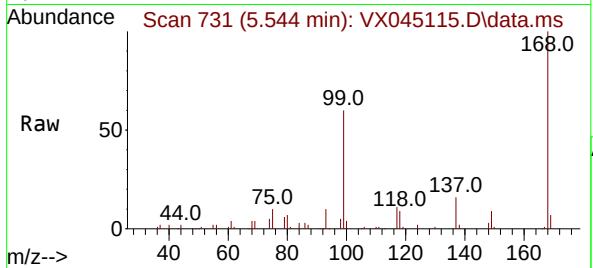

#33
1,2-Dichloroethane-d4
Concen: 51.880 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX045115.D
Acq: 03 Mar 2025 16:03

Tgt Ion: 65 Resp: 62144
Ion Ratio Lower Upper
65 100
67 53.1 0.0 106.2


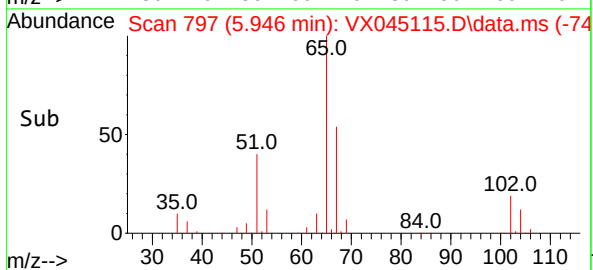
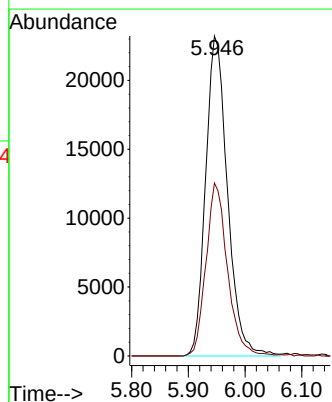
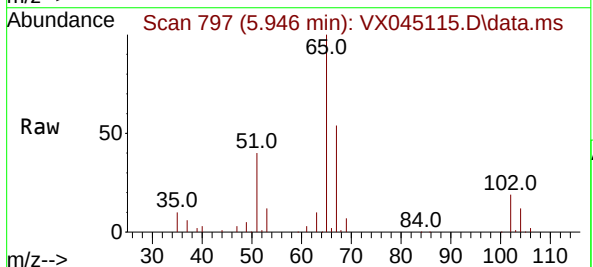


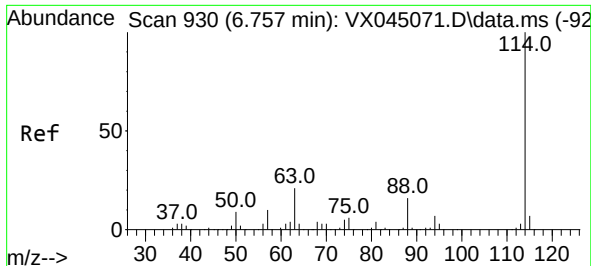

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX045115.D
Acq: 03 Mar 2025 16:03




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 150223
Ion Ratio Lower Upper
114 100
63 21.4 0.0 41.8
88 16.1 0.0 32.8

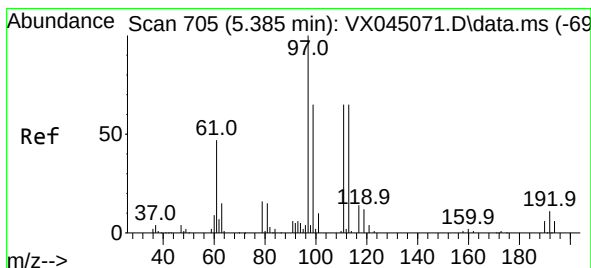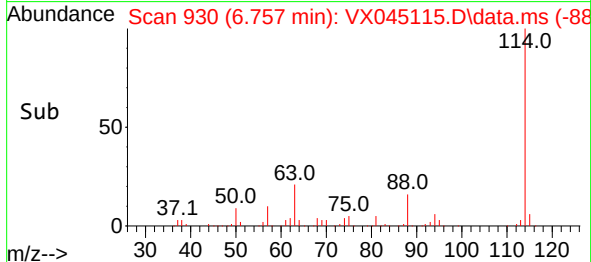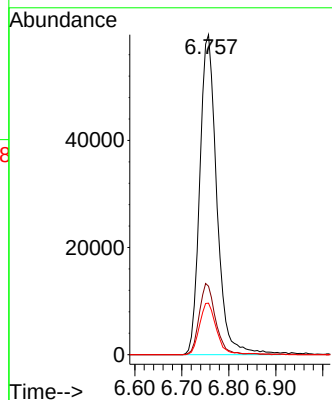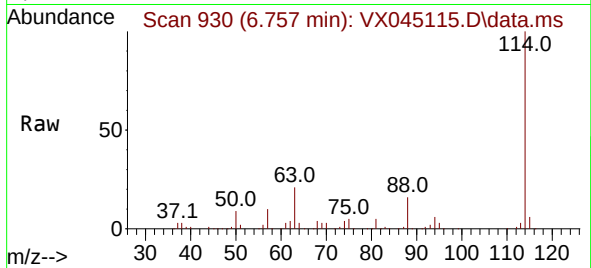

#35
Dibromofluoromethane
Concen: 51.057 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX045115.D
Acq: 03 Mar 2025 16:03

Tgt Ion:113 Resp: 51287
Ion Ratio Lower Upper
113 100
111 101.8 81.8 122.6
192 17.8 14.3 21.5


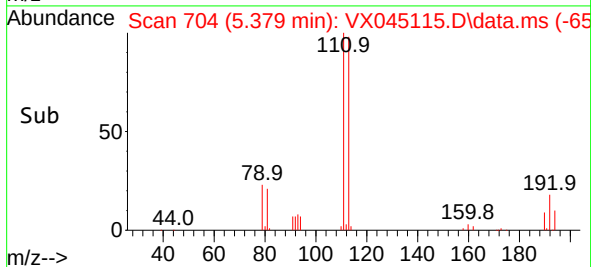
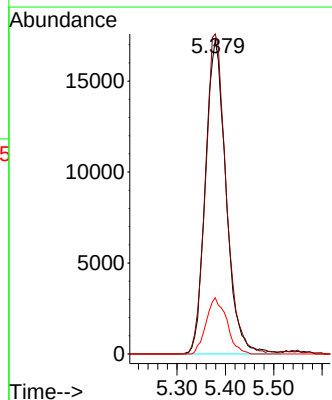
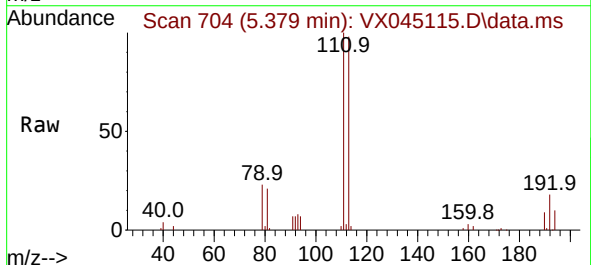


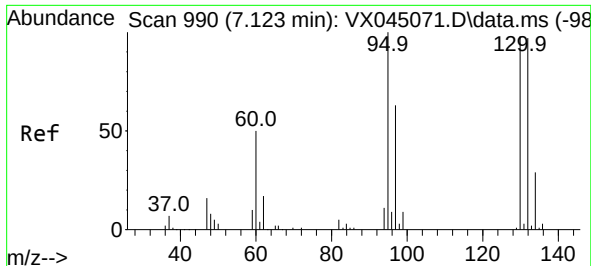

#44
 Trichloroethene
 Concen: 2.412 ug/l
 RT: 7.123 min Scan# 990
 Delta R.T. -0.000 min
 Lab File: VX045115.D
 Acq: 03 Mar 2025 16:03




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion:130 Resp: 2464
 Ion Ratio Lower Upper
 130 100
 95 99.5 0.0 205.0

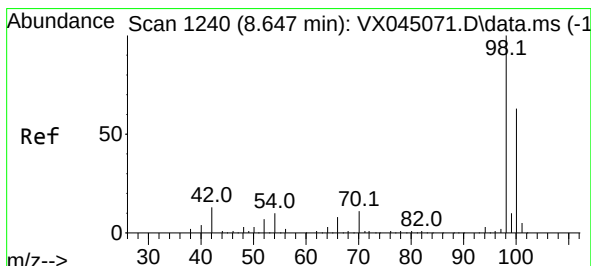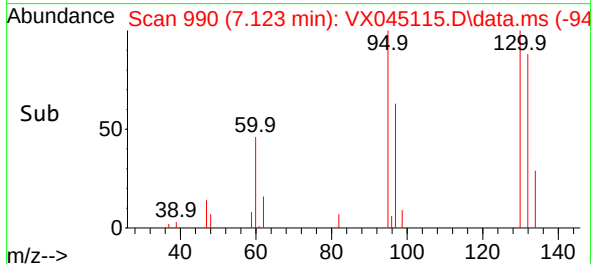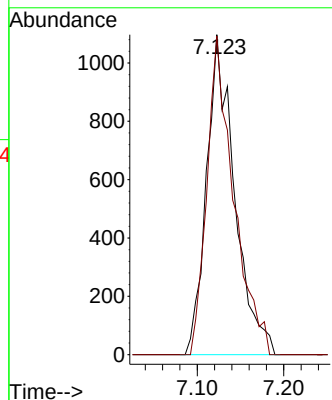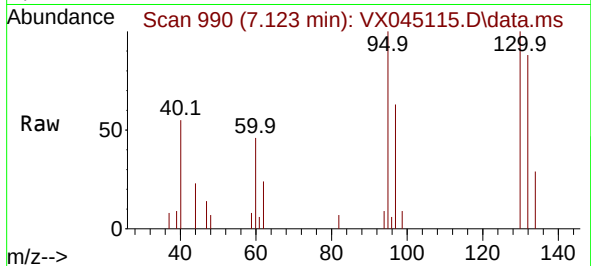

#50
 Toluene-d8
 Concen: 51.172 ug/l
 RT: 8.647 min Scan# 1240
 Delta R.T. -0.000 min
 Lab File: VX045115.D
 Acq: 03 Mar 2025 16:03

Tgt Ion: 98 Resp: 186352
 Ion Ratio Lower Upper
 98 100
 100 66.2 52.0 78.0


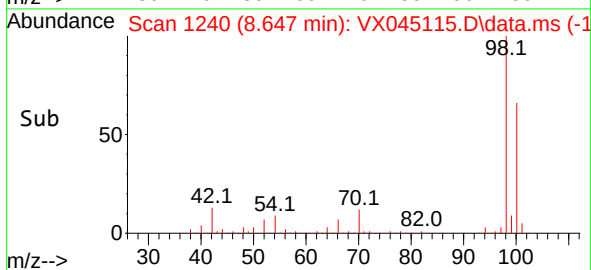
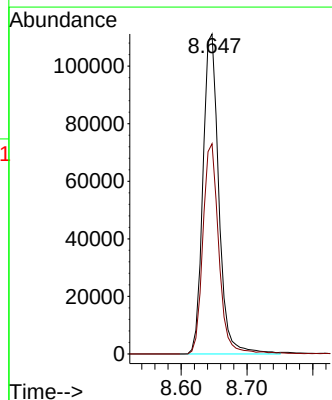
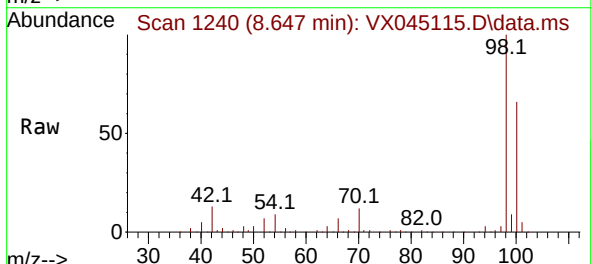


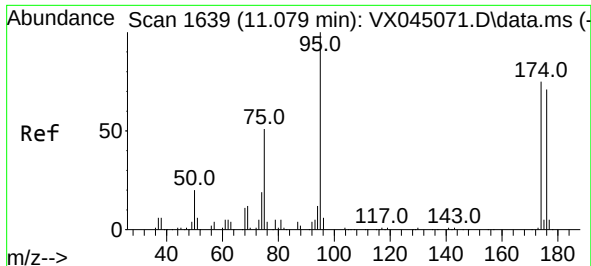

#62
4-Bromofluorobenzene
Concen: 52.957 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045115.D
Acq: 03 Mar 2025 16:03




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 95 Resp: 63905
Ion Ratio Lower Upper
95 100
174 74.0 0.0 148.2
176 71.3 0.0 141.4

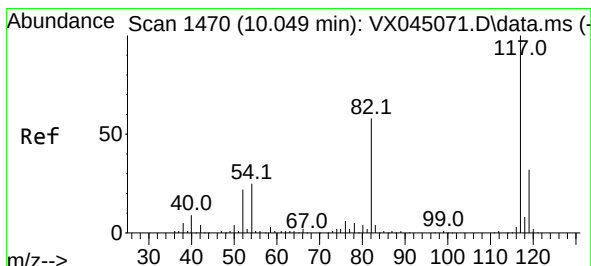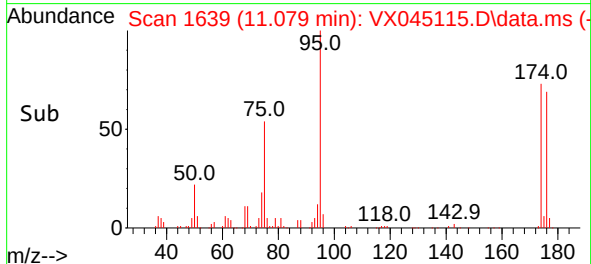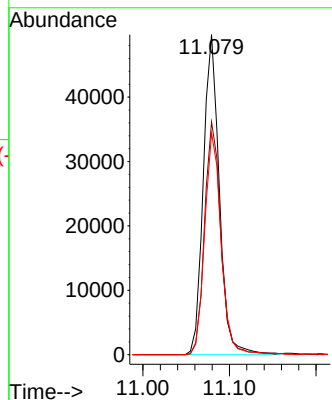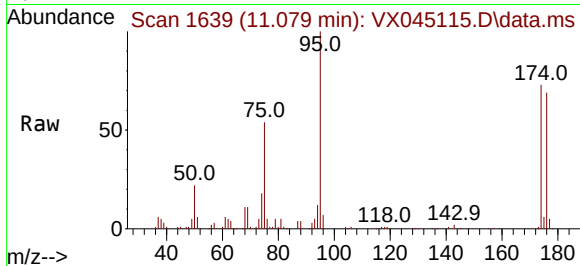

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX045115.D
Acq: 03 Mar 2025 16:03


Tgt Ion: 117 Resp: 138820
Ion Ratio Lower Upper
117 100
82 58.9 46.3 69.5
119 32.1 25.7 38.5

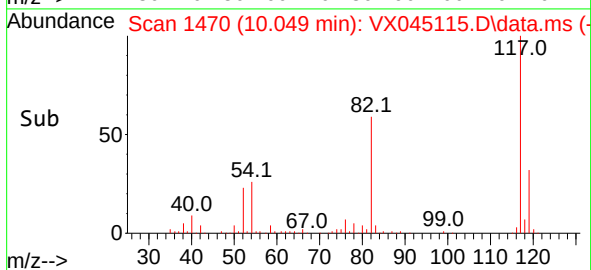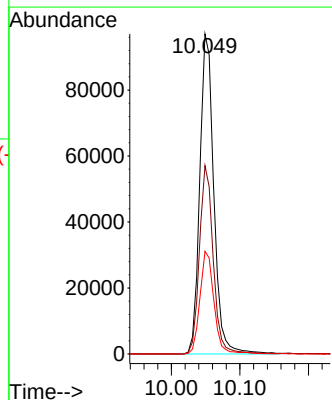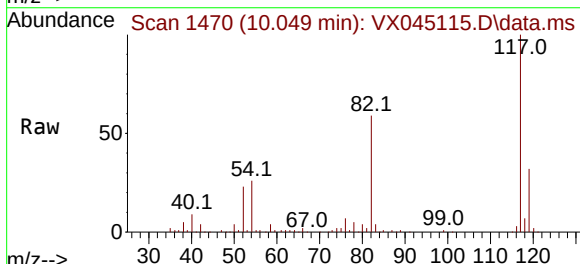

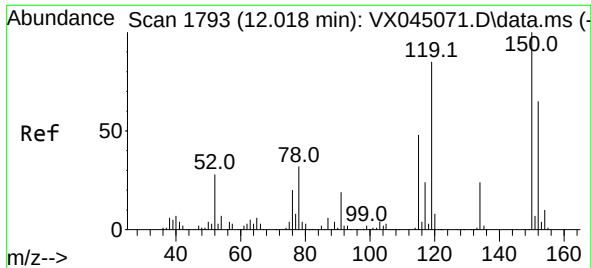

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX045115.D
 Acq: 03 Mar 2025 16:03

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

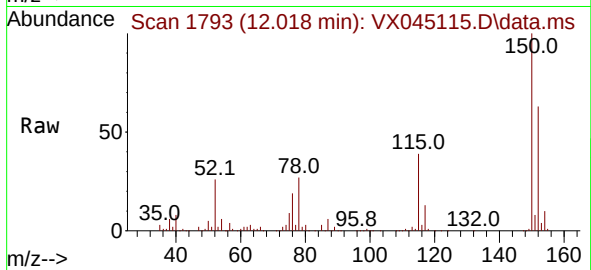

Tgt Ion:152	Resp:	58431
Ion	Ratio	Lower Upper
152	100	
115	62.1	44.2 132.6
150	159.1	0.0 349.0

