

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
Data File : VX045101.D
Acq On : 03 Mar 2025 09:16
Operator : JC/MD
Sample : VX0303MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0303MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M

Title : SW846 8260

Signal : TIC: VX045101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	21	25	31	rBV	11810	17175	3.03%	0.581%
2	1.593	69	83	85	rBV10	7088	23424	4.13%	0.792%
3	5.373	692	703	719	rBV	63924	192822	34.03%	6.522%
4	5.538	719	730	743	rBV3	90230	259403	45.78%	8.774%
5	5.940	786	796	814	rBV	73010	197991	34.94%	6.697%
6	6.751	921	929	948	rBV	159790	400562	70.69%	13.549%
7	8.641	1233	1239	1260	rBV	346883	566672	100.00%	19.168%
8	10.049	1464	1470	1486	rBV	354124	495423	87.43%	16.758%
9	11.079	1633	1639	1652	rBV	272044	359919	63.51%	12.174%
10	12.018	1788	1793	1806	rBV	355018	442992	78.17%	14.984%




Sum of corrected areas: 2956383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
Data File : VX045101.D
Acq On : 03 Mar 2025 09:16
Operator : JC/MD
Sample : VX0303MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0303MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

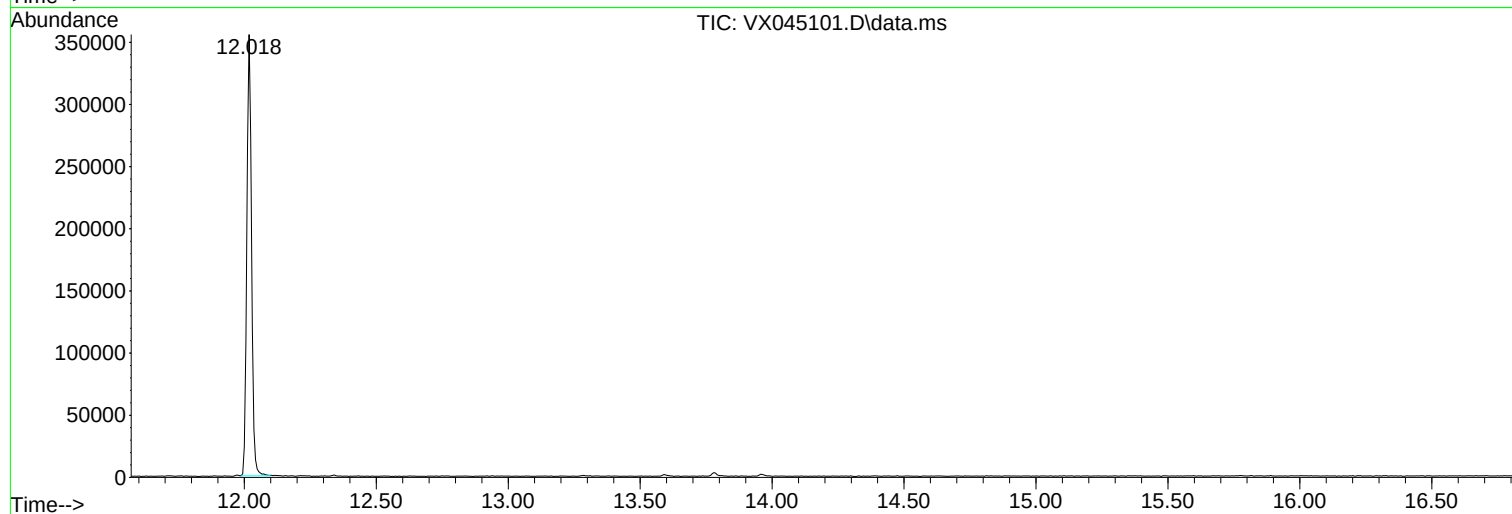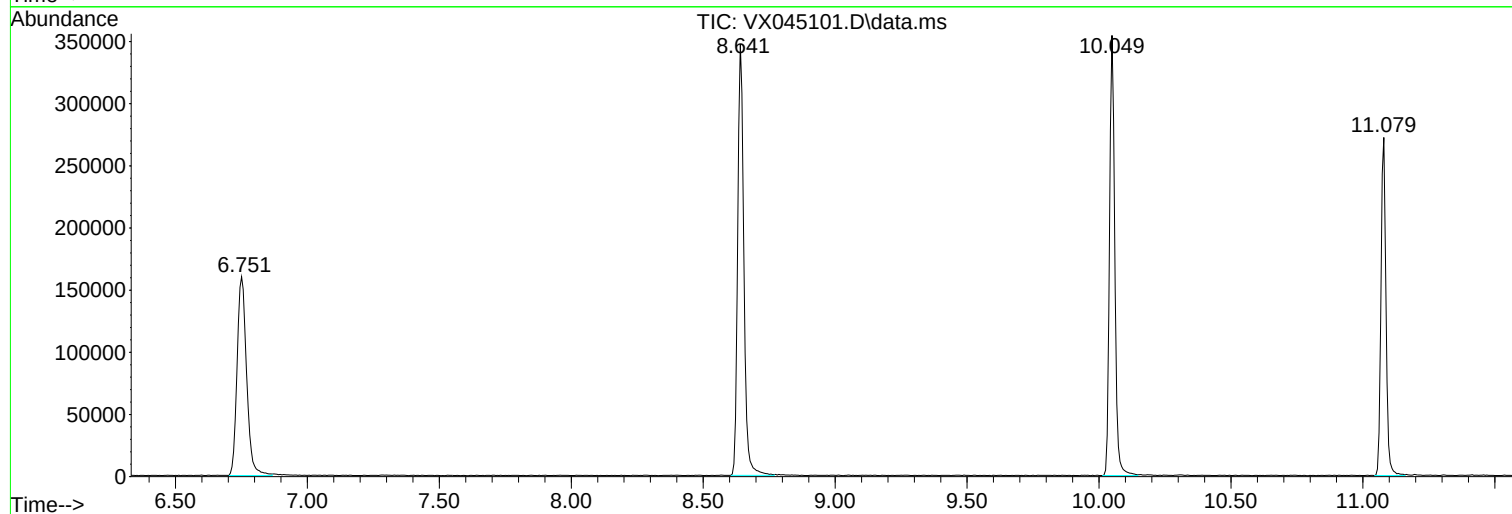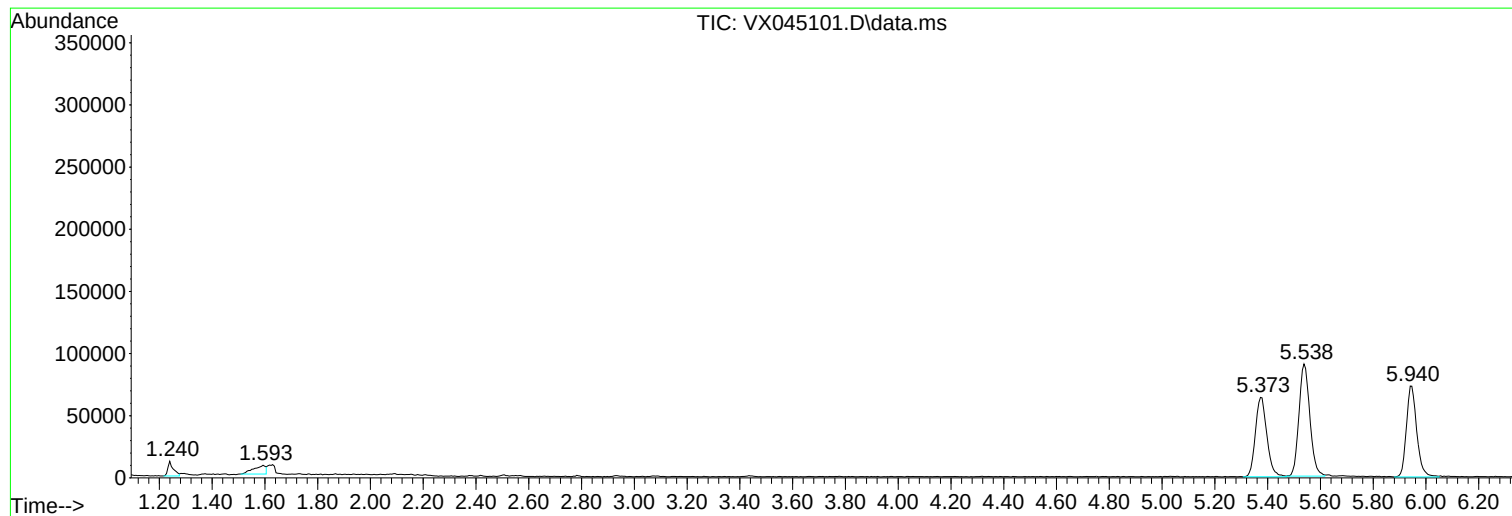

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
Data File : VX045101.D
Acq On : 03 Mar 2025 09:16
Operator : JC/MD
Sample : VX0303MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0303MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
Data File : VX045101.D
Acq On : 03 Mar 2025 09:16
Operator : JC/MD
Sample : VX0303MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0303MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc