

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
Data File : VX045115.D
Acq On : 03 Mar 2025 16:03
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M

Title : SW846 8260

Signal : TIC: VX045115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	21	25	32	rBV2	4614	8479	1.66%	0.321%
2	1.636	68	90	91	rBV9	7405	36436	7.15%	1.379%
3	5.379	694	704	721	rBV	57522	167954	32.97%	6.356%
4	5.544	721	731	744	rBV2	79674	230821	45.31%	8.735%
5	5.946	787	797	815	rBV	67675	180336	35.40%	6.824%
6	6.757	921	930	953	rBV	141776	357212	70.13%	13.517%
7	7.123	984	990	997	rBV5	5684	12481	2.45%	0.472%
8	8.647	1233	1240	1257	rBV	300516	509388	100.00%	19.276%
9	10.049	1465	1470	1489	rBV	317283	448895	88.12%	16.987%
10	11.079	1634	1639	1655	rBV	243871	315372	61.91%	11.934%
11	12.018	1788	1793	1802	rBV	306253	375220	73.66%	14.199%




Sum of corrected areas: 2642594

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
Data File : VX045115.D
Acq On : 03 Mar 2025 16:03
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

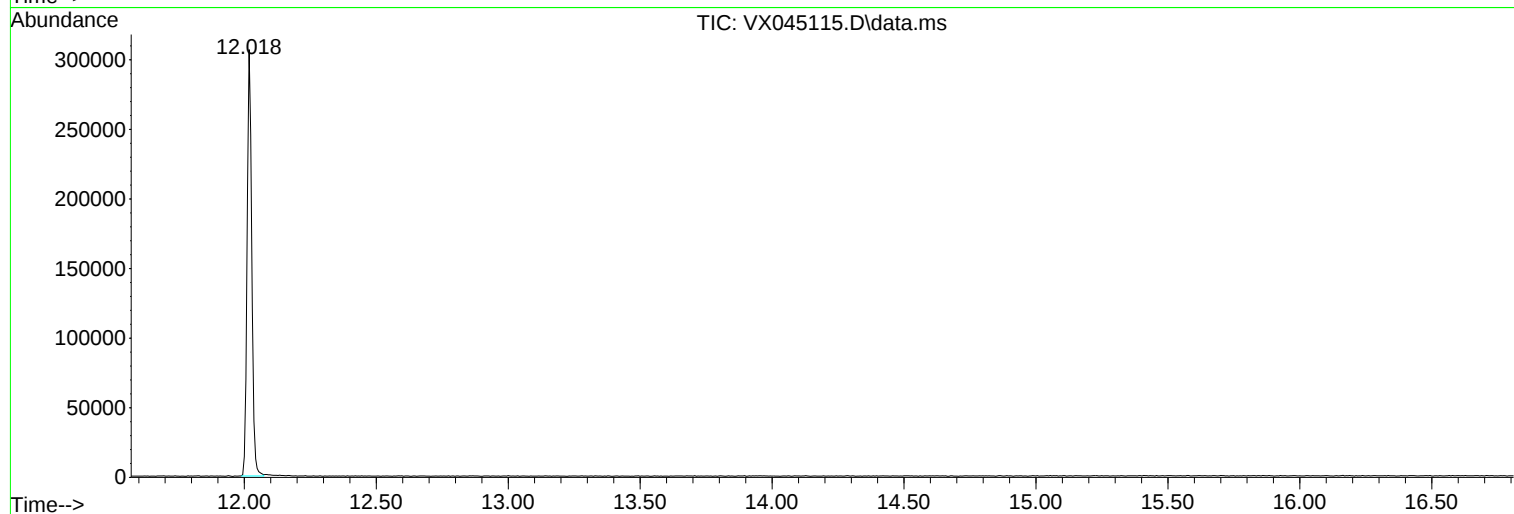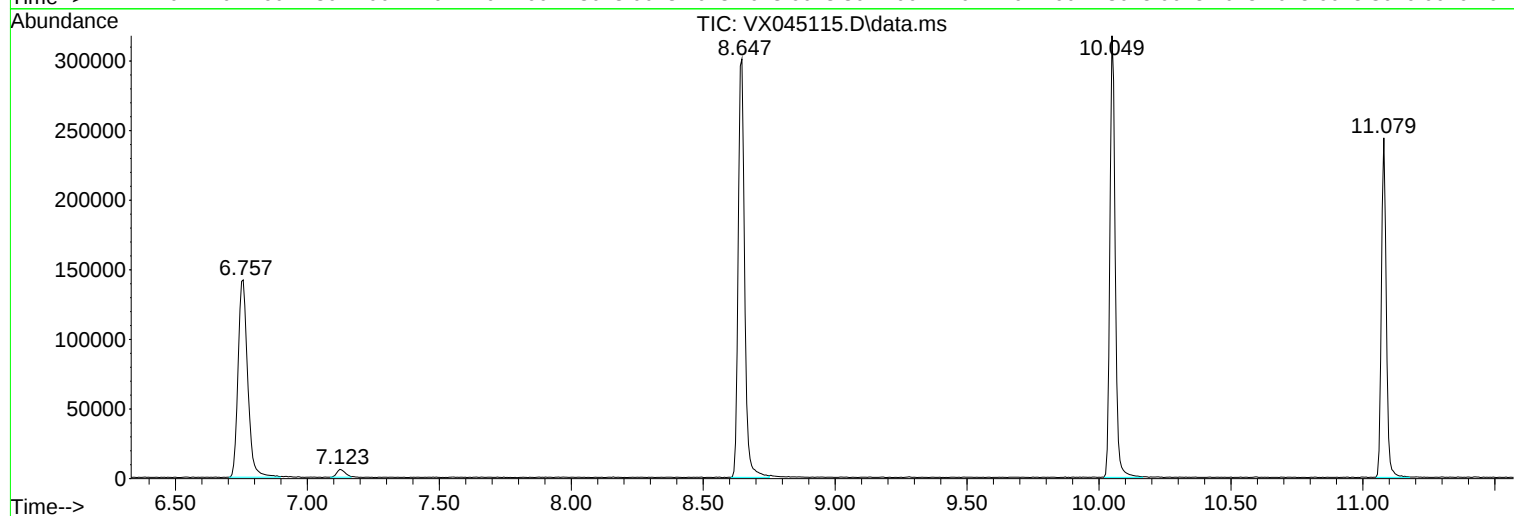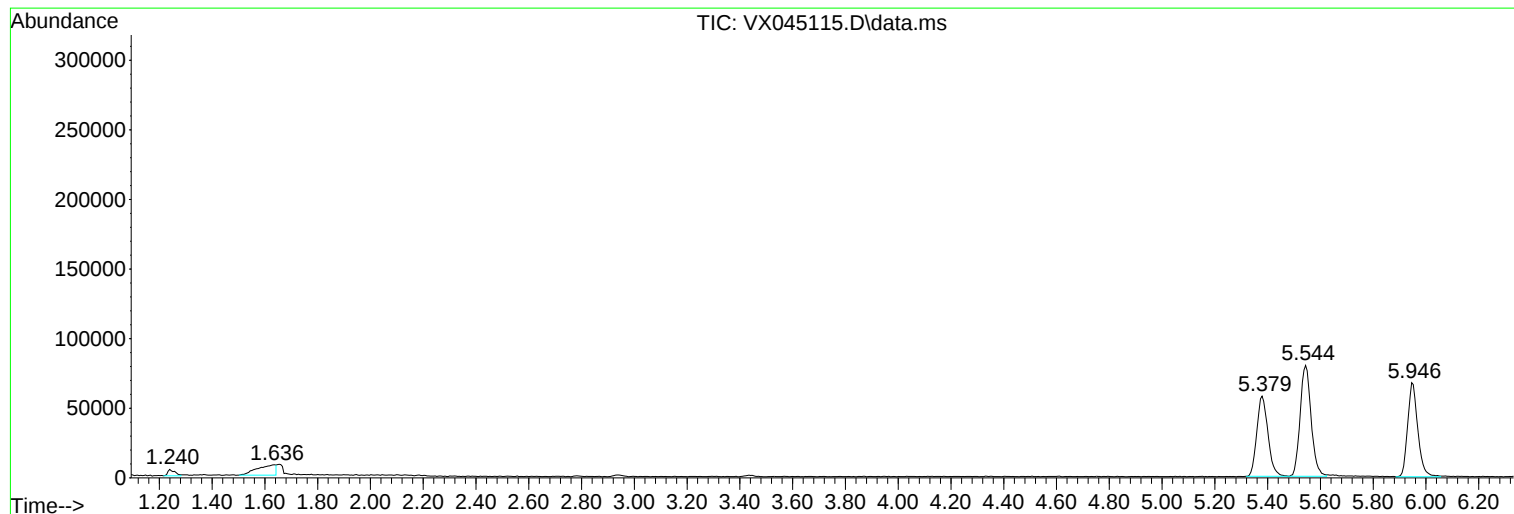

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
Data File : VX045115.D
Acq On : 03 Mar 2025 16:03
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.636 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
1.636	7.89 ug/l	36436	Pentafluorobenzene	5.544	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Dimethyl Sulfoxide	78	C2H6OS	000067-68-5	10
2	Ethylamine	45	C2H7N	000075-04-7	5
3	2-Chloroethyl methyl sulfone	142	C3H7ClO2S	050890-51-2	4
4	(S)-(-)-2-Chloropropionic acid	108	C3H5ClO2	029617-66-1	4
5	Boron trifluoride etherate	142	C4H10BF3O	000109-63-7	4

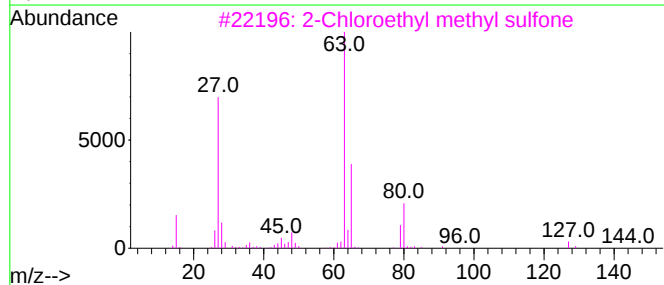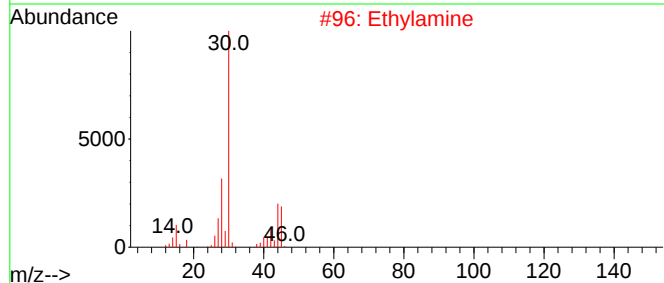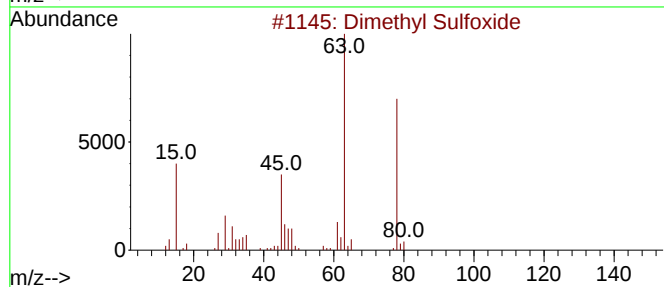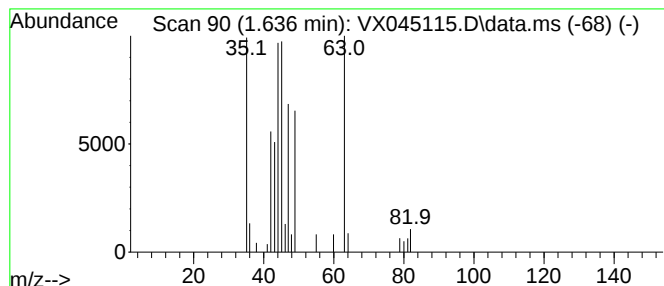

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030325\
Data File : VX045115.D
Acq On : 03 Mar 2025 16:03
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.636	1.636	7.9	ug/l	36436	1	5.544	230821	50.0