

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX030419\
 Data File : VX007811.D
 Acq On : 04 Mar 2019 15:28
 Operator : JC/SP
 Sample : K1719-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB201-TB-20190227

Quant Time: Mar 04 22:11:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X022519W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 26 01:53:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	355970	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	546932	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	512737	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	246994	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	188007	42.64	ug/l	0.00
Spiked Amount			Recovery	=	85.28%	
35) Dibromofluoromethane	5.51	113	173673	47.50	ug/l	0.00
Spiked Amount			Recovery	=	95.00%	
50) Toluene-d8	8.71	98	656855	46.93	ug/l	0.00
Spiked Amount			Recovery	=	93.86%	
62) 4-Bromofluorobenzene	11.13	95	241560	47.02	ug/l	0.00
Spiked Amount			Recovery	=	94.04%	


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX030419\
Data File : VX007811.D
Acq On : 04 Mar 2019 15:28
Operator : JC/SP
Sample : K1719-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB201-TB-20190227

Quant Time: Mar 04 22:11:22 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X022519W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 26 01:53:13 2019
Response via : Initial Calibration

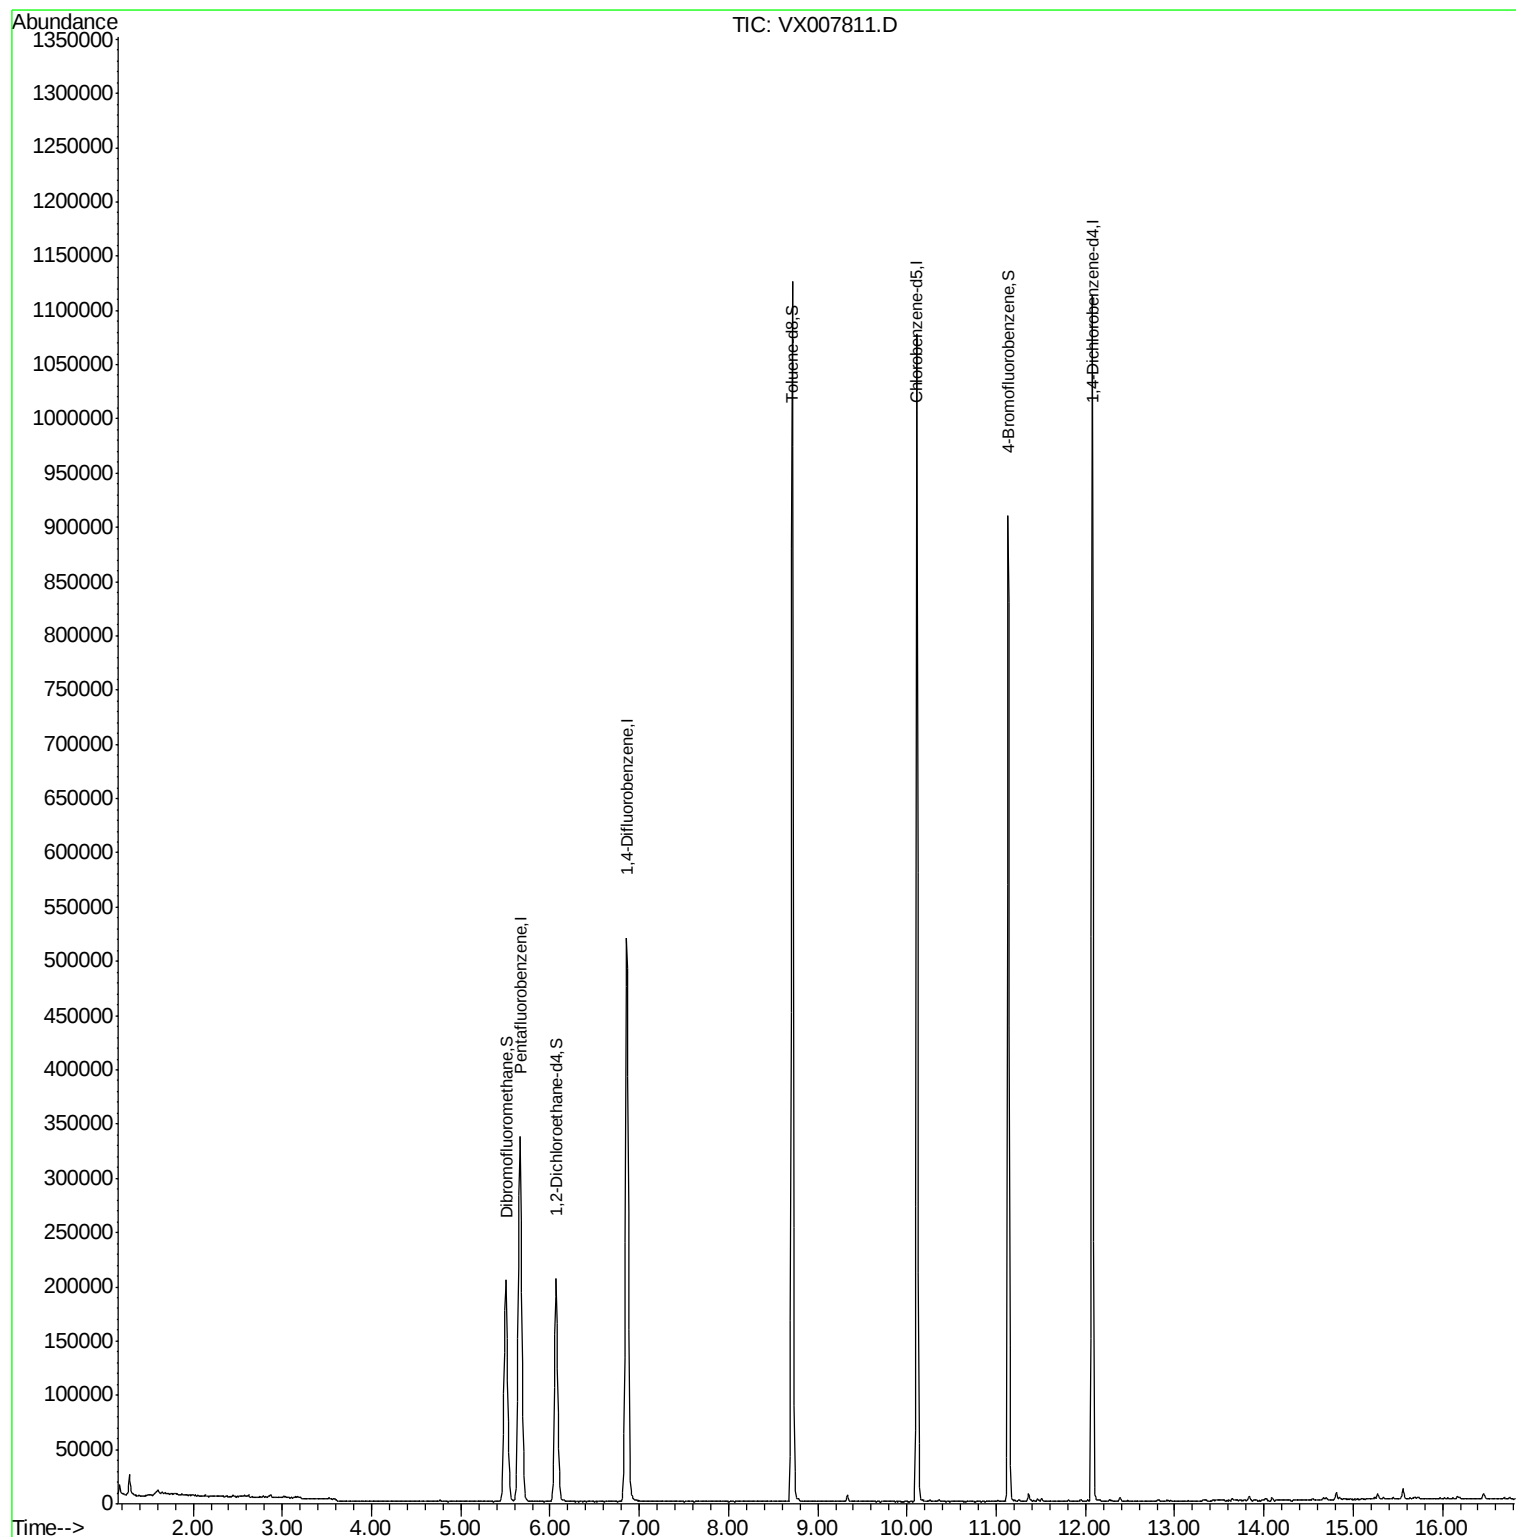



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX007811.D

Acq: 04 Mar 2019 15:28

Instrument :

MSVOA_X

ClientSampleId :


BP-VPB201-TB-20190227

Tot Ion:168 Resp: 355970

Ion Ratio Lower Upper

168 100

99 46.9 37.9 56.9

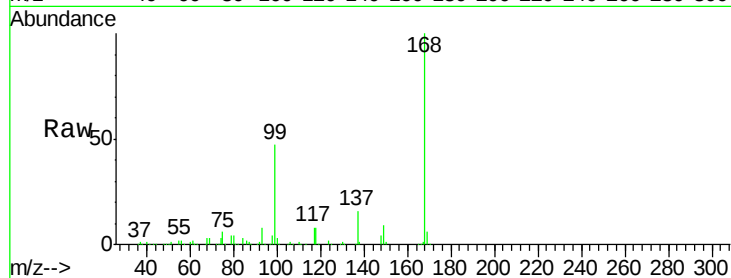

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67



150000

100000

50000

0

Time--> 5.50 5.60 5.70 5.80

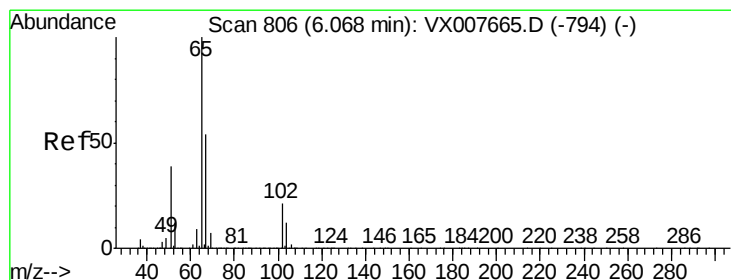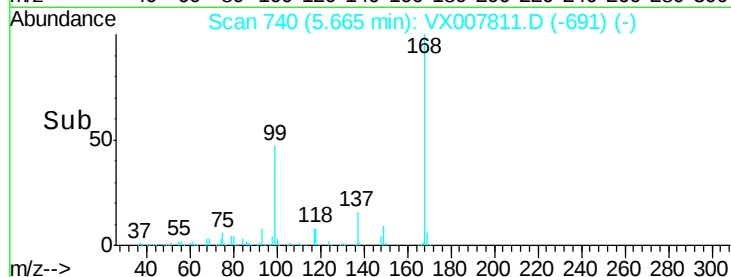

#33

1,2-Dichloroethane-d4

Concen: 42.638 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX007811.D


Acq: 04 Mar 2019 15:28

Tgt Ion: 65 Resp: 188007

Ion Ratio Lower Upper

65 100

67 55.5 0.0 108.8

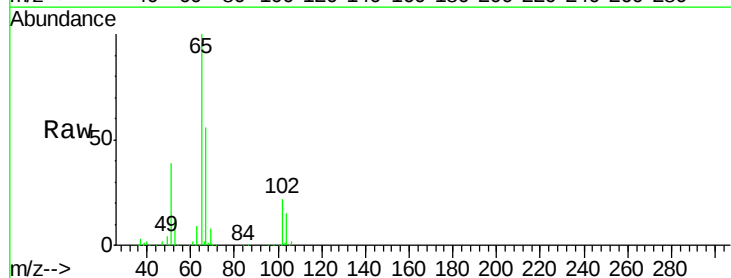

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

80000


60000


40000

20000

0

Time--> 6.00 6.10 6.20

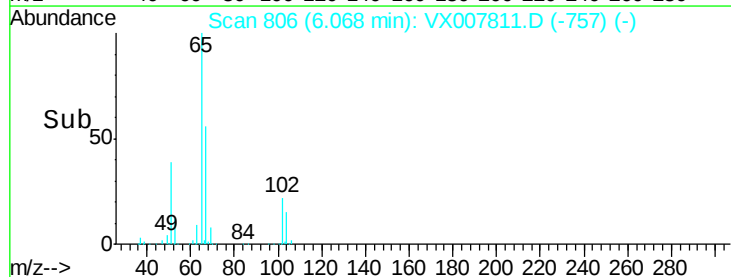

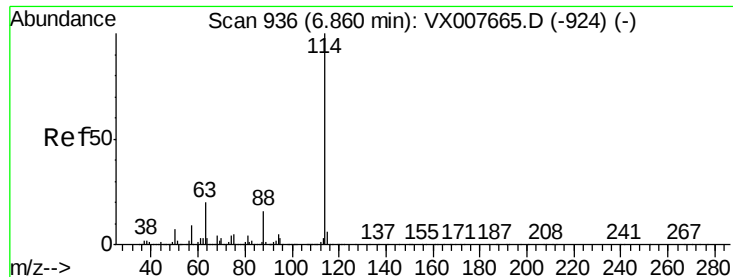

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX007811.D

Acq: 04 Mar 2019 15:28

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB201-TB-20190227


Tot Ion:114 Resp: 546932

Ion Ratio Lower Upper

114 100

63 19.7 0.0 35.6




88 15.3 0.0 29.6

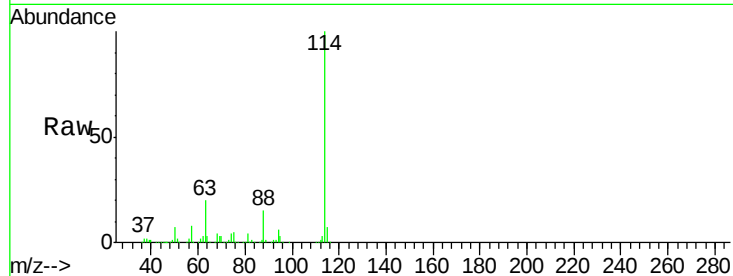

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

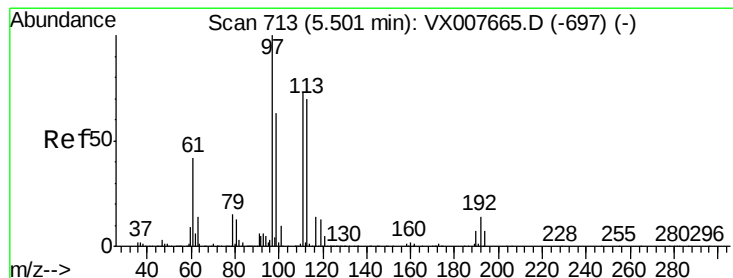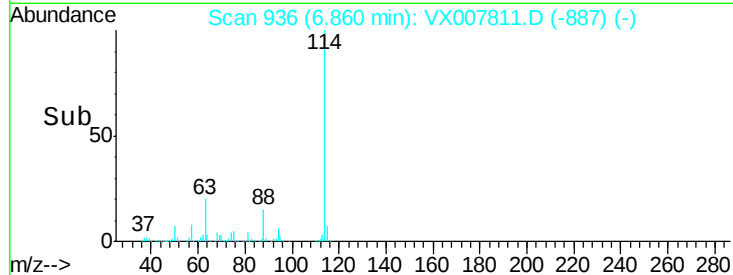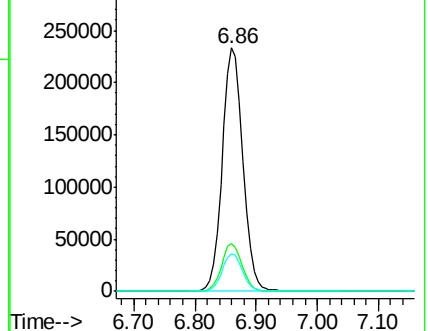

#35

Dibromofluoromethane

Concen: 47.503 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX007811.D

Acq: 04 Mar 2019 15:28


Tgt Ion:113 Resp: 173673

Ion Ratio Lower Upper

113 100

111 103.3 81.8 122.8



192 24.7 18.5 27.7

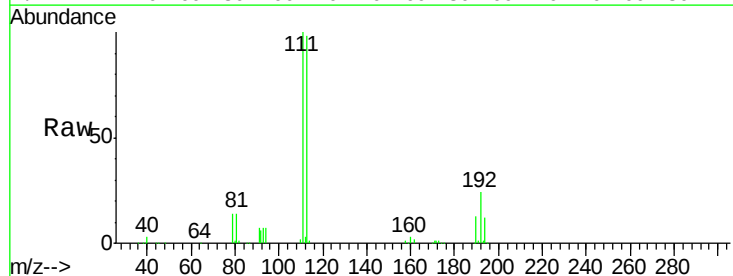

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



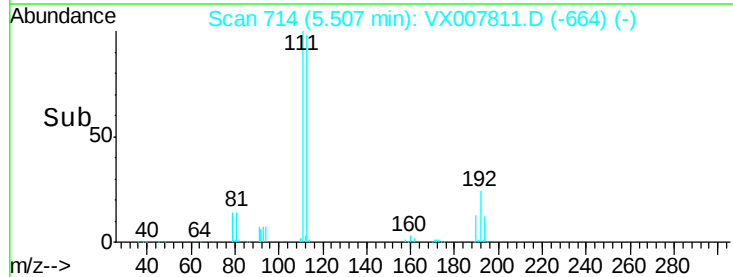
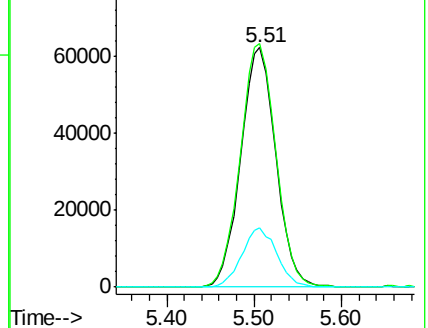




#50
Toluene-d8
Concen: 46.929 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. 0.00 min
Lab File: VX007811.D
Acq: 04 Mar 2019 15:28




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB201-TB-20190227


Tot Ion: 98 Resp: 656855
Ion Ratio Lower Upper
98 100
100 65.3 51.6 77.4

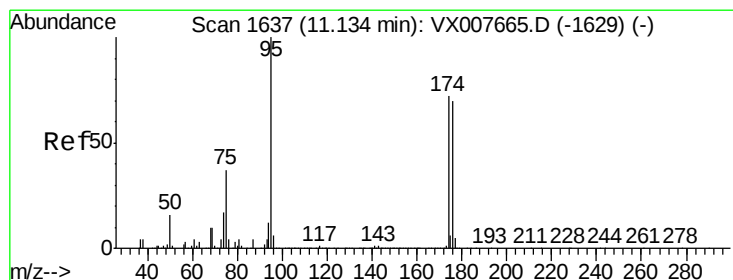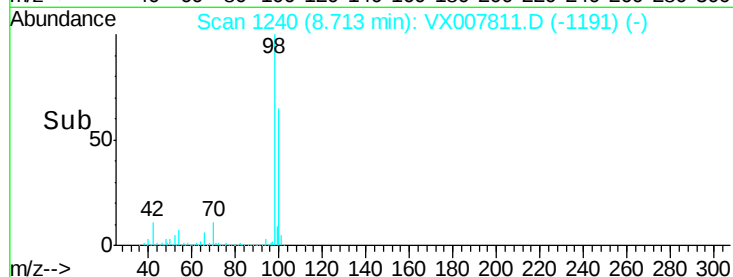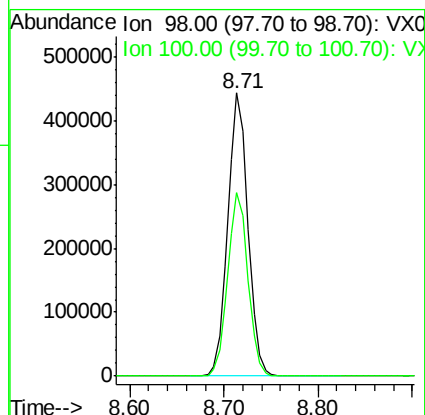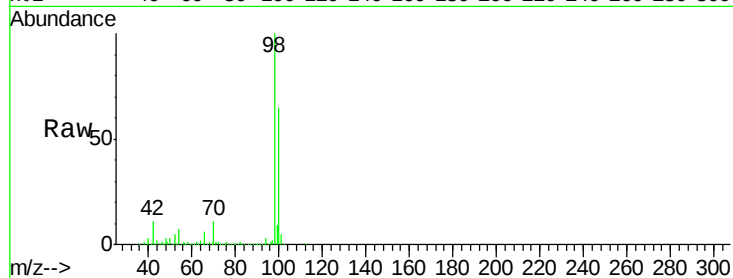

#62
4-Bromofluorobenzene
Concen: 47.020 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.00 min
Lab File: VX007811.D
Acq: 04 Mar 2019 15:28

Tgt Ion: 95 Resp: 241560
Ion Ratio Lower Upper
95 100
174 92.5 0.0 189.2
176 89.6 0.0 186.2

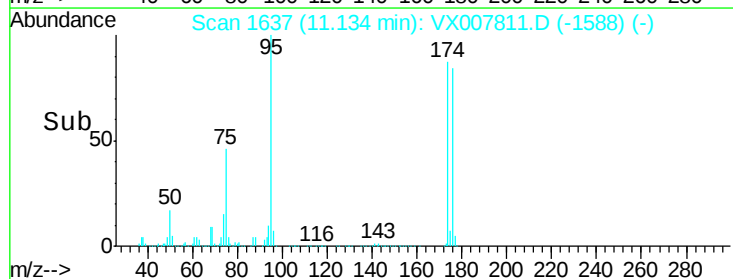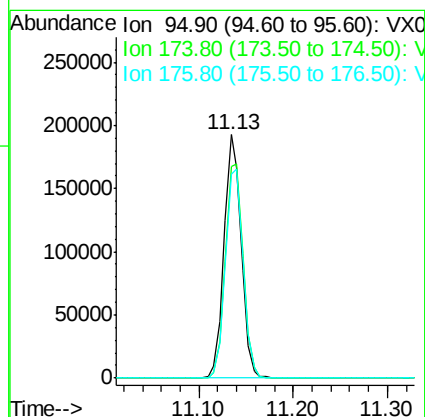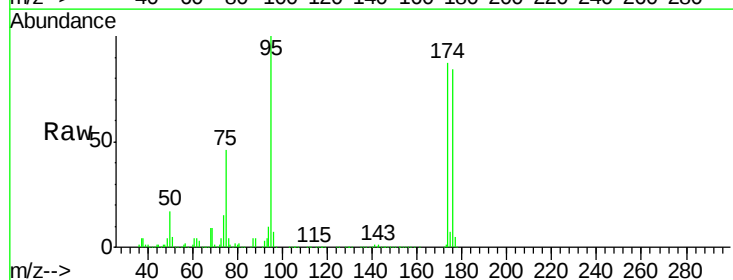

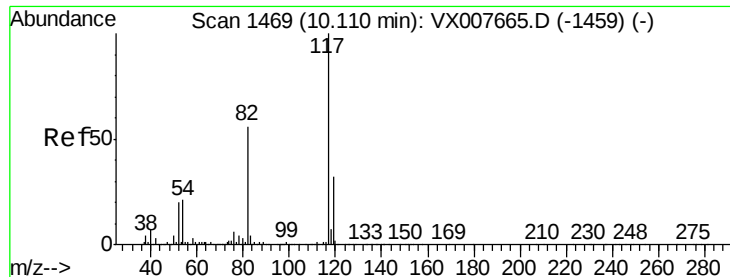

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VX007811.D

Acq: 04 Mar 2019 15:28

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB201-TB-20190227


Tot Ion:117 Resp: 512737

Ion Ratio Lower Upper

117 100

82 55.0 42.1 63.1




119 32.1 26.5 39.7

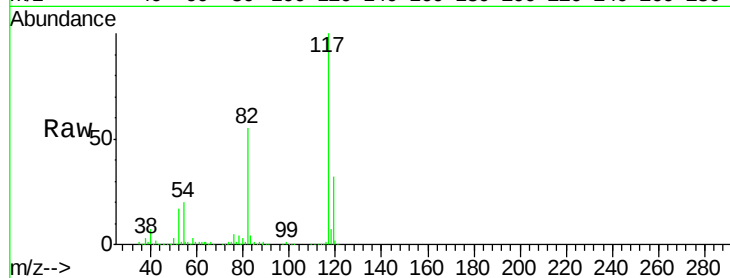

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

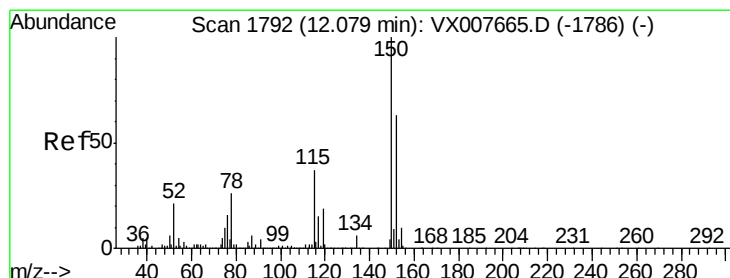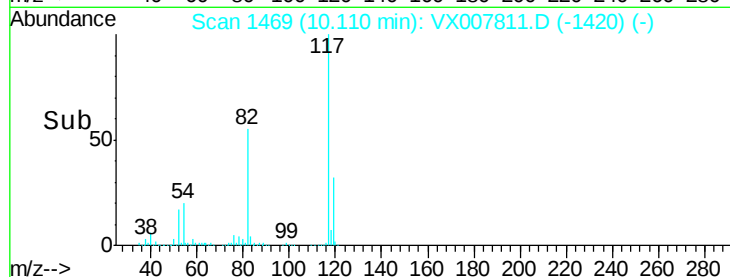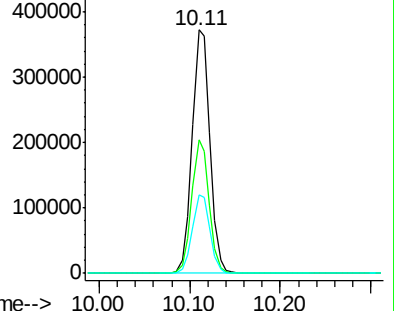

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX007811.D

Acq: 04 Mar 2019 15:28


Tgt Ion:152 Resp: 246994

Ion Ratio Lower Upper

152 100

115 54.5 38.0 114.0

150 155.1 0.0 346.4

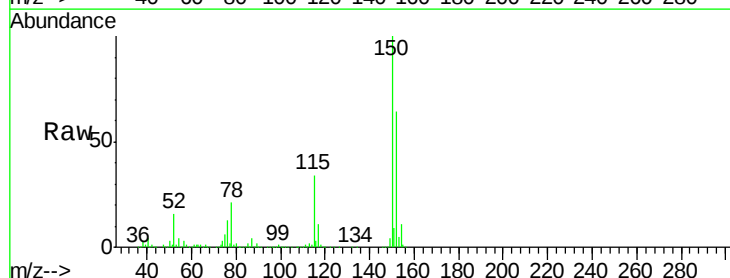

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

