


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX030419\
Data File : VX007803.D
Acq On : 04 Mar 2019 10:07
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X022519W.M
Title : SW846 8260
Last Update : Tue Feb 26 01:53:13 2019

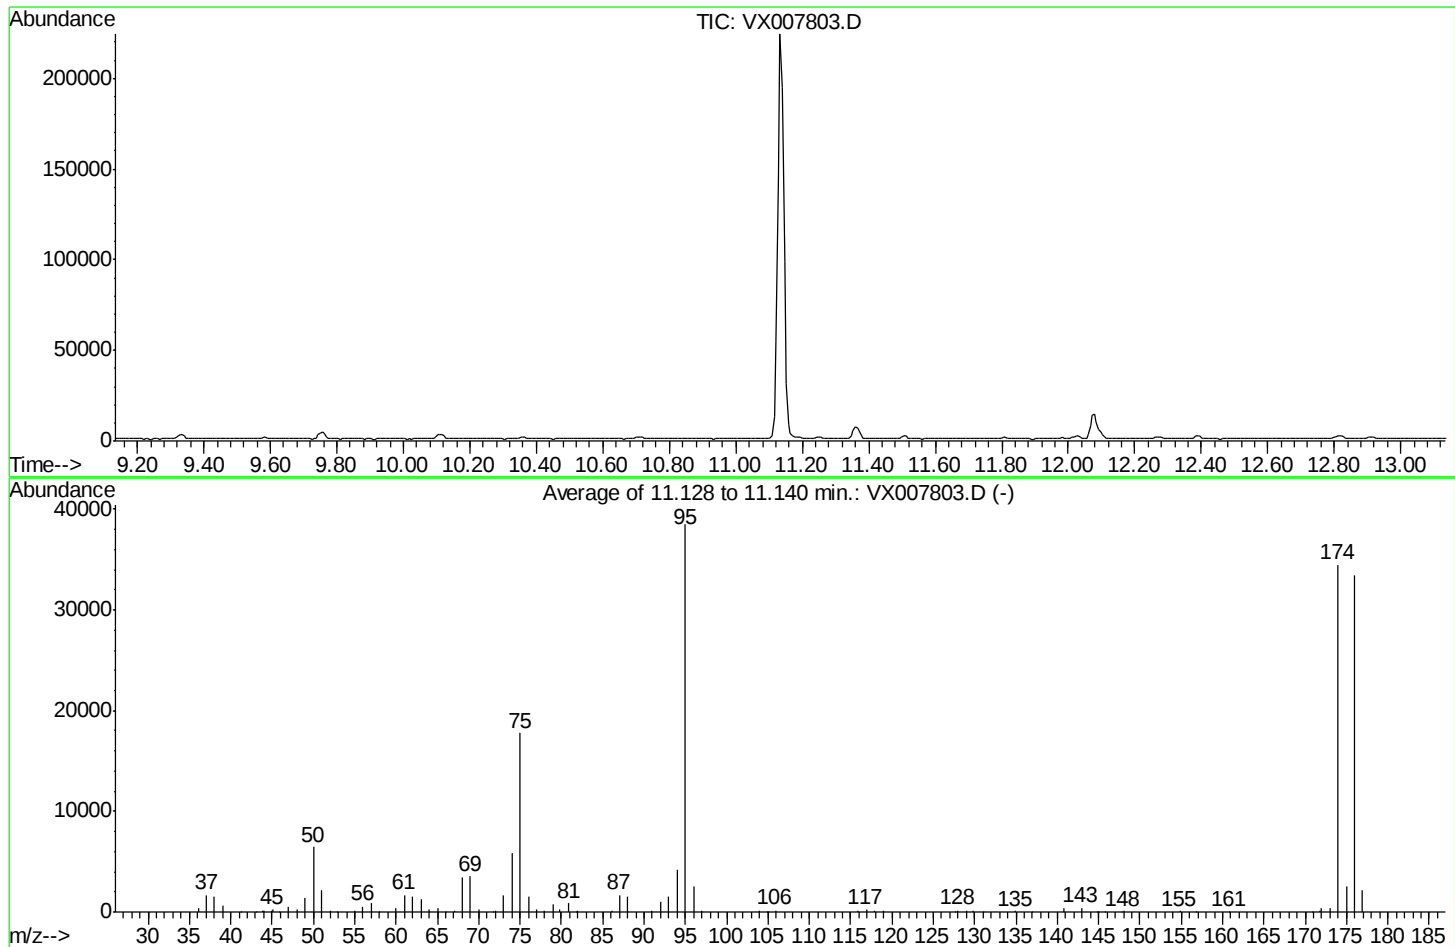

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	6452	PASS
75	95	30	60	46.2	17783	PASS
95	95	100	100	100.0	38501	PASS
96	95	5	9	6.5	2503	PASS
173	174	0.00	2	1.2	402	PASS
174	95	50	100	89.6	34504	PASS
175	174	5	9	7.4	2563	PASS
176	174	95	101	96.7	33378	PASS
177	176	5	9	6.6	2202	PASS