

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
 Data File : VX020975.D
 Acq On : 02 Mar 2021 19:28
 Operator : JC/MD
 Sample : M1545-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-725

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M

Title : SW846 8260

Signal : TIC: VX020975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.287	28	34	38	rBV4	11380	19677	1.76%	0.330%
2	5.464	732	744	758	rBV2	123461	354321	31.66%	5.943%
3	5.629	761	772	789	rBV	196298	556054	49.68%	9.326%
4	6.029	828	840	855	rBV	132863	350541	31.32%	5.879%
5	6.829	965	976	996	rBV	332487	787741	70.38%	13.212%
6	8.694	1286	1293	1317	rBV	690353	1119255	100.00%	18.773%
7	10.094	1525	1531	1549	rBV	727447	993157	88.73%	16.658%
8	10.341	1568	1573	1578	rBV	8985	11986	1.07%	0.201%
9	11.118	1699	1705	1719	rVB	593245	772598	69.03%	12.958%
10	12.059	1859	1865	1873	rBV	762756	925738	82.71%	15.527%
11	12.283	1896	1903	1908	rBV	41477	51484	4.60%	0.864%
12	13.818	2159	2164	2169	rBV	15540	19555	1.75%	0.328%




Sum of corrected areas: 5962107

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
Data File : VX020975.D
Acq On : 02 Mar 2021 19:28
Operator : JC/MD
Sample : M1545-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-725

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

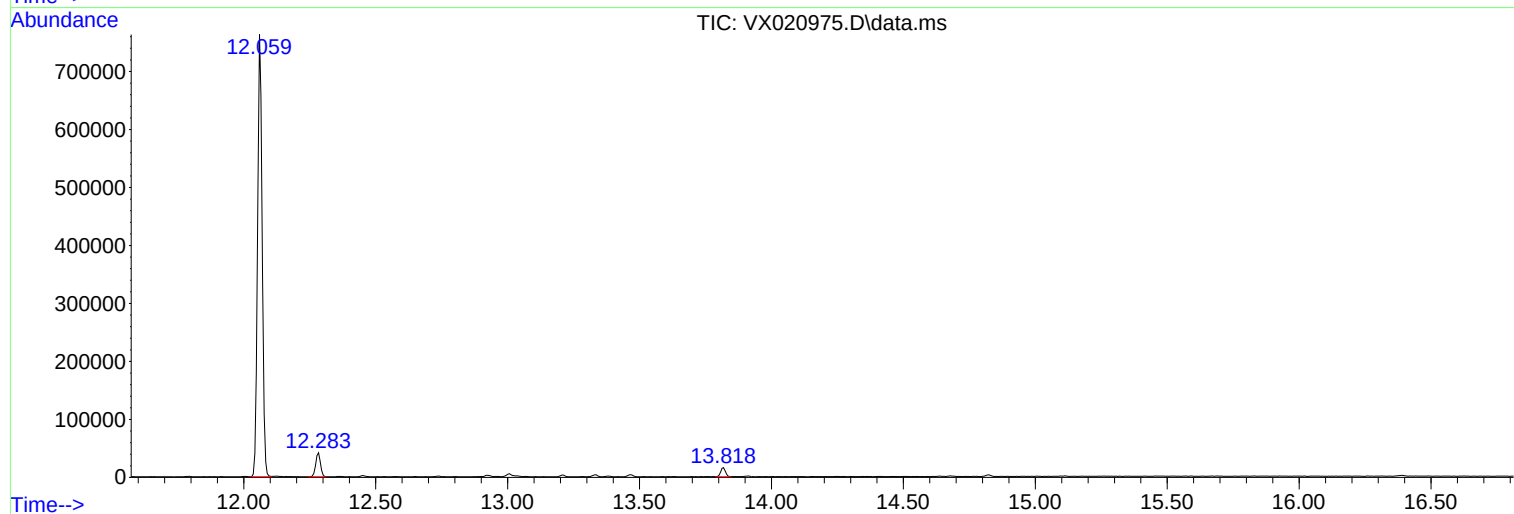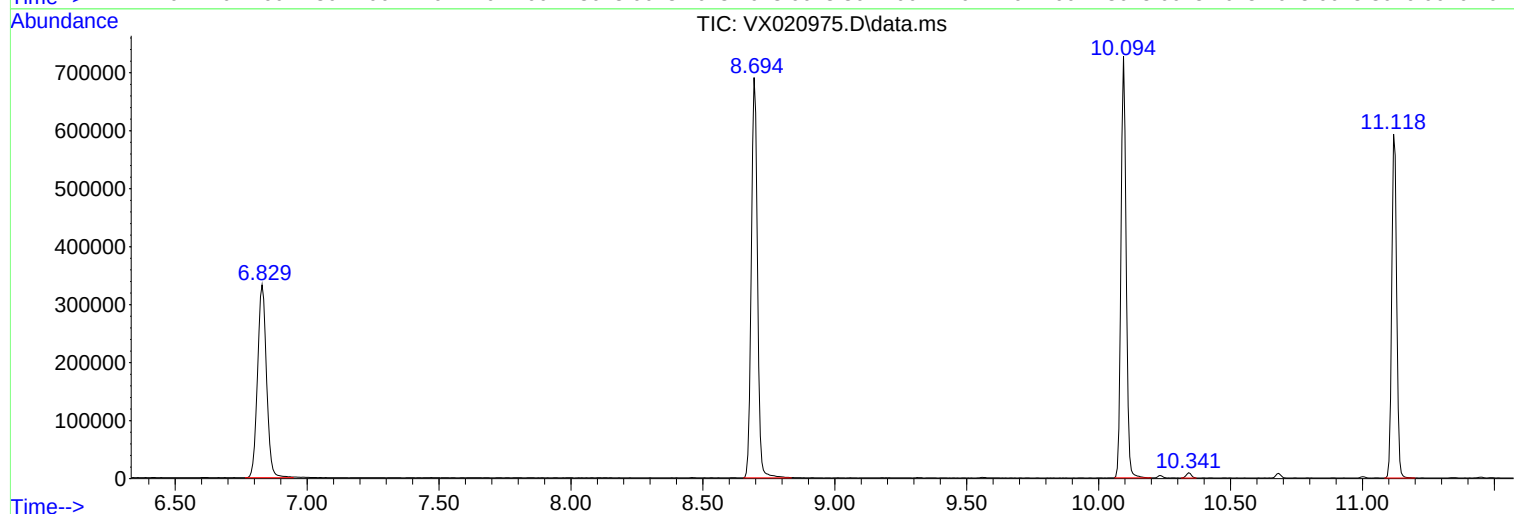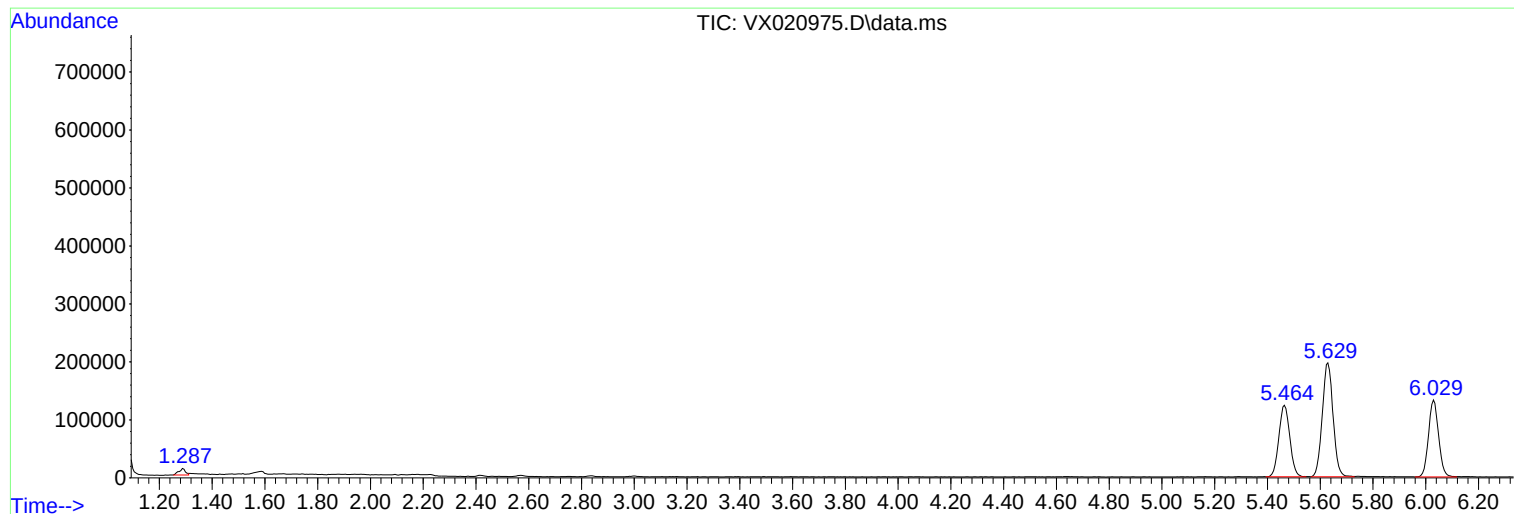

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
Data File : VX020975.D
Acq On : 02 Mar 2021 19:28
Operator : JC/MD
Sample : M1545-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-725

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
Data File : VX020975.D
Acq On : 02 Mar 2021 19:28
Operator : JC/MD
Sample : M1545-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-725

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------