

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
 Data File : VX020980.D
 Acq On : 02 Mar 2021 21:23
 Operator : JC/MD
 Sample : M1545-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RIM-7.55

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M

Title : SW846 8260

Signal : TIC: VX020980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.293	28	35	41	rBV2	71406	89351	7.53%	1.396%
2	2.416	220	226	232	rBV	9623	16437	1.39%	0.257%
3	2.569	246	252	262	rBV	7608	14766	1.24%	0.231%
4	5.464	733	744	758	rVB	131757	374098	31.54%	5.847%
5	5.629	760	772	789	rBV2	206783	580026	48.89%	9.065%
6	6.029	829	840	858	rBV	141242	370716	31.25%	5.794%
7	6.829	965	976	996	rBV	357046	838391	70.67%	13.103%
8	8.694	1286	1293	1304	rBV	767958	1186273	100.00%	18.540%
9	10.094	1525	1531	1545	rBV	784540	1062073	89.53%	16.598%
10	11.000	1680	1685	1691	rBV	36725	46698	3.94%	0.730%
11	11.117	1699	1705	1716	rBV	612465	789242	66.53%	12.335%
12	11.923	1837	1842	1849	rBV3	21089	29341	2.47%	0.459%
13	12.059	1859	1865	1873	rBV	758418	946500	79.79%	14.792%
14	12.141	1873	1879	1886	rBV3	27198	41326	3.48%	0.646%
15	12.812	1988	1993	1998	rBV	9488	13382	1.13%	0.209%




Sum of corrected areas: 6398620

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
Data File : VX020980.D
Acq On : 02 Mar 2021 21:23
Operator : JC/MD
Sample : M1545-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RIM-7.55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

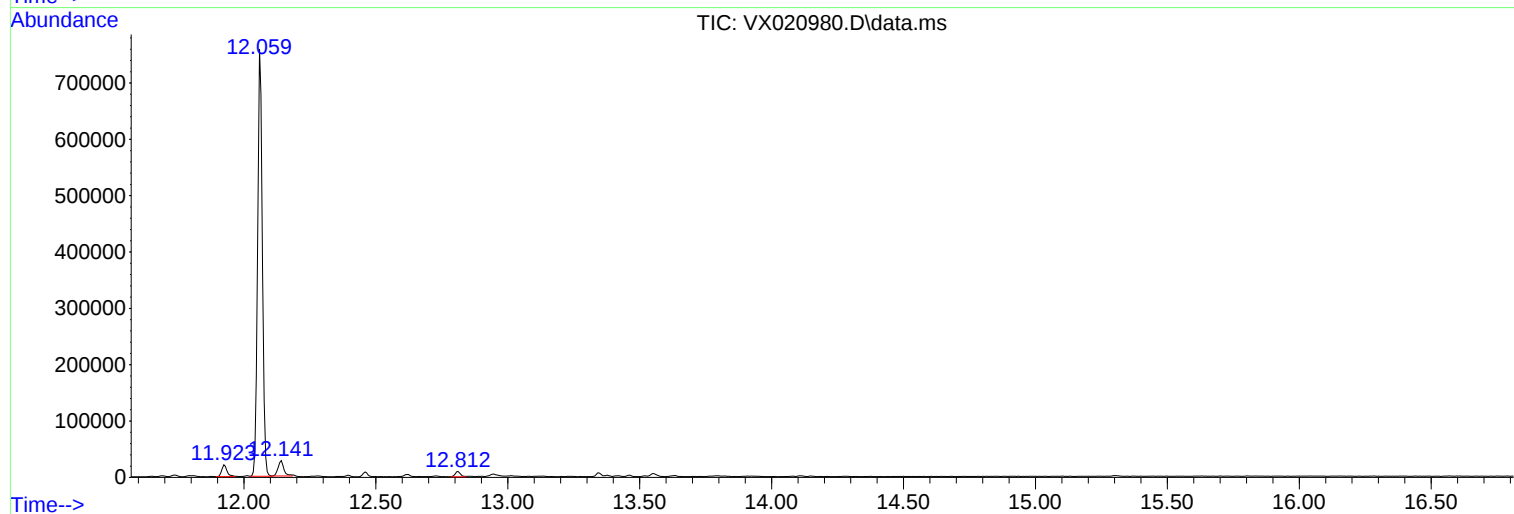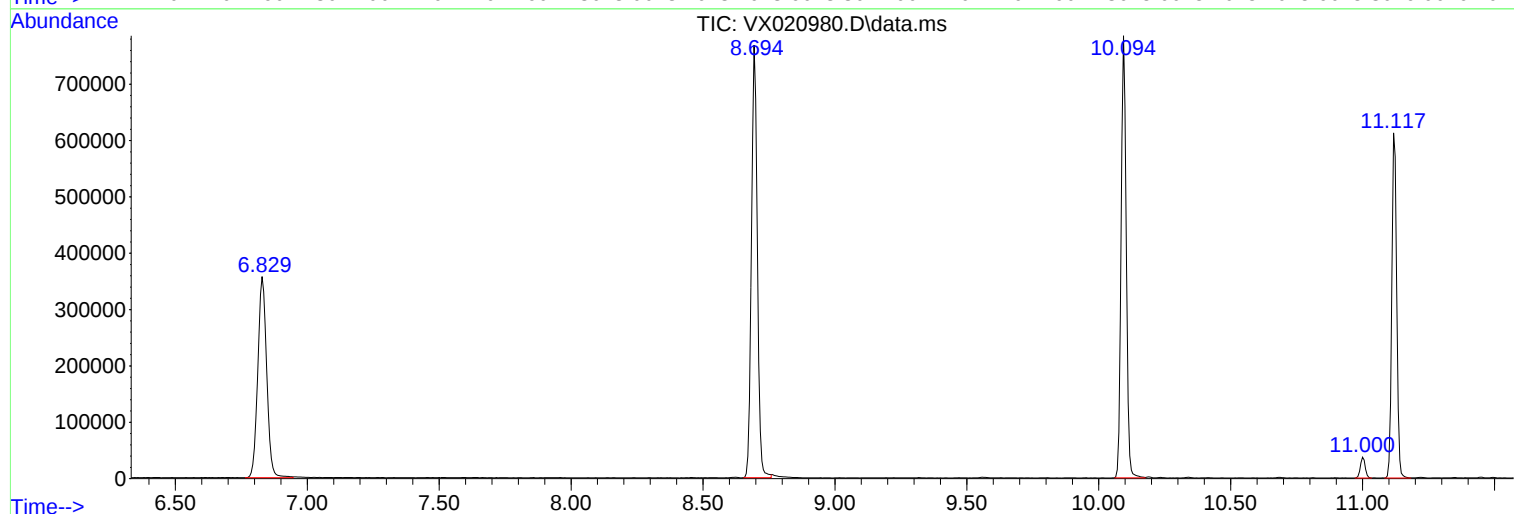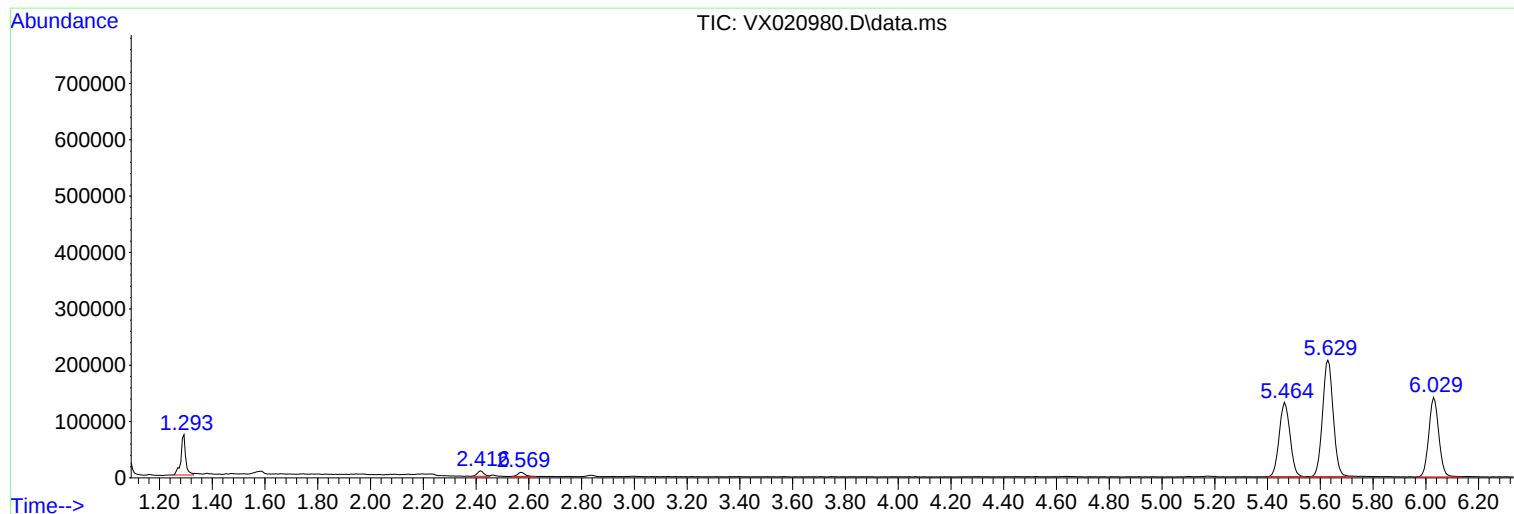

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
Data File : VX020980.D
Acq On : 02 Mar 2021 21:23
Operator : JC/MD
Sample : M1545-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RIM-7.55










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1-chloro-1,1-difluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.293	7.70 ug/l	89351	Pentafluorobenzene	5.629

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1-chloro-1,1-difluoro-	100	C2H3ClF2	000075-68-3	90
2			Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	43
3			(2-Aminophenyl)(3,6-dihydro-2H-p...	203	C11H13N3O	1000305-06-4	4
4			Propane, 1,1,2,2-tetrafluoro-	116	C3H4F4	040723-63-5	4
5			Pentane, 1,1,2,2,3,3,4,4-octaflu...	216	C5H4F8	040723-64-6	4

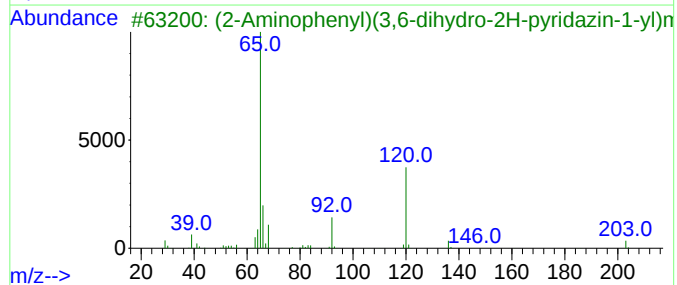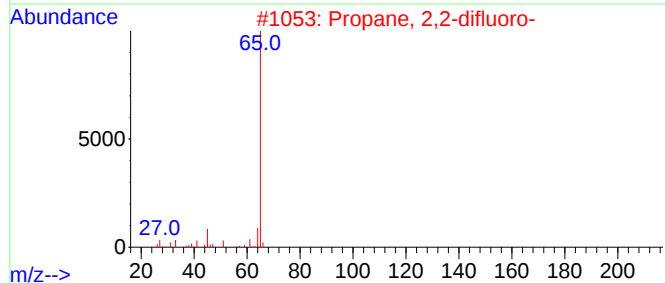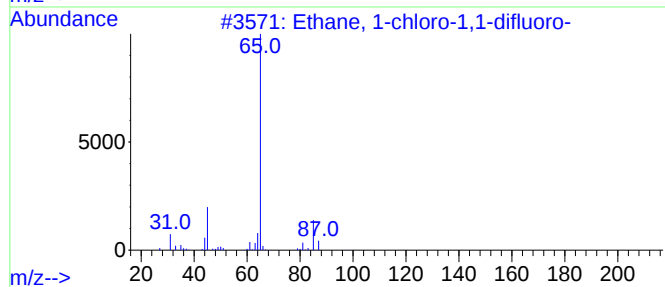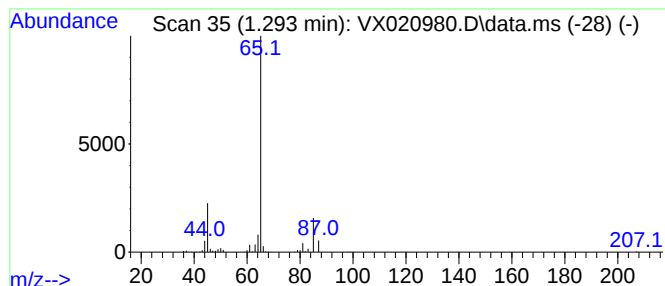

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
Data File : VX020980.D
Acq On : 02 Mar 2021 21:23
Operator : JC/MD
Sample : M1545-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RIM-7.55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1-chlor...	1.293	7.7	ug/l	89351	1	5.629	580026	50.0