

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
 Data File : VX020987.D
 Acq On : 03 Mar 2021 00:05
 Operator : JC/MD
 Sample : M1536-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FIELD-BLANK

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
 Title : SW846 8260

Signal : TIC: VX020987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.611	80	89	95	rBV7	4870	11562	1.00%	0.193%
2	2.417	220	226	235	rBV	8347	14855	1.29%	0.248%
3	2.581	248	254	265	rVB	8360	19158	1.66%	0.320%
4	2.987	318	323	334	rVB	6234	14805	1.28%	0.248%
5	5.464	732	744	759	rBV	128868	362476	31.42%	6.060%
6	5.629	761	772	787	rBV	198428	556458	48.23%	9.303%
7	6.029	829	840	856	rBV	134536	354555	30.73%	5.928%
8	6.829	965	976	991	rBV	339201	800716	69.40%	13.387%
9	8.694	1286	1293	1315	rBV	728599	1153730	100.00%	19.288%
10	10.094	1525	1531	1551	rVB	769384	1022091	88.59%	17.088%
11	11.118	1699	1705	1714	rBV	588753	762857	66.12%	12.754%
12	12.059	1860	1865	1879	rBV	735073	908217	78.72%	15.184%




Sum of corrected areas: 5981480

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
Data File : VX020987.D
Acq On : 03 Mar 2021 00:05
Operator : JC/MD
Sample : M1536-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

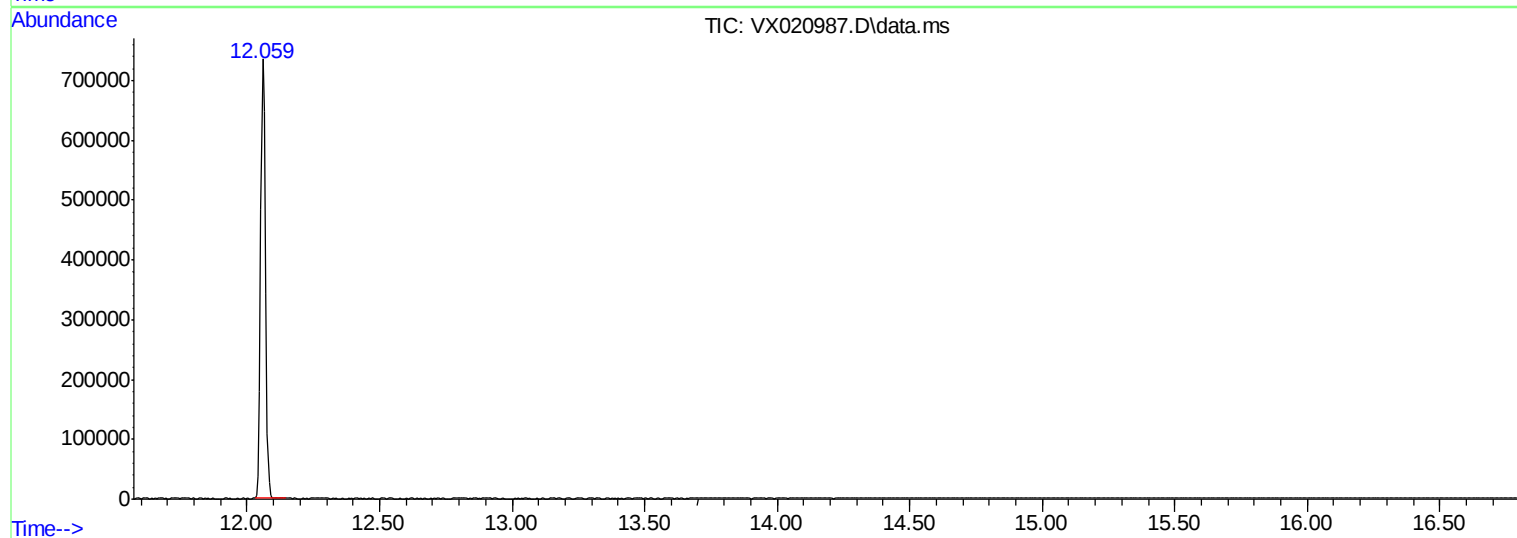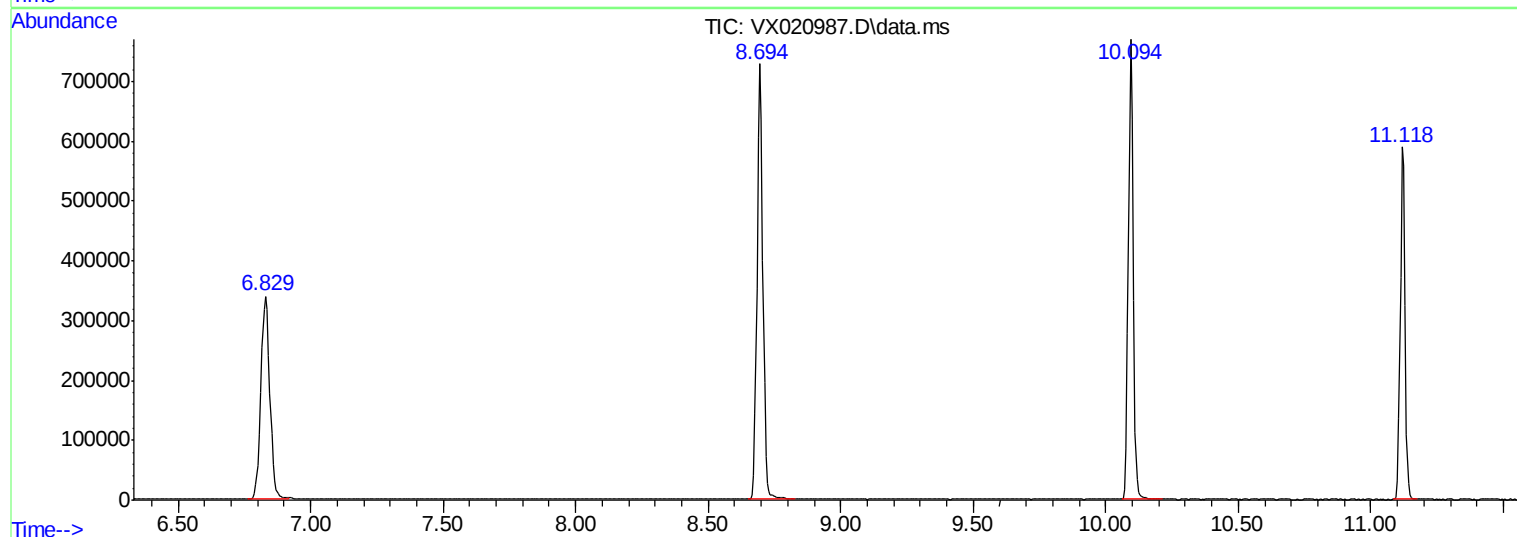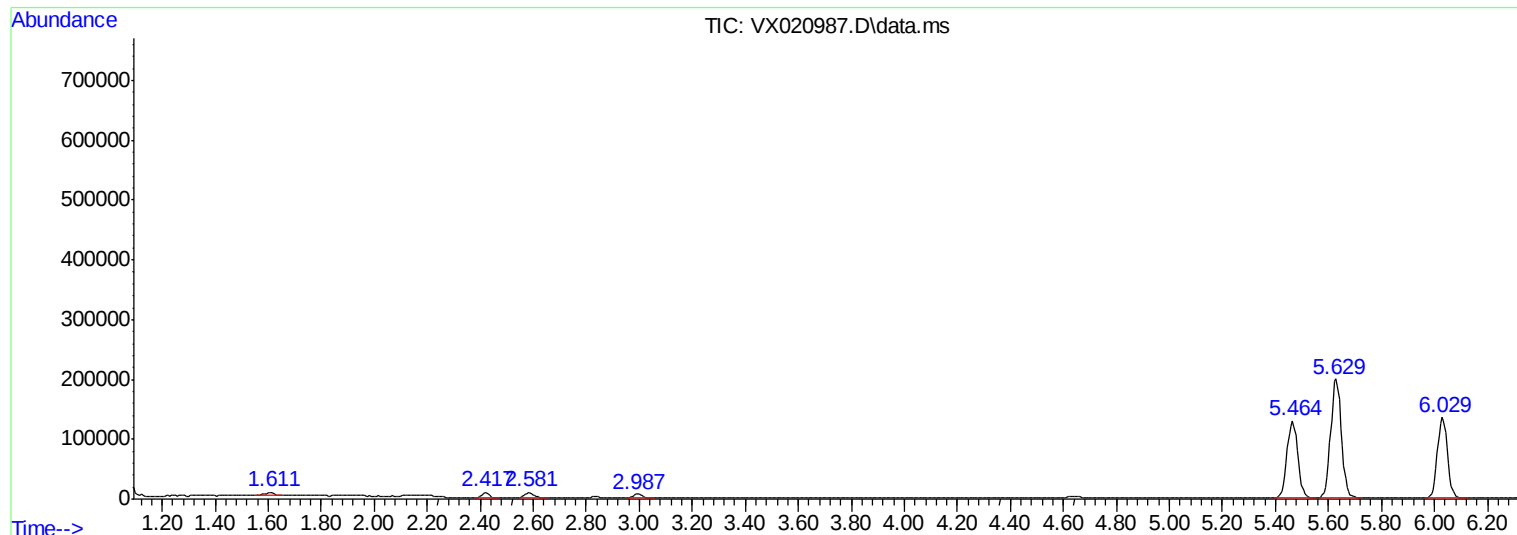

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
Data File : VX020987.D
Acq On : 03 Mar 2021 00:05
Operator : JC/MD
Sample : M1536-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030421\
Data File : VX020987.D
Acq On : 03 Mar 2021 00:05
Operator : JC/MD
Sample : M1536-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FIELD-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc
