

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030422\
 Data File : VX027305.D
 Acq On : 04 Mar 2022 16:41
 Operator : JC/MD
 Sample : N1793-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-6

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M

Title : SW846 8260

Signal : TIC: VX027305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	23	30	43	rVB4	2475	7123	1.90%	0.353%
2	2.538	233	238	243	rBV	2734	4876	1.30%	0.242%
3	5.391	695	706	722	rBV2	44308	128122	34.12%	6.347%
4	5.556	722	733	745	rBV	76339	212563	56.61%	10.530%
5	5.964	790	800	812	rBV	45364	120953	32.21%	5.992%
6	6.769	922	932	945	rBV	119975	277468	73.90%	13.746%
7	8.647	1234	1240	1250	rBV	249594	375478	100.00%	18.601%
8	10.055	1465	1471	1481	rBV	246560	326574	86.98%	16.178%
9	11.079	1634	1639	1648	rBV	193419	251946	67.10%	12.481%
10	12.024	1789	1794	1807	rVB	254374	313472	83.49%	15.529%




Sum of corrected areas: 2018575

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030422\
Data File : VX027305.D
Acq On : 04 Mar 2022 16:41
Operator : JC/MD
Sample : N1793-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

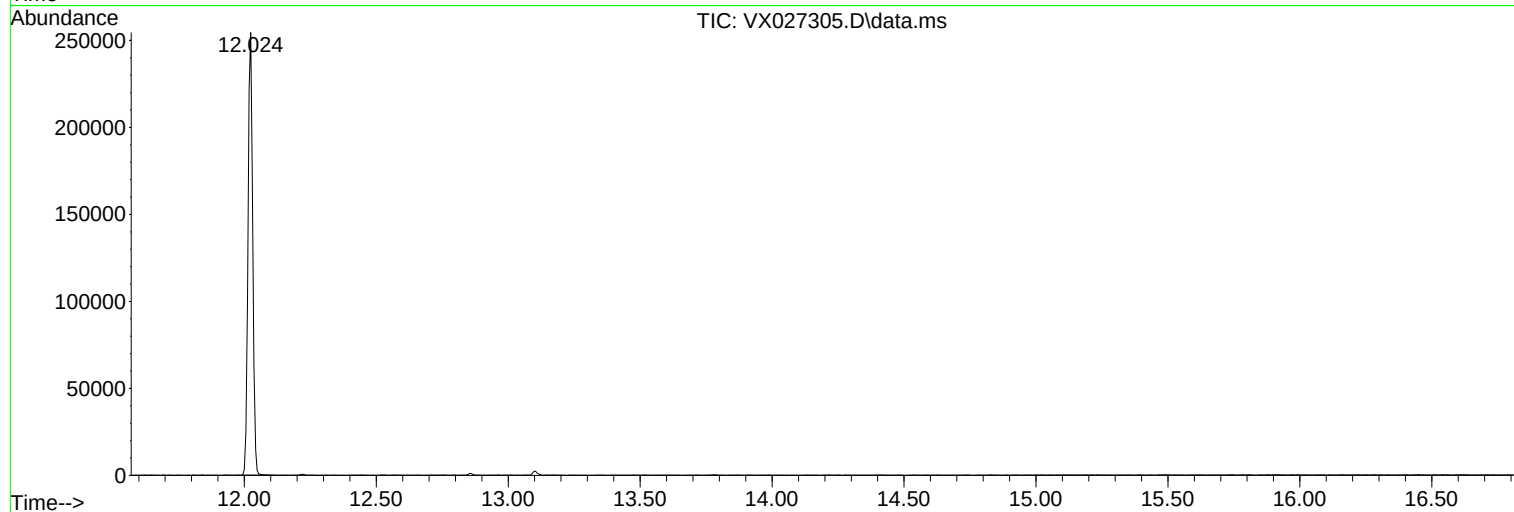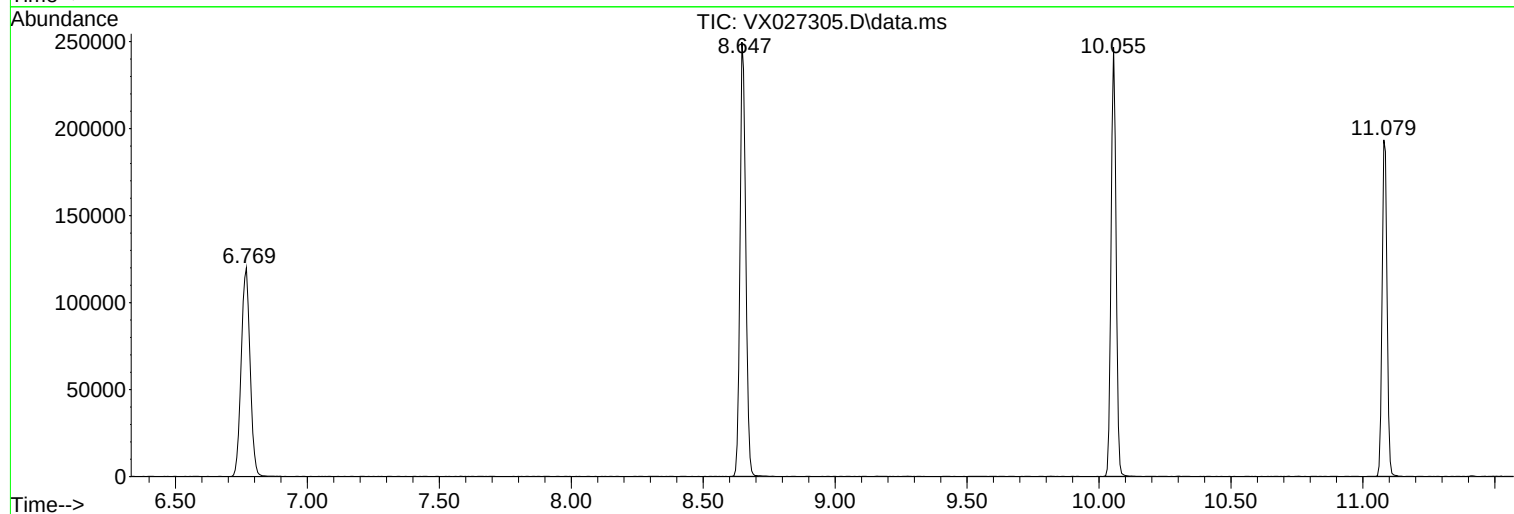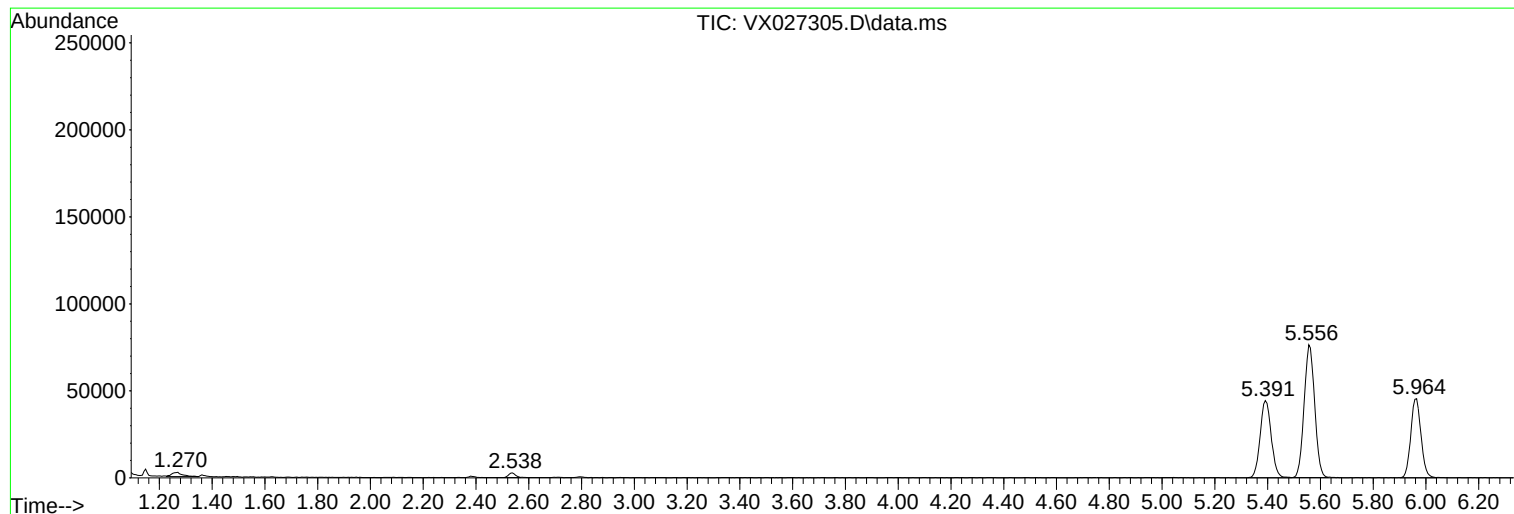

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030422\
Data File : VX027305.D
Acq On : 04 Mar 2022 16:41
Operator : JC/MD
Sample : N1793-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030422\
Data File : VX027305.D
Acq On : 04 Mar 2022 16:41
Operator : JC/MD
Sample : N1793-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc