


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030422\
Data File : VX027289.D
Acq On : 04 Mar 2022 09:41
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022322W.M
Title : SW846 8260
Last Update : Wed Feb 23 13:06:57 2022

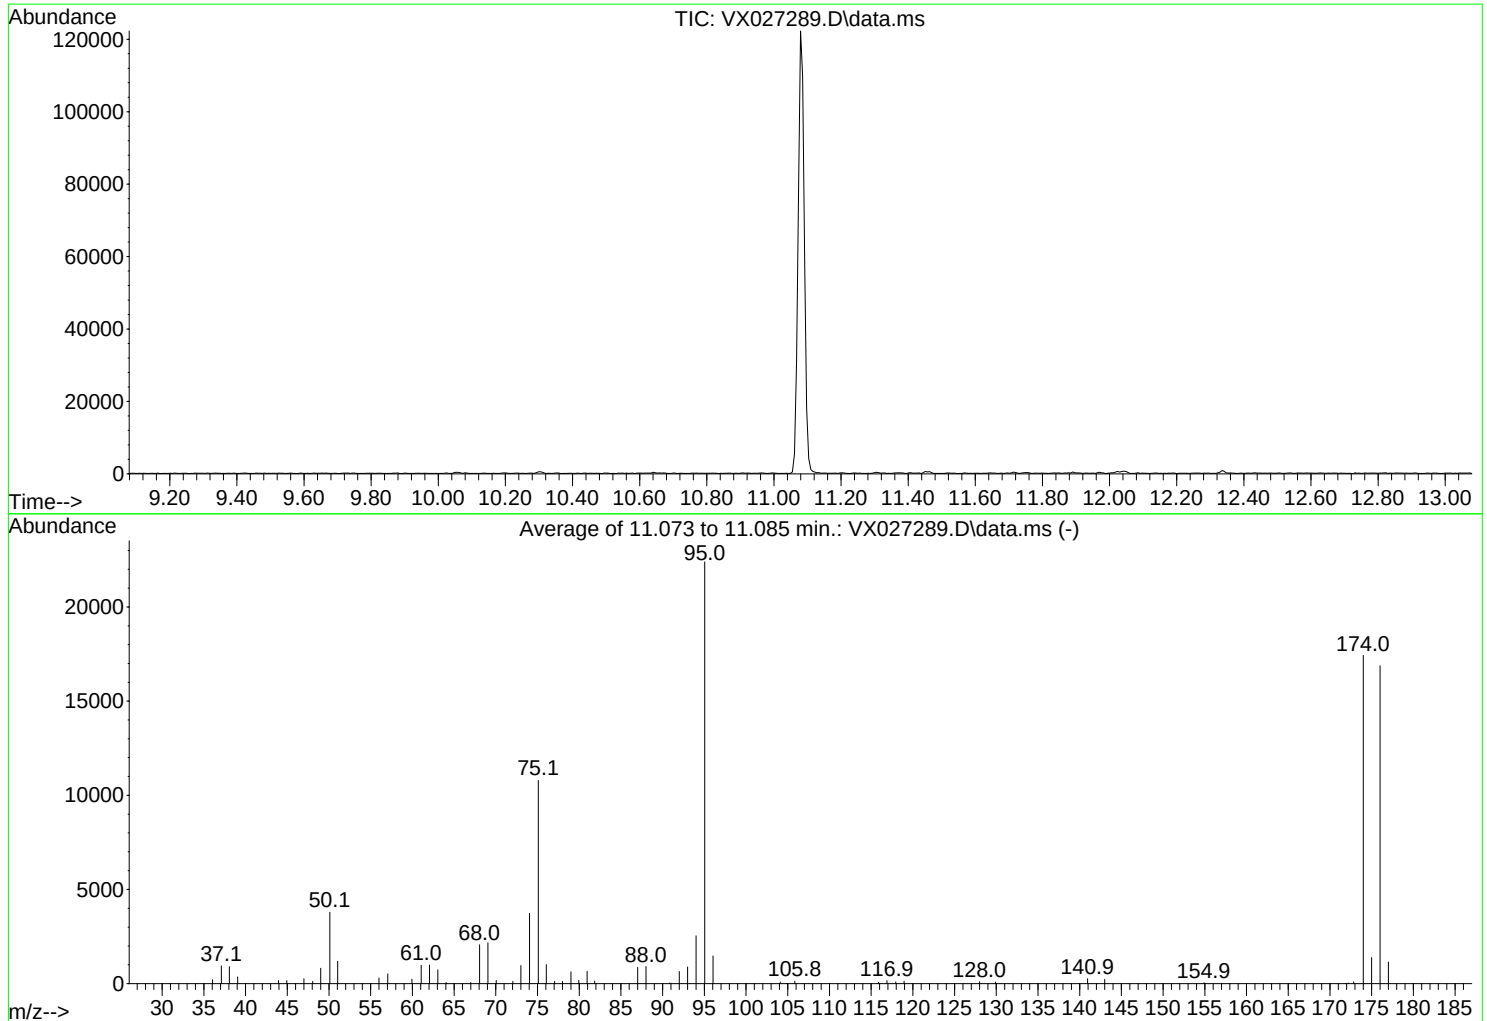

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	3785	PASS
75	95	30	60	48.2	10791	PASS
95	95	100	100	100.0	22395	PASS
96	95	5	9	6.6	1473	PASS
173	174	0.00	2	0.5	93	PASS
174	95	50	100	77.8	17430	PASS
175	174	5	9	7.9	1385	PASS
176	174	95	101	96.8	16879	PASS
177	176	5	9	6.8	1143	PASS