

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030424\
 Data File : VX040561.D
 Acq On : 04 Mar 2024 12:04
 Operator : JC/MD
 Sample : VX0304MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0304MBL01

Quant Time: Mar 05 00:22:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 27 05:01:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	77989	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	130985	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	125460	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	62175	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	71204	54.587	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 109.180%	
35) Dibromofluoromethane	5.385	113	50542	55.488	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 110.980%	
50) Toluene-d8	8.647	98	185551	56.120	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 112.240%	
62) 4-Bromofluorobenzene	11.079	95	72106	57.212	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	= 114.420%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030424\
Data File : VX040561.D
Acq On : 04 Mar 2024 12:04
Operator : JC/MD
Sample : VX0304MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0304MBL01

Quant Time: Mar 05 00:22:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 27 05:01:33 2024
Response via : Initial Calibration




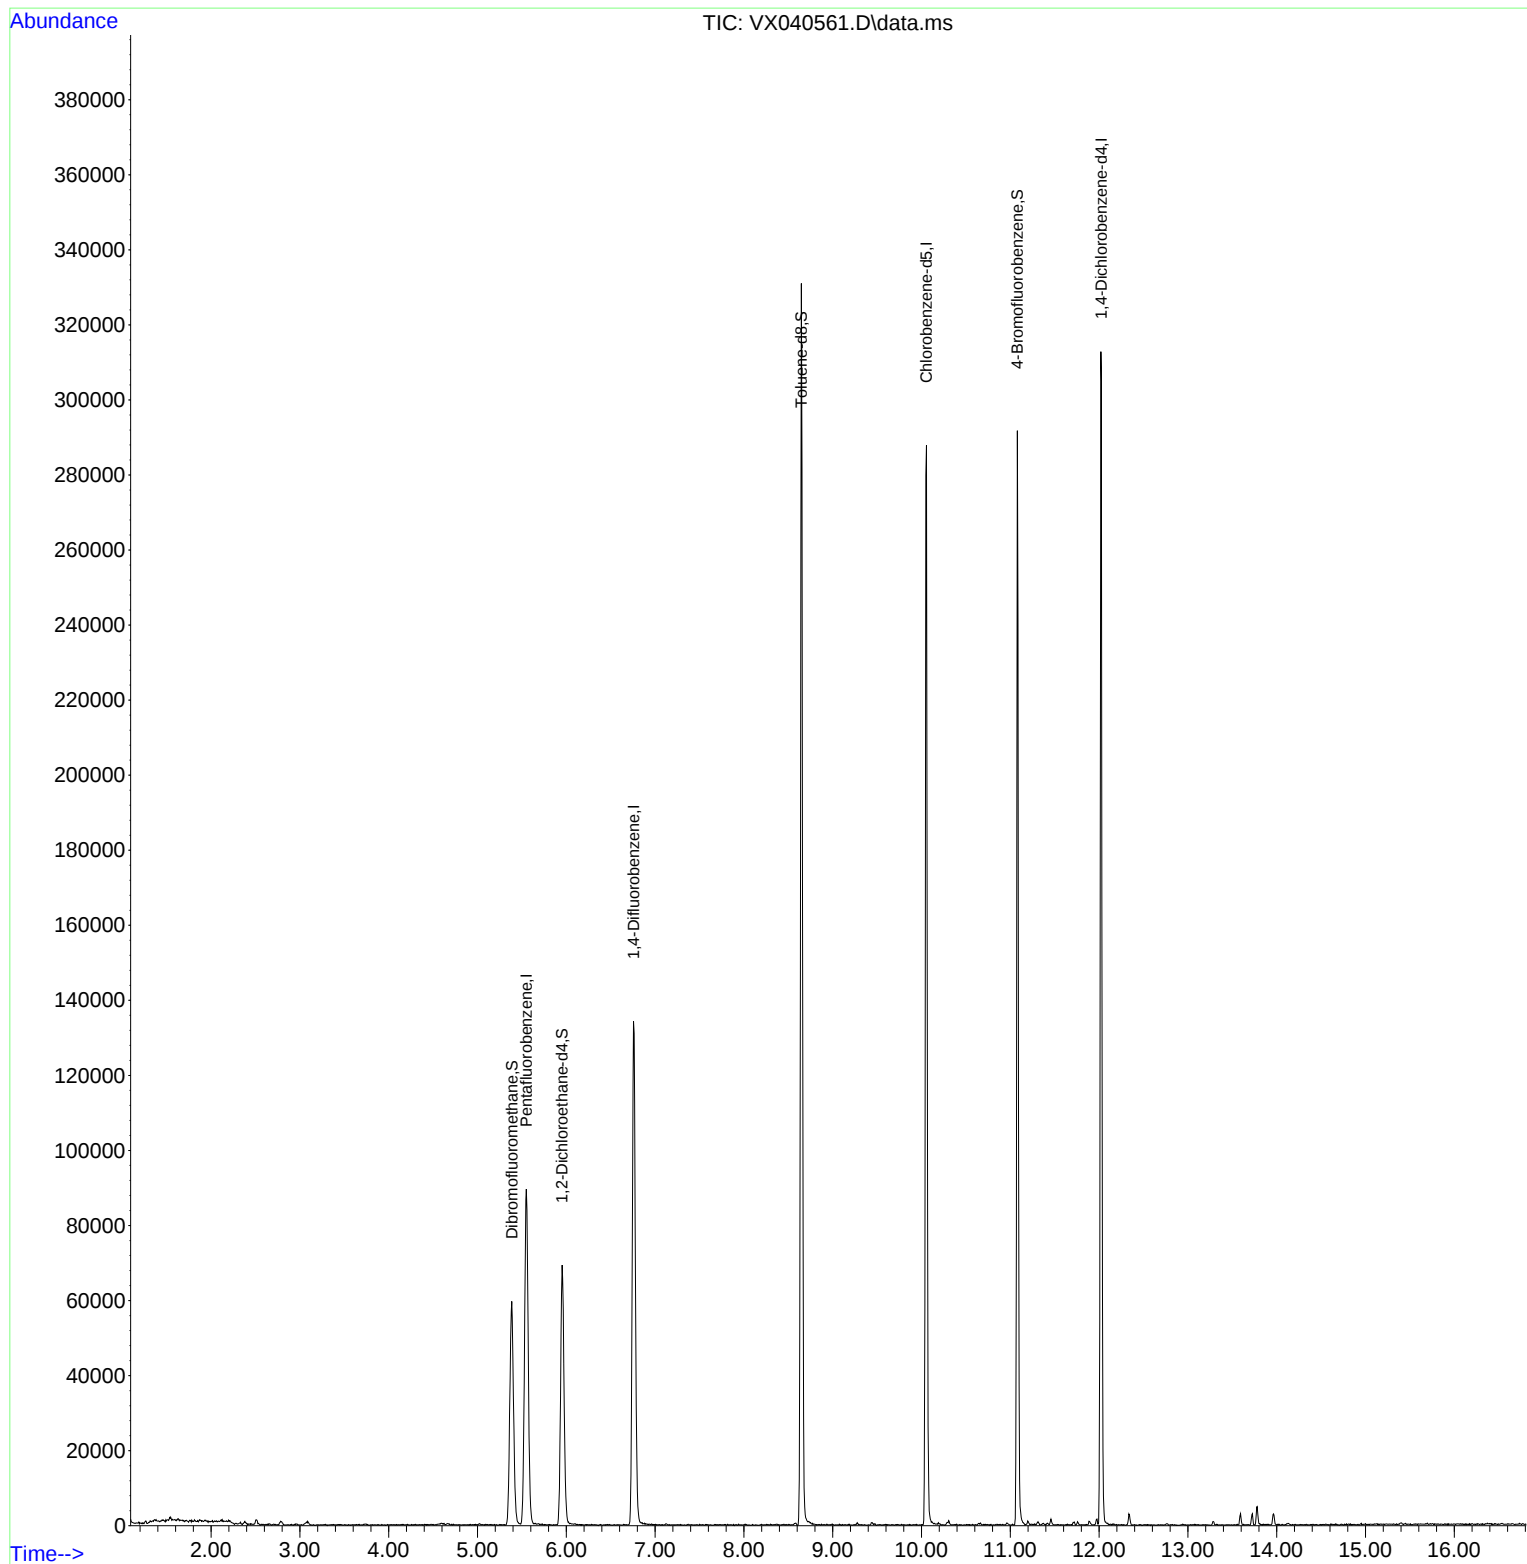


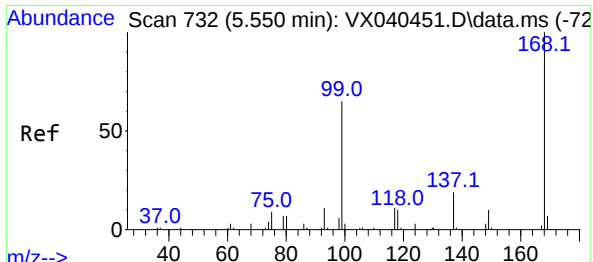

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX040561.D
Acq: 04 Mar 2024 12:04




Instrument :
MSVOA_X
ClientSampleId :
VX0304MBL01


Tgt Ion:168 Resp: 77989
Ion Ratio Lower Upper
168 100
99 69.5 56.6 85.0

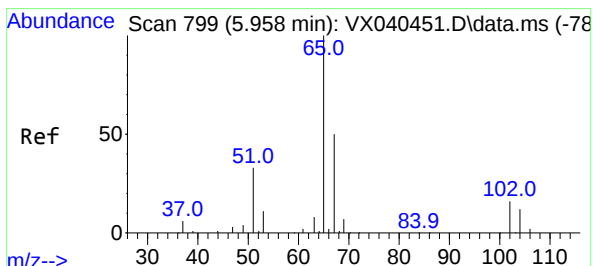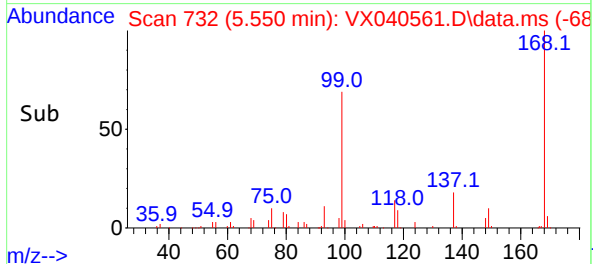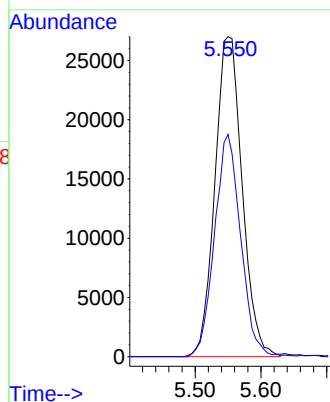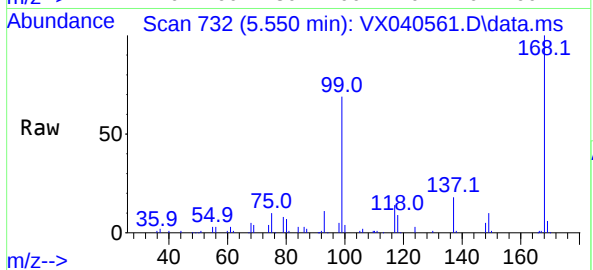

#33
1,2-Dichloroethane-d4
Concen: 54.587 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX040561.D
Acq: 04 Mar 2024 12:04

Tgt Ion: 65 Resp: 71204
Ion Ratio Lower Upper
65 100
67 48.9 0.0 100.2


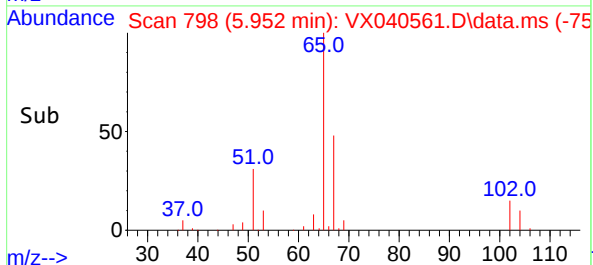
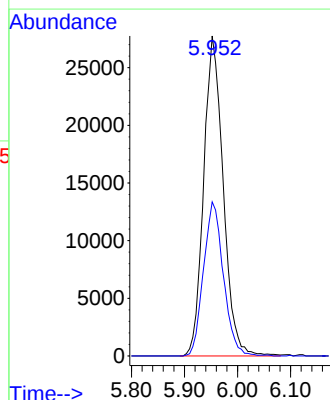
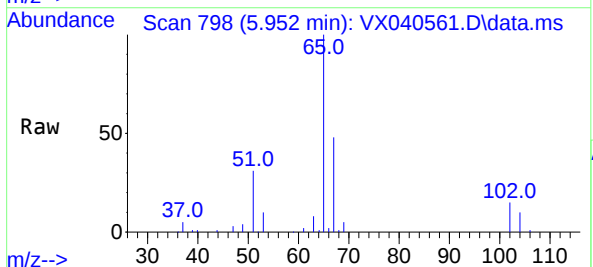


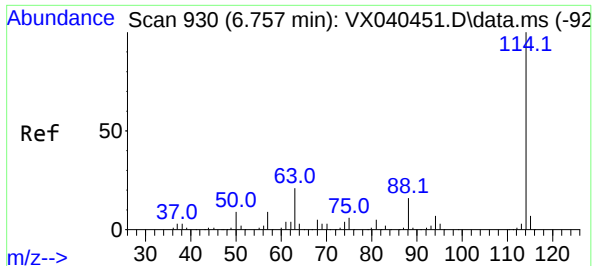

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX040561.D
Acq: 04 Mar 2024 12:04




Instrument :
MSVOA_X
ClientSampleId :
VX0304MBL01


Tgt Ion:114 Resp: 130985
Ion Ratio Lower Upper
114 100
63 23.5 0.0 45.0
88 17.5 0.0 36.6

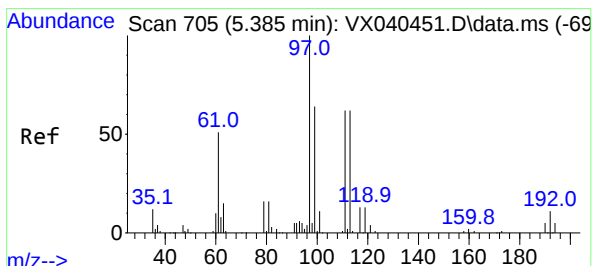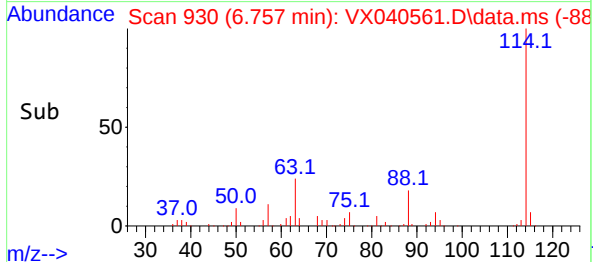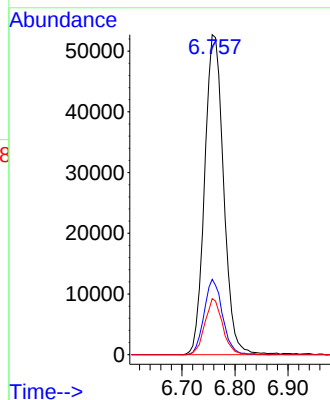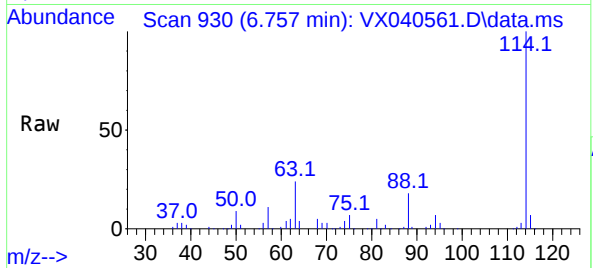

#35
Dibromofluoromethane
Concen: 55.488 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX040561.D
Acq: 04 Mar 2024 12:04

Tgt Ion:113 Resp: 50542
Ion Ratio Lower Upper
113 100
111 100.6 82.9 124.3
192 18.5 13.3 19.9


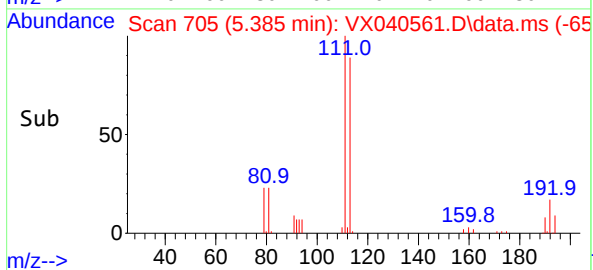
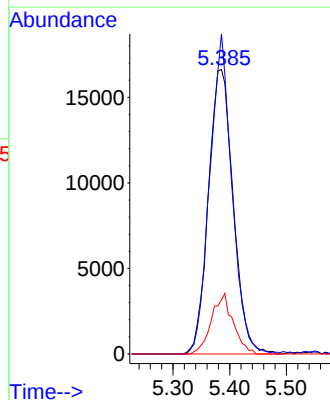
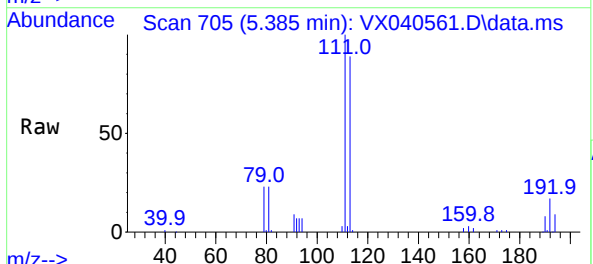


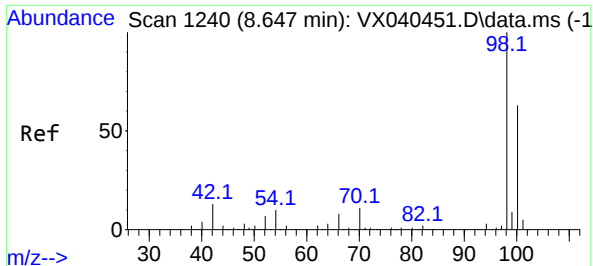

#50
Toluene-d8
Concen: 56.120 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX040561.D
Acq: 04 Mar 2024 12:04




Instrument :
MSVOA_X
ClientSampleId :
VX0304MBL01


Tgt Ion: 98 Resp: 185551
Ion Ratio Lower Upper
98 100
100 63.1 53.1 79.7

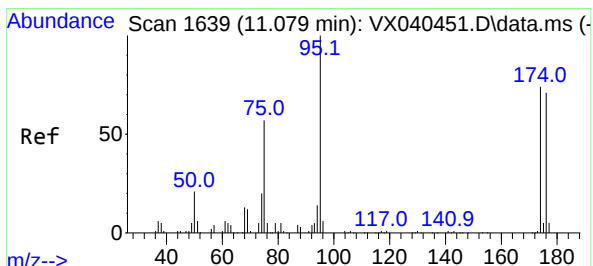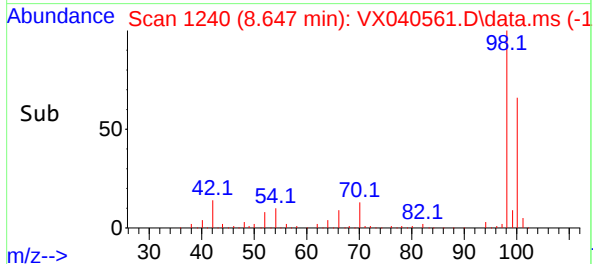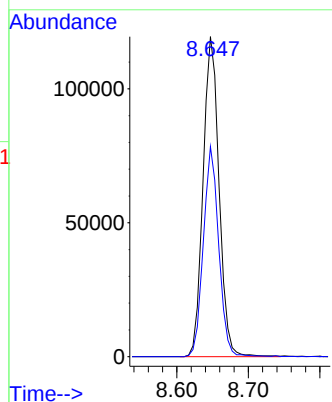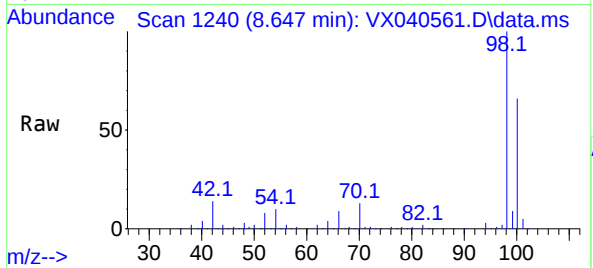

#62
4-Bromofluorobenzene
Concen: 57.212 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX040561.D
Acq: 04 Mar 2024 12:04

Tgt Ion: 95 Resp: 72106
Ion Ratio Lower Upper
95 100
174 74.8 0.0 135.6
176 71.8 0.0 131.0


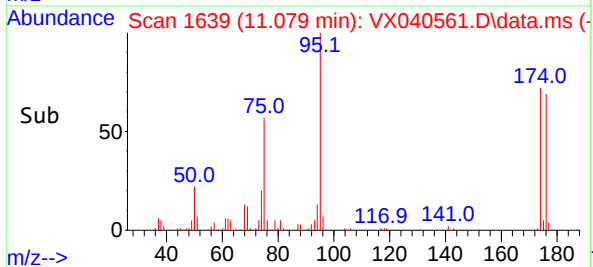
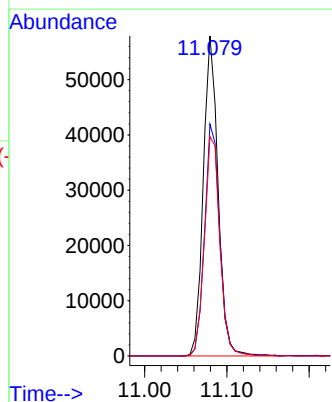
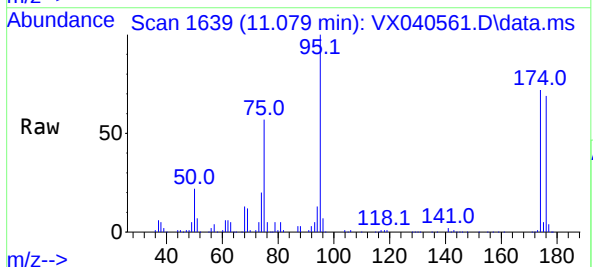


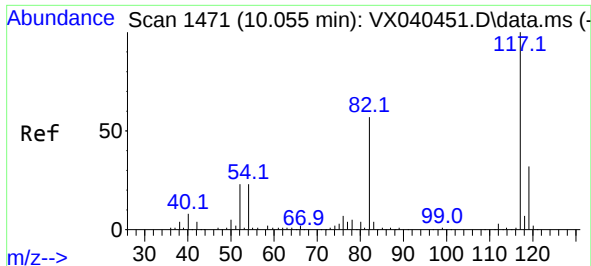

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX040561.D
Acq: 04 Mar 2024 12:04

Instrument :
MSVOA_X
ClientSampleId :
VX0304MBL01

Tgt Ion:117 Resp: 125460
Ion Ratio Lower Upper
117 100
82 59.0 46.2 69.4
119 32.5 25.5 38.3

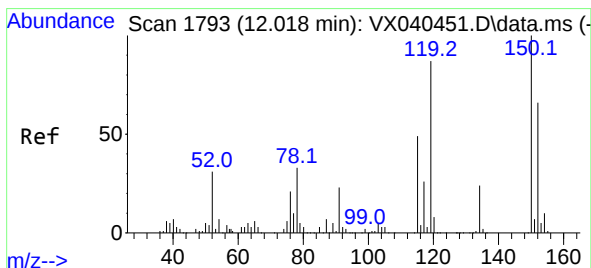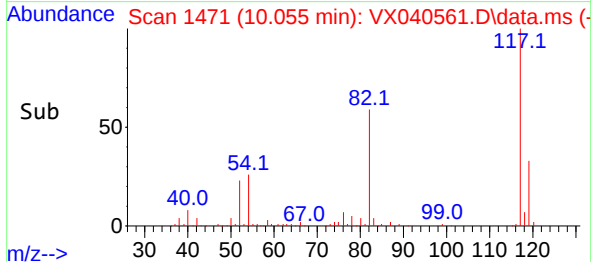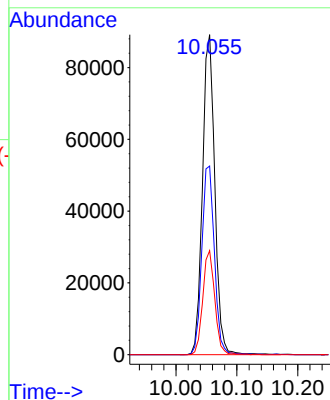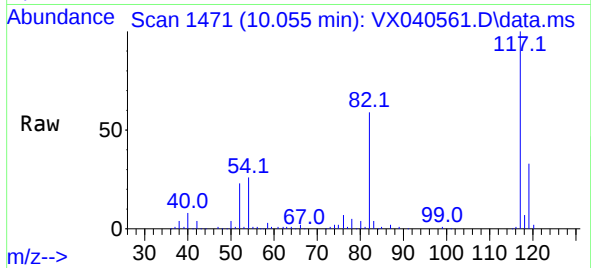

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX040561.D
Acq: 04 Mar 2024 12:04

Tgt Ion:152 Resp: 62175
Ion Ratio Lower Upper
152 100
115 62.7 43.3 129.9
150 155.1 0.0 345.0

