

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030424\
 Data File : VX040575.D
 Acq On : 04 Mar 2024 17:38
 Operator : JC/MD
 Sample : P1661-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Mar 05 00:28:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 27 05:01:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	73015	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	126640	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	127387	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	65622	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	60890	49.860	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	99.720%
35) Dibromofluoromethane	5.385	113	43479	49.372	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.740%
50) Toluene-d8	8.647	98	156623	48.996	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.000%
62) 4-Bromofluorobenzene	11.079	95	64125	52.625	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	105.240%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030424\
Data File : VX040575.D
Acq On : 04 Mar 2024 17:38
Operator : JC/MD
Sample : P1661-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Mar 05 00:28:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 27 05:01:33 2024
Response via : Initial Calibration




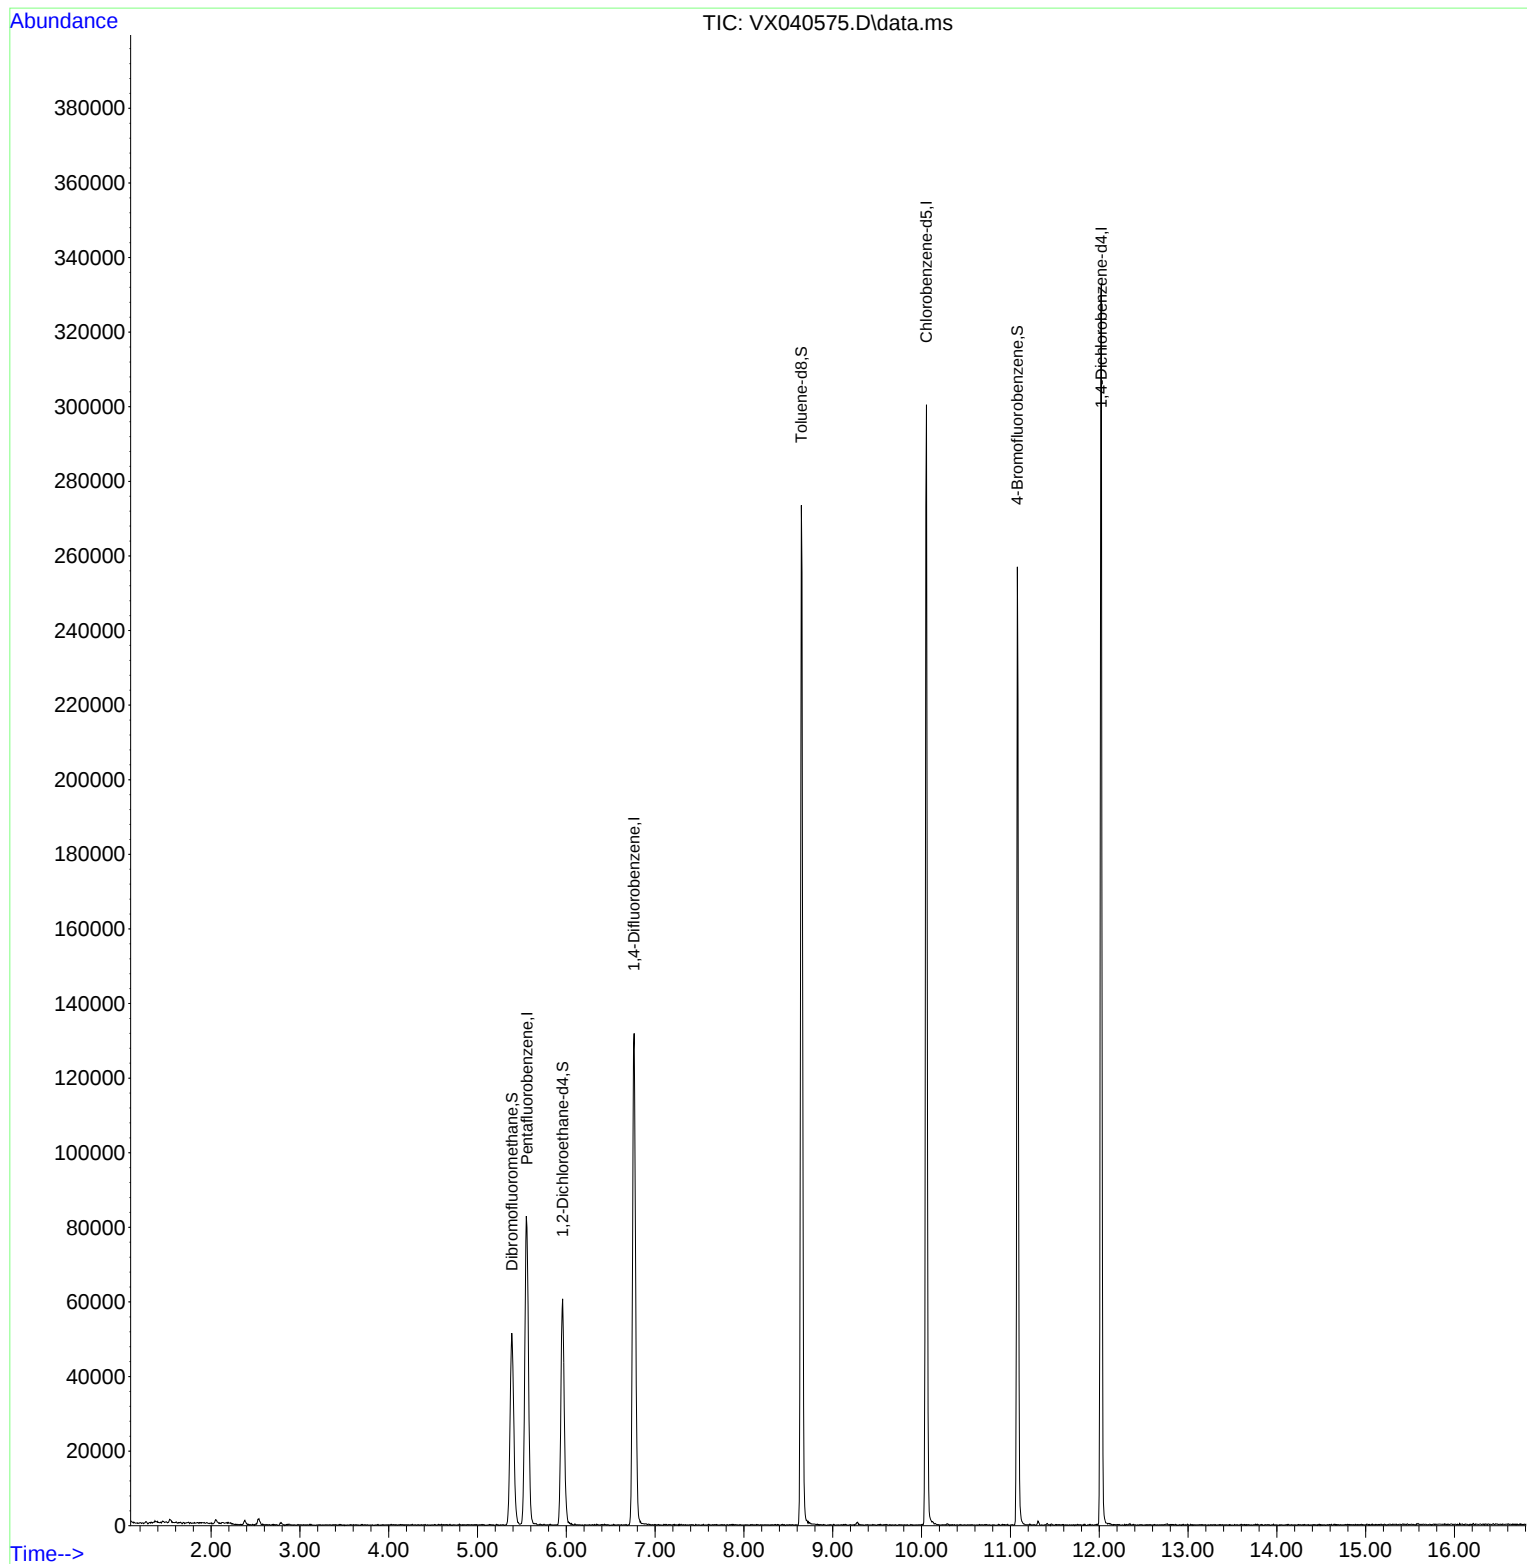


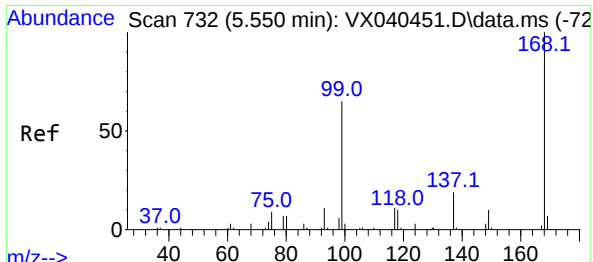

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.006 min
Lab File: VX040575.D
Acq: 04 Mar 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 73015
Ion Ratio Lower Upper
168 100
99 64.9 56.6 85.0

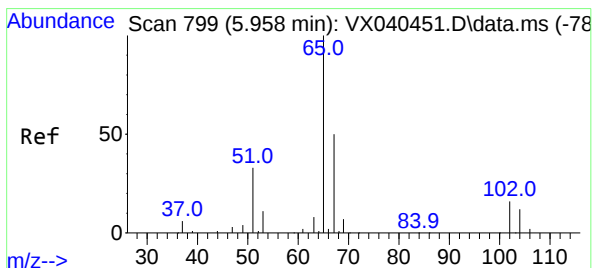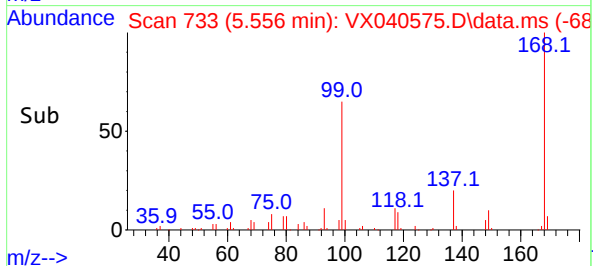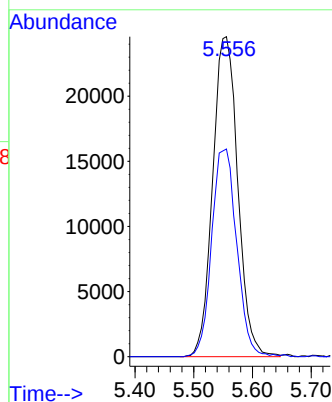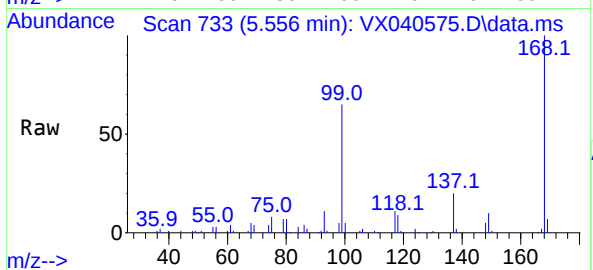

#33
1,2-Dichloroethane-d4
Concen: 49.860 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX040575.D
Acq: 04 Mar 2024 17:38

Tgt Ion: 65 Resp: 60890
Ion Ratio Lower Upper
65 100
67 49.6 0.0 100.2


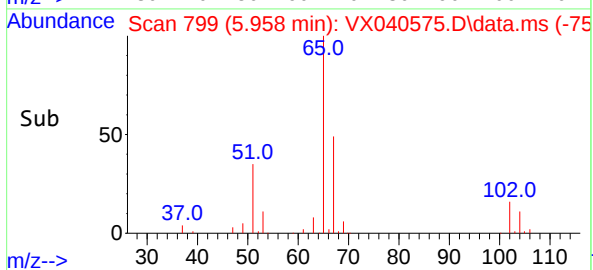
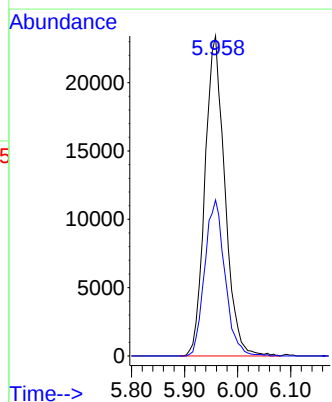
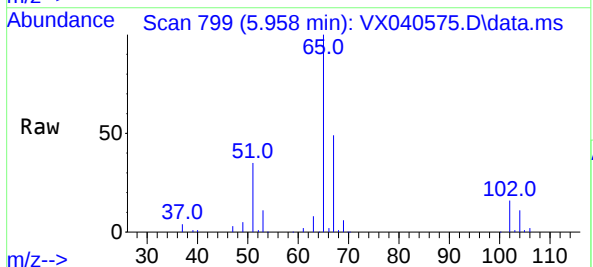


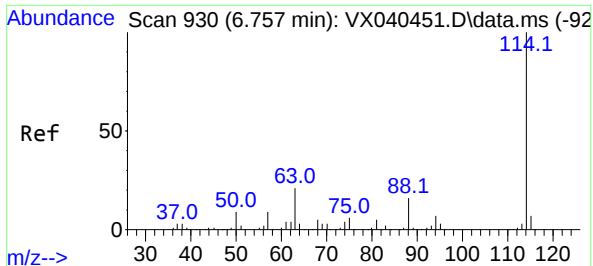

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.006 min
Lab File: VX040575.D
Acq: 04 Mar 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:114 Resp: 126640
Ion Ratio Lower Upper
114 100
63 22.4 0.0 45.0
88 15.6 0.0 36.6

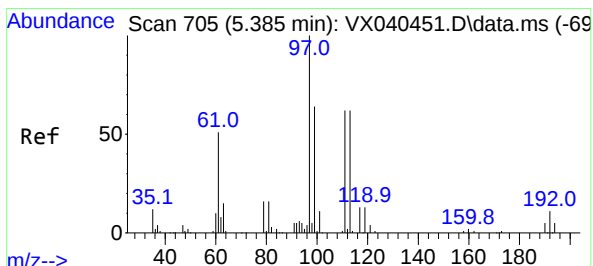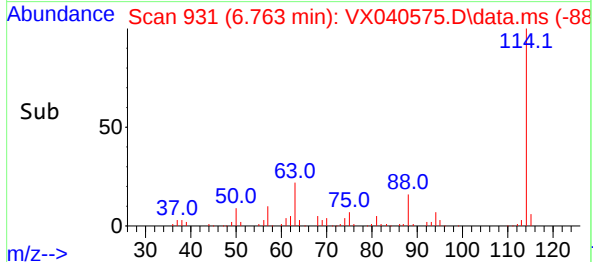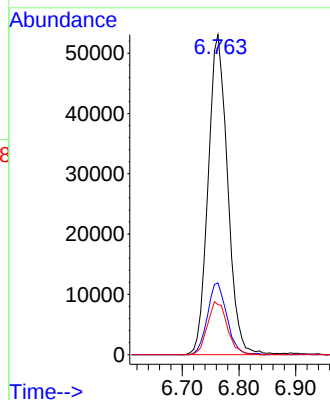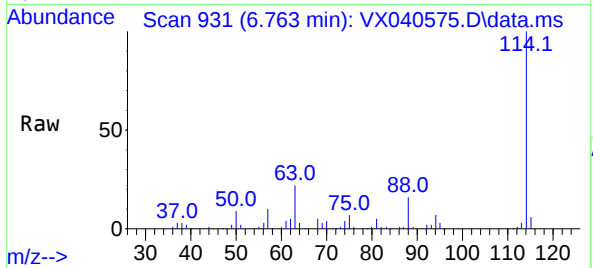

#35
Dibromofluoromethane
Concen: 49.372 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX040575.D
Acq: 04 Mar 2024 17:38

Tgt Ion:113 Resp: 43479
Ion Ratio Lower Upper
113 100
111 103.7 82.9 124.3
192 18.4 13.3 19.9


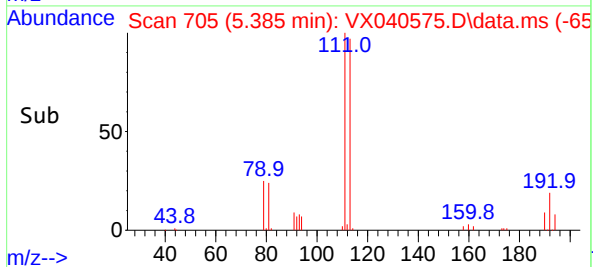
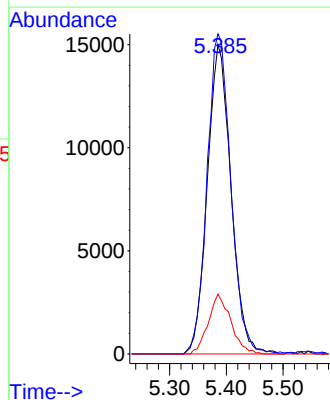
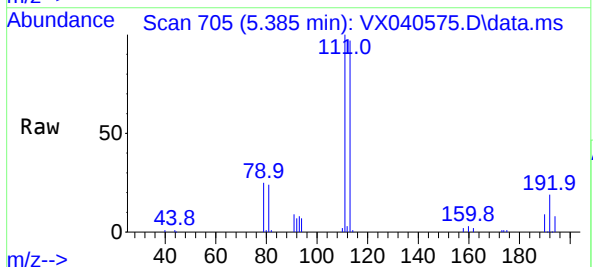


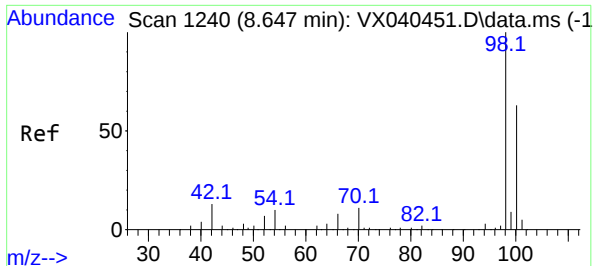

#50
Toluene-d8
Concen: 48.996 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX040575.D
Acq: 04 Mar 2024 17:38




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 156623
Ion Ratio Lower Upper
98 100
100 64.1 53.1 79.7

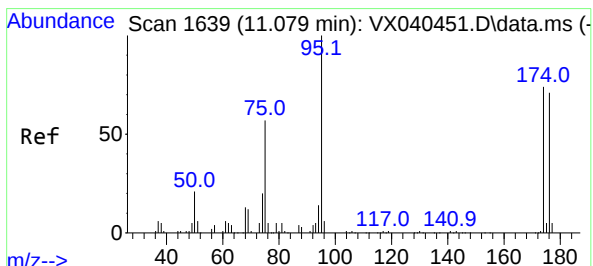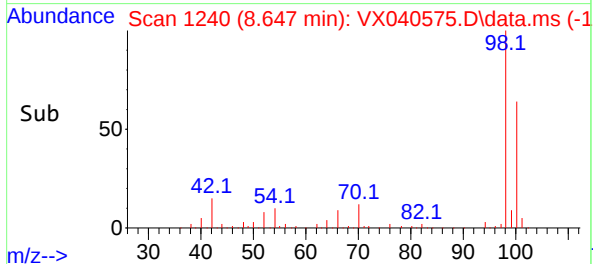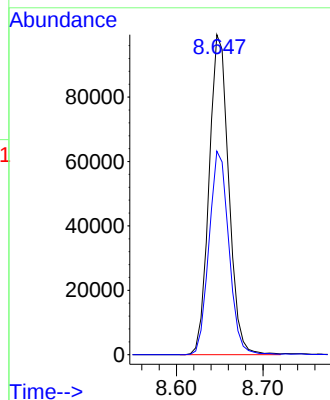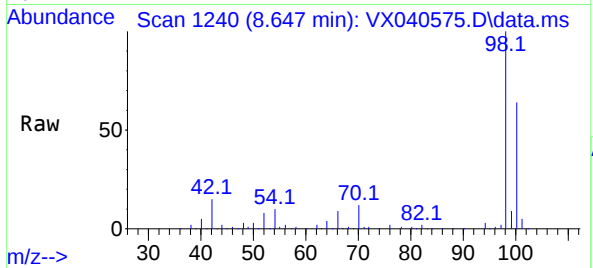

#62
4-Bromofluorobenzene
Concen: 52.625 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX040575.D
Acq: 04 Mar 2024 17:38

Tgt Ion: 95 Resp: 64125
Ion Ratio Lower Upper
95 100
174 75.3 0.0 135.6
176 70.4 0.0 131.0


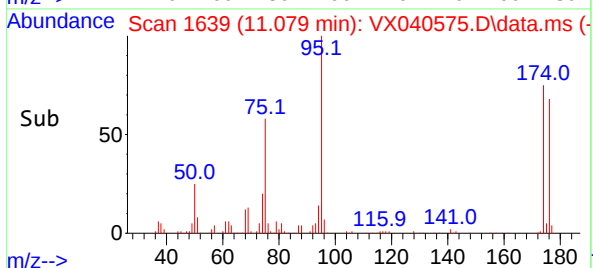
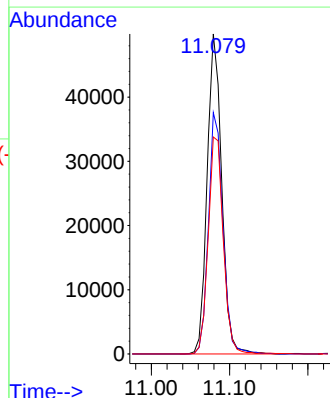
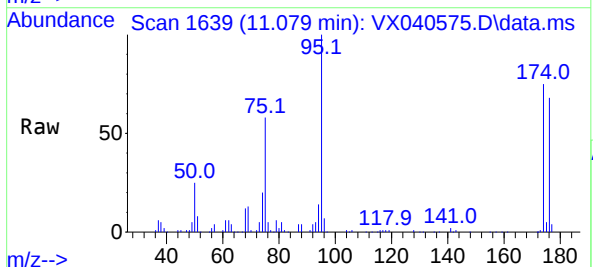


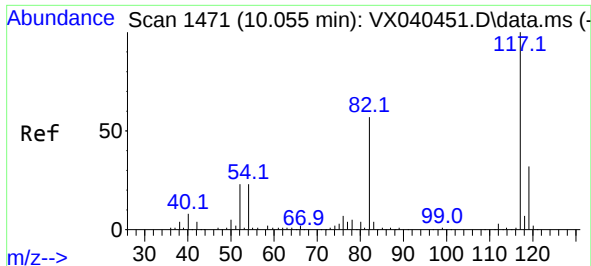

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX040575.D
Acq: 04 Mar 2024 17:38

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:117 Resp: 127387
Ion Ratio Lower Upper
117 100
82 58.8 46.2 69.4
119 30.9 25.5 38.3

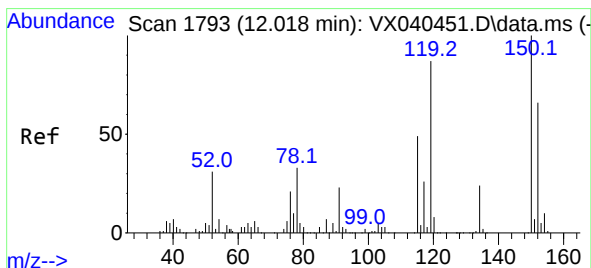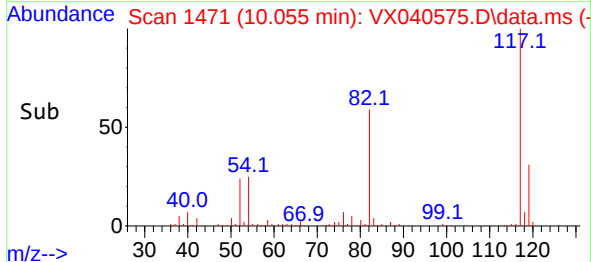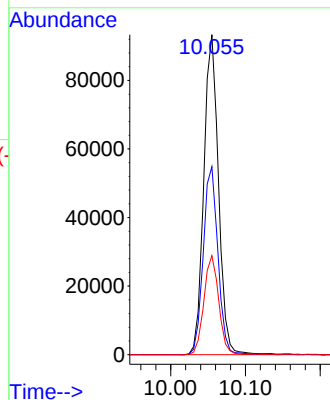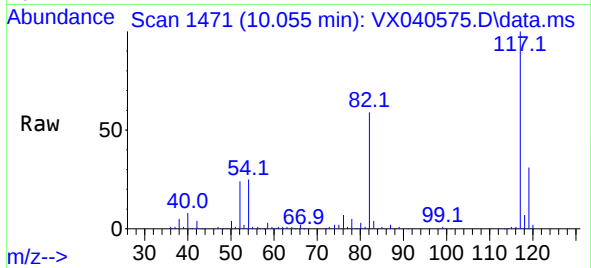

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX040575.D
Acq: 04 Mar 2024 17:38

Tgt Ion:152 Resp: 65622
Ion Ratio Lower Upper
152 100
115 62.3 43.3 129.9
150 158.7 0.0 345.0

