
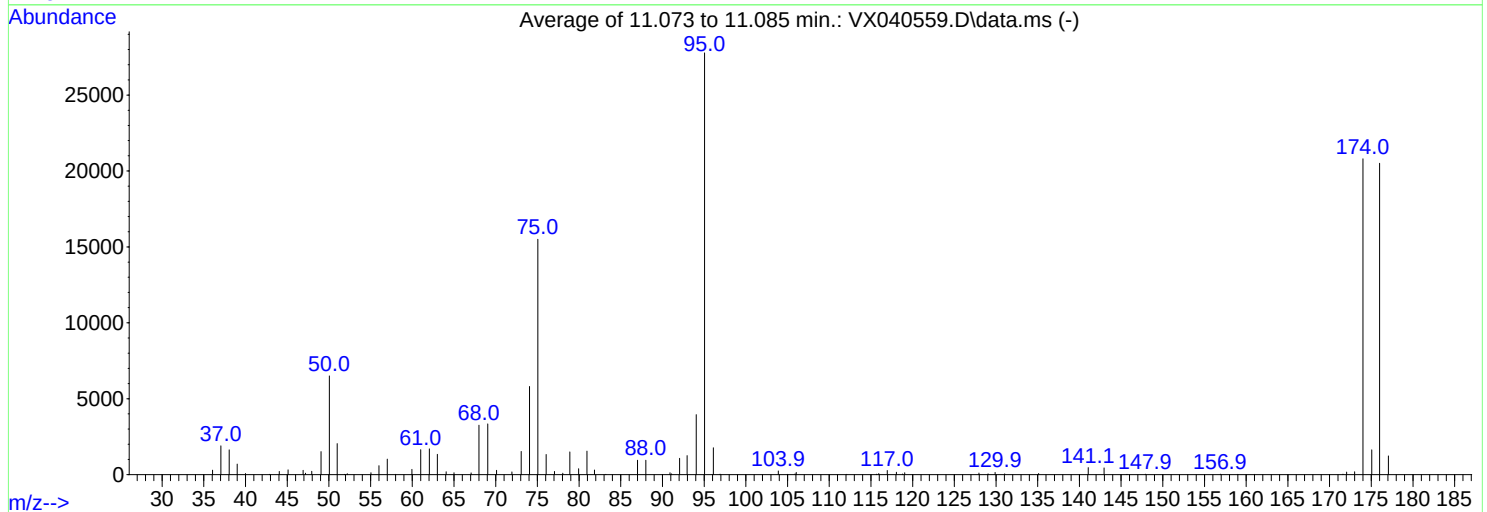


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030424\
Data File : VX040559.D
Acq On : 04 Mar 2024 08:49
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022624W.M
Title : SW846 8260
Last Update : Tue Feb 27 05:01:33 2024

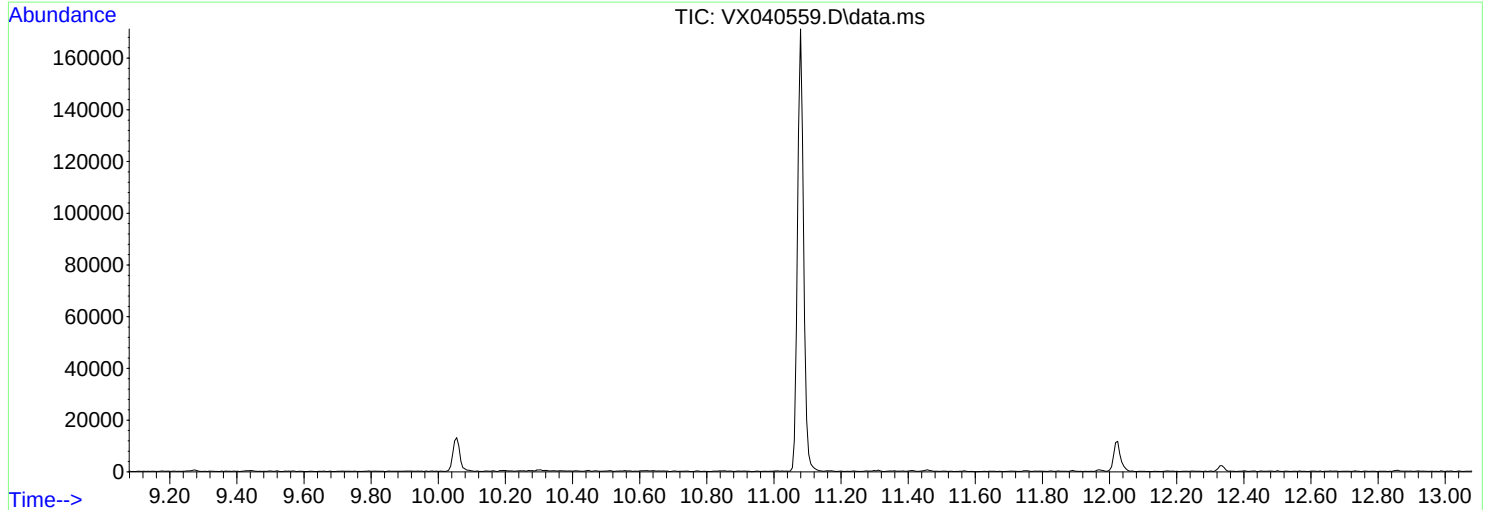

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.4	6503	PASS
75	95	30	60	55.8	15505	PASS
95	95	100	100	100.0	27781	PASS
96	95	5	9	6.4	1771	PASS
173	174	0.00	2	0.9	188	PASS
174	95	50	100	74.9	20808	PASS
175	174	5	9	7.9	1637	PASS
176	174	95	101	98.5	20506	PASS
177	176	5	9	6.0	1233	PASS