


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX030519\
Data File : VX007826.D
Acq On : 05 Mar 2019 09:10
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X022519W.M
Title : SW846 8260
Last Update : Tue Feb 26 01:53:13 2019

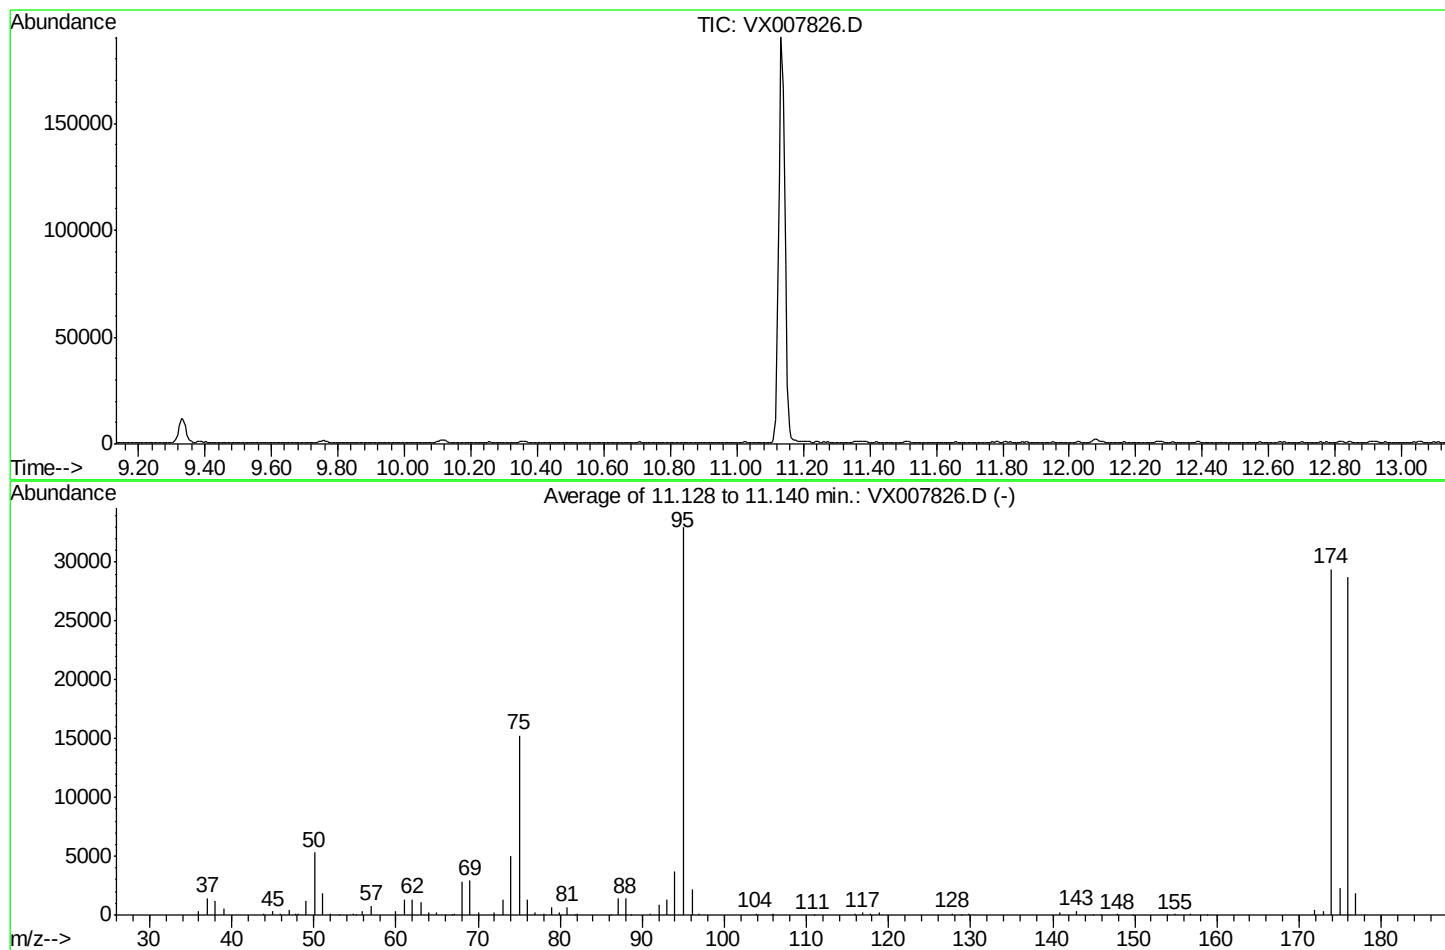

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	5320	PASS
75	95	30	60	46.4	15280	PASS
95	95	100	100	100.0	32960	PASS
96	95	5	9	6.5	2148	PASS
173	174	0.00	2	1.1	317	PASS
174	95	50	100	89.3	29432	PASS
175	174	5	9	7.8	2305	PASS
176	174	95	101	97.7	28741	PASS
177	176	5	9	6.6	1887	PASS