

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX030520\
 Data File : VX015108.D
 Acq On : 05 Mar 2020 13:48
 Operator : JC/SP
 Sample : L1812-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WASTE-TANK -030420

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	45	rBV	3390062	4368572	100.00%	28.749%
2	1.338	67	74	79	rBV	77079	262784	6.02%	1.729%
3	5.118	685	694	713	rVB2	119224	367010	8.40%	2.415%
4	5.490	742	755	769	rBV	216404	608347	13.93%	4.004%
5	5.655	769	782	798	rVV	366973	1014793	23.23%	6.678%
6	6.051	838	847	861	rBV	229730	600865	13.75%	3.954%
7	6.850	969	978	988	rBV	574523	1332674	30.51%	8.770%
8	8.709	1276	1283	1290	rBV	1229382	1866267	42.72%	12.282%
9	8.782	1290	1295	1300	rVB	66351	103348	2.37%	0.680%
10	10.105	1507	1512	1522	rBV	1202898	1657840	37.95%	10.910%
11	11.135	1675	1681	1690	rBV	984695	1308834	29.96%	8.613%
12	12.074	1829	1835	1843	rBV	1419916	1704022	39.01%	11.214%


Sum of corrected areas: 15195356

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX030520\
Data File : VX015108.D
Acq On : 05 Mar 2020 13:48
Operator : JC/SP
Sample : L1812-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-TANK -030420

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

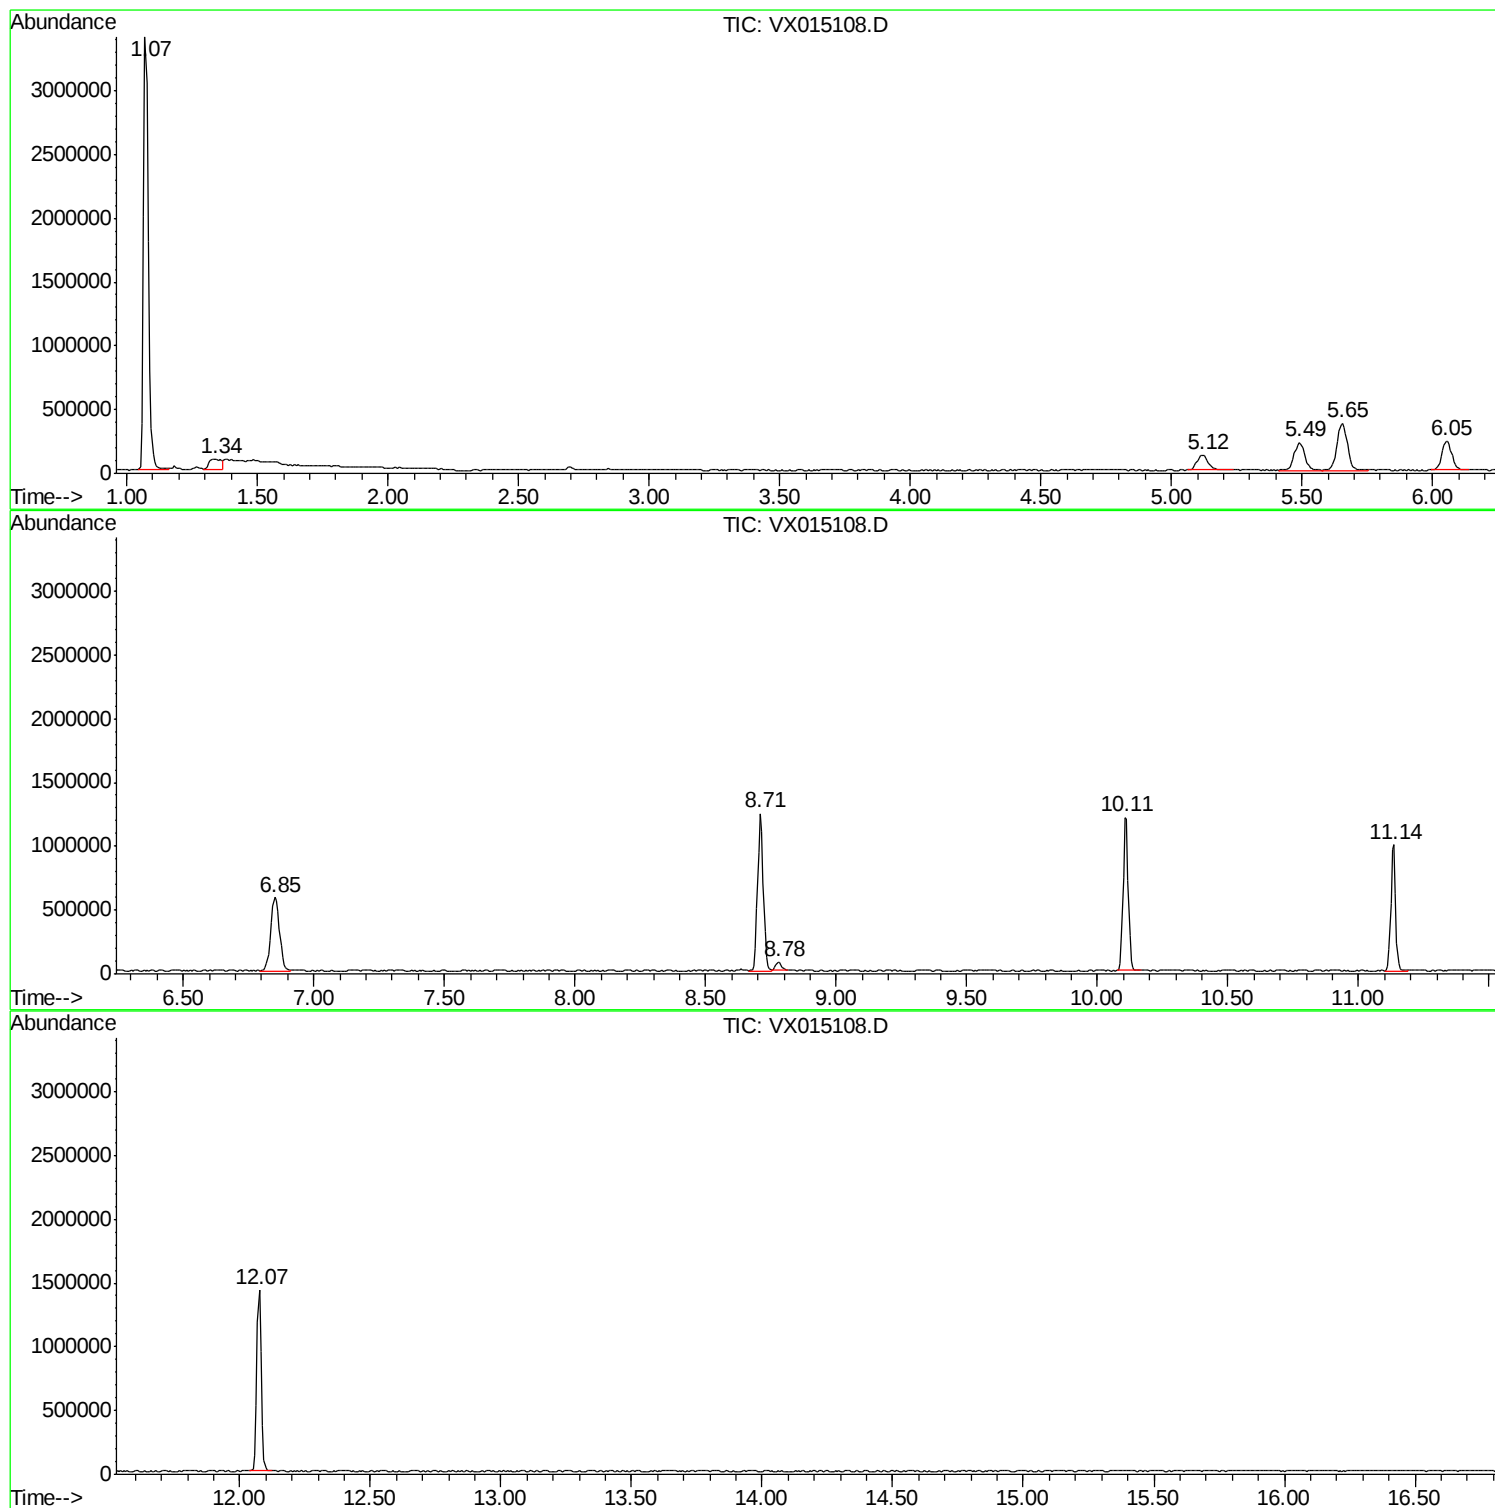

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX030520\
Data File : VX015108.D
Acq On : 05 Mar 2020 13:48
Operator : JC/SP
Sample : L1812-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-TANK -030420










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Sulfur dioxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.34	12.95 ug/l	262784	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Sulfur dioxide	64	O2S	007446-09-5	83
2		2-Aminoethyl hydrogen sulfate	141	C2H7N04S	000926-39-6	74
3		Aminomethanesulfonic acid	111	CH5N03S	013881-91-9	74
4		L-Alanine, 3-sulfo-	169	C3H7N05S	000498-40-8	64
5		Dibenzo[cd,g]indazole-3-sulfonic...	300	C14H8N2O4S	293765-87-4	64

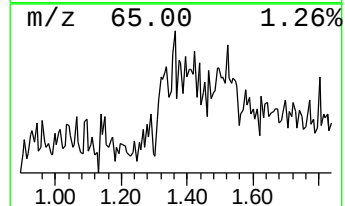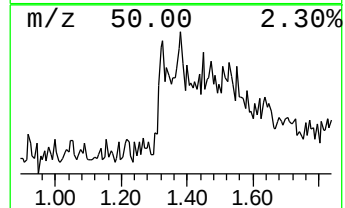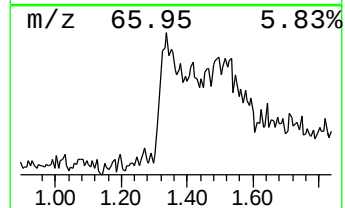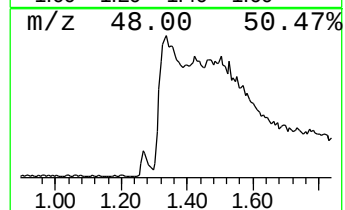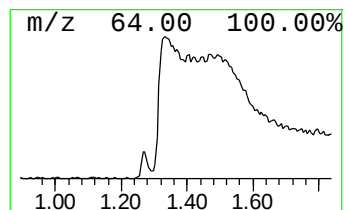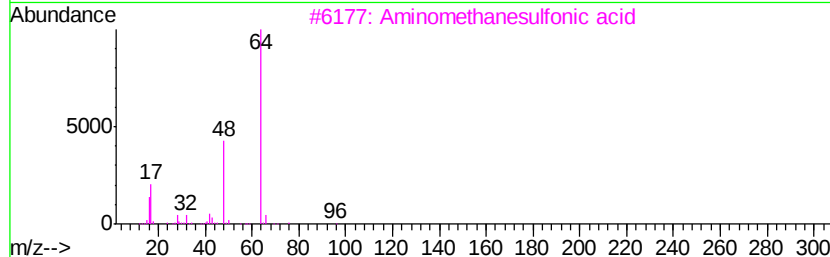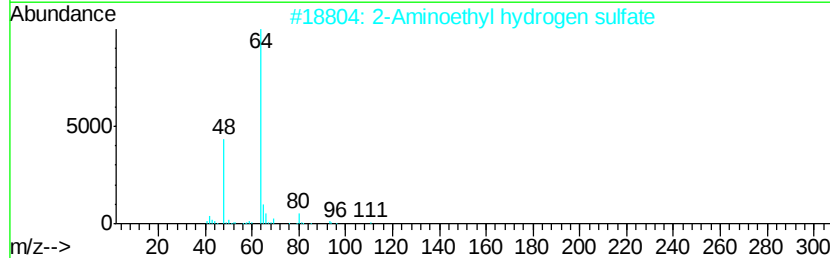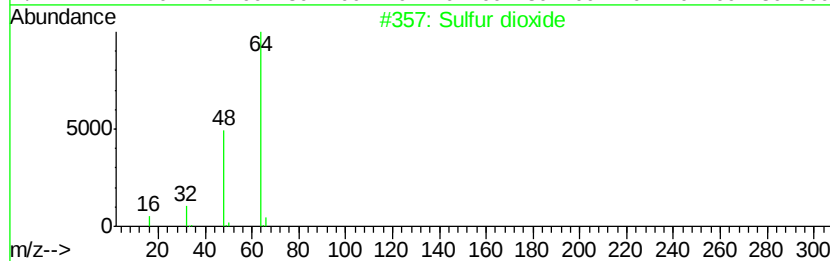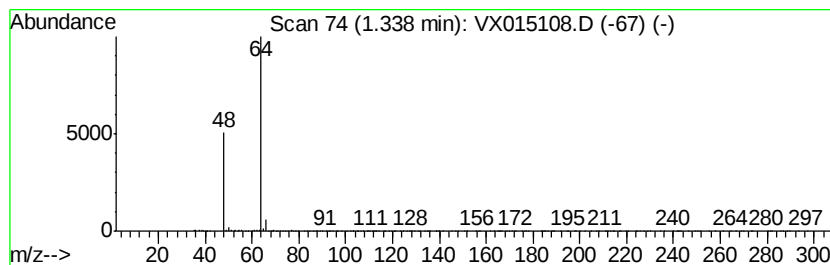

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX030520\
Data File : VX015108.D
Acq On : 05 Mar 2020 13:48
Operator : JC/SP
Sample : L1812-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WASTE-TANK -030420

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X030420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.34	12.9	ug/l	262784	1	5.65	1014790	50.0