
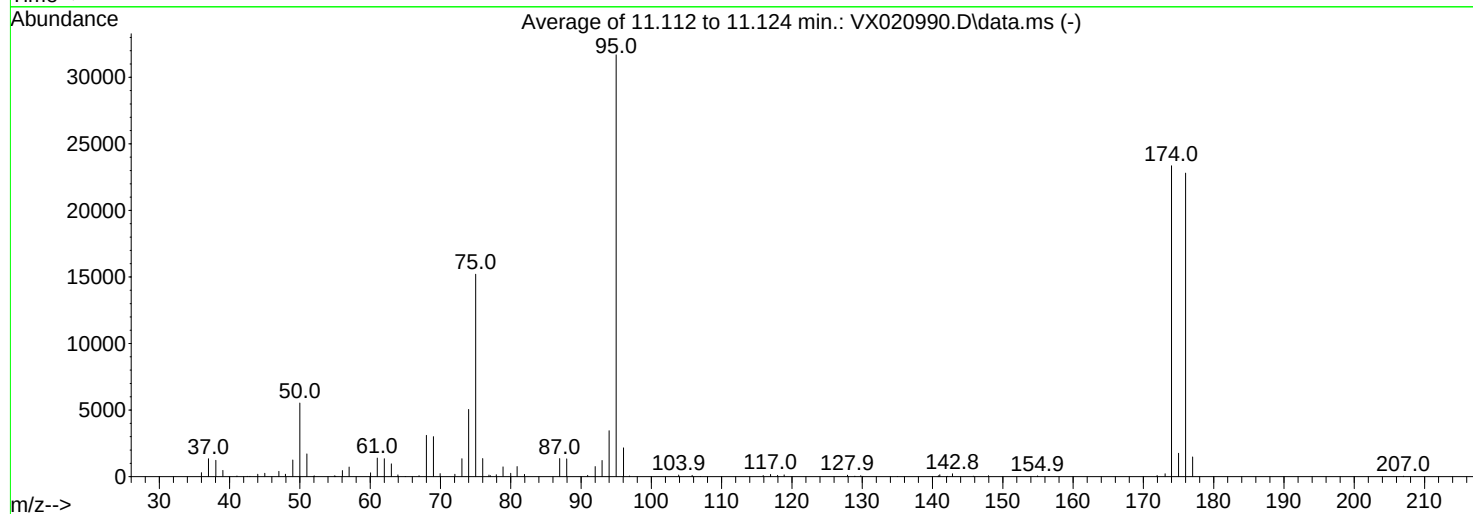


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030521\
Data File : VX020990.D
Acq On : 03 Mar 2021 09:40
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Title : SW846 8260
Last Update : Wed Feb 24 13:50:55 2021

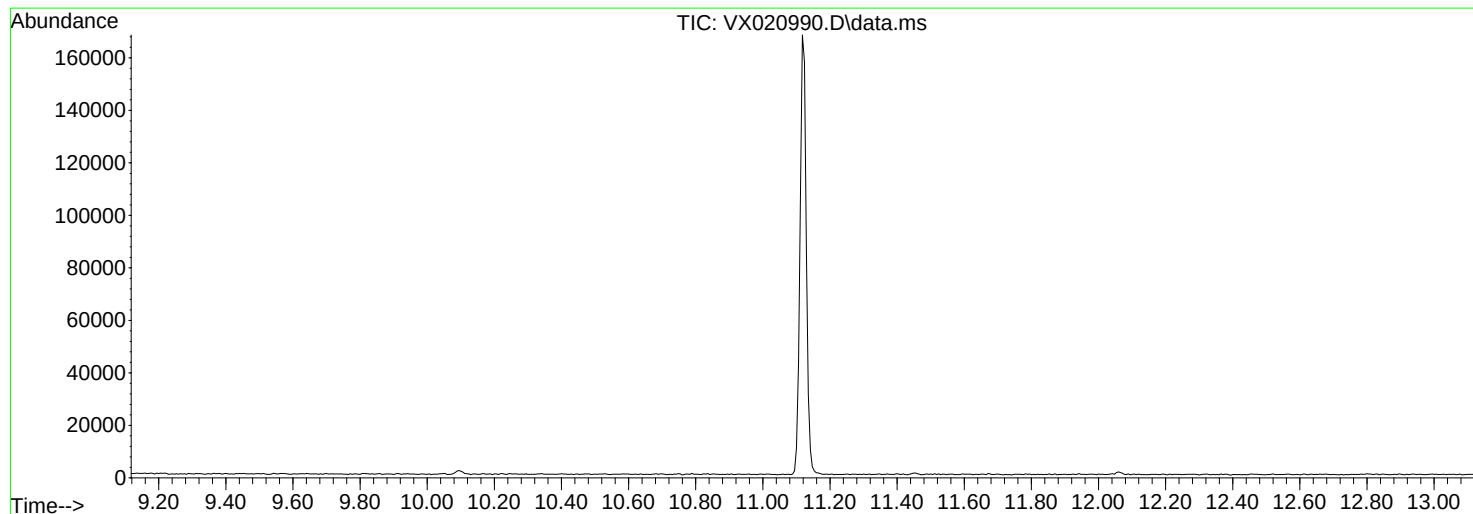

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	5534	PASS
75	95	30	60	48.0	15209	PASS
95	95	100	100	100.0	31688	PASS
96	95	5	9	6.9	2171	PASS
173	174	0.00	2	0.9	216	PASS
174	95	50	100	73.7	23359	PASS
175	174	5	9	7.5	1754	PASS
176	174	95	101	97.6	22800	PASS
177	176	5	9	6.5	1480	PASS