
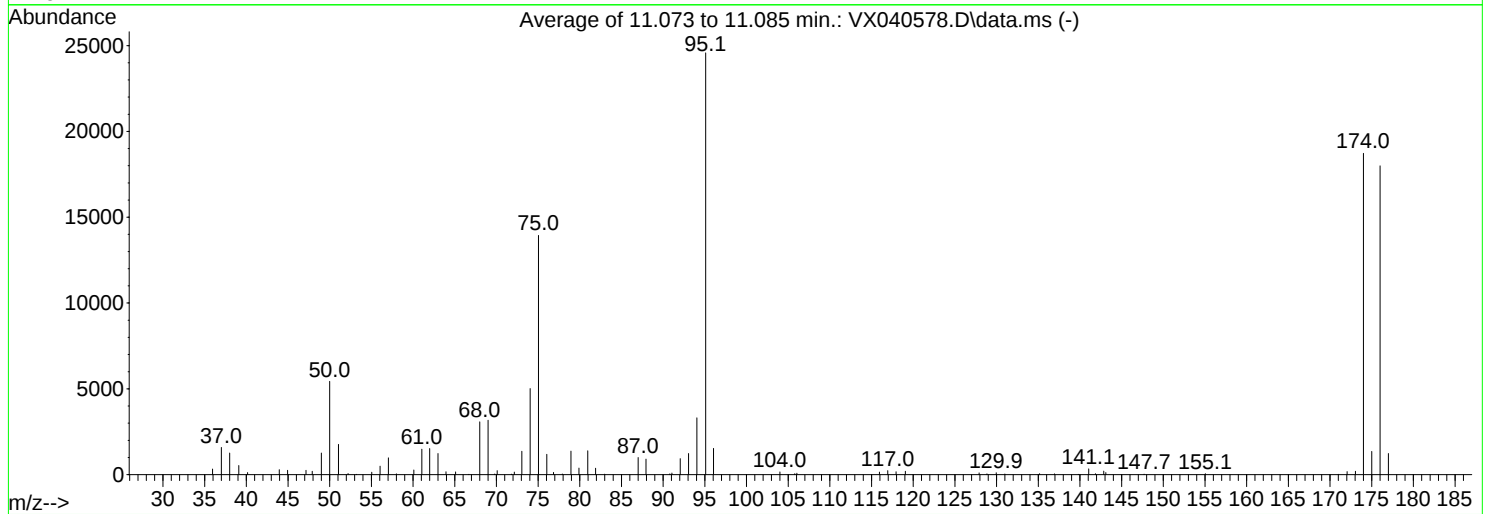


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030524\
Data File : VX040578.D
Acq On : 05 Mar 2024 08:37
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X030524W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Mar 05 13:21:29 2024

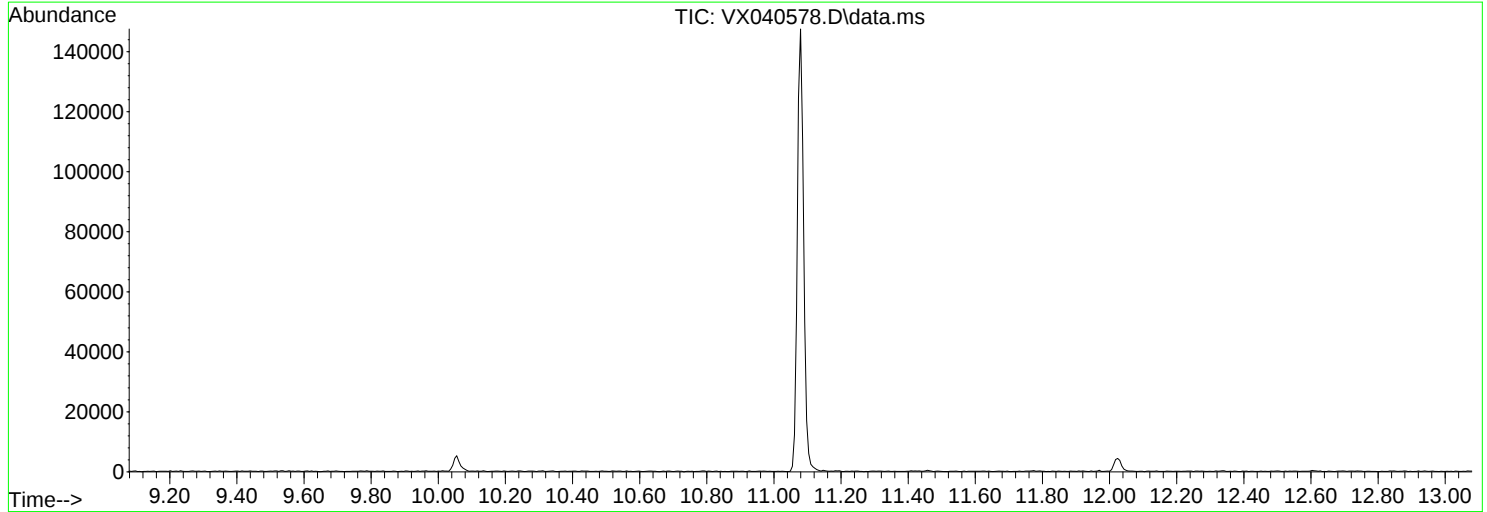

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.1	5434	PASS
75	95	30	60	56.7	13941	PASS
95	95	100	100	100.0	24579	PASS
96	95	5	9	6.2	1528	PASS
173	174	0.00	2	1.0	192	PASS
174	95	50	100	76.2	18723	PASS
175	174	5	9	7.2	1353	PASS
176	174	95	101	96.1	17999	PASS
177	176	5	9	6.8	1232	PASS