

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030621\
 Data File : VX021015.D
 Acq On : 04 Mar 2021 15:36
 Operator : JC/MD
 Sample : M1552-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 435-416

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M

Title : SW846 8260

Signal : TIC: VX021015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.417	220	226	236	rBV	23587	39617	2.95%	0.575%
2	2.576	245	253	261	rBV	7094	16176	1.21%	0.235%
3	5.464	732	744	759	rBV2	145519	415588	30.98%	6.029%
4	5.629	760	772	790	rVB	230413	638280	47.58%	9.259%
5	6.029	828	840	858	rBV	159840	419329	31.26%	6.083%
6	6.829	965	976	998	rBV	388825	933837	69.61%	13.546%
7	8.618	1272	1280	1286	rBV	16805	27383	2.04%	0.397%
8	8.694	1286	1293	1316	rVV	861007	1341445	100.00%	19.459%
9	10.094	1525	1531	1549	rVB	859803	1161361	86.58%	16.847%
10	11.118	1699	1705	1717	rBV	660287	852401	63.54%	12.365%
11	12.059	1859	1865	1872	rBV	814485	1010685	75.34%	14.661%
12	12.253	1893	1898	1906	rBV	22020	37609	2.80%	0.546%




Sum of corrected areas: 6893711

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030621\
Data File : VX021015.D
Acq On : 04 Mar 2021 15:36
Operator : JC/MD
Sample : M1552-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
435-416

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

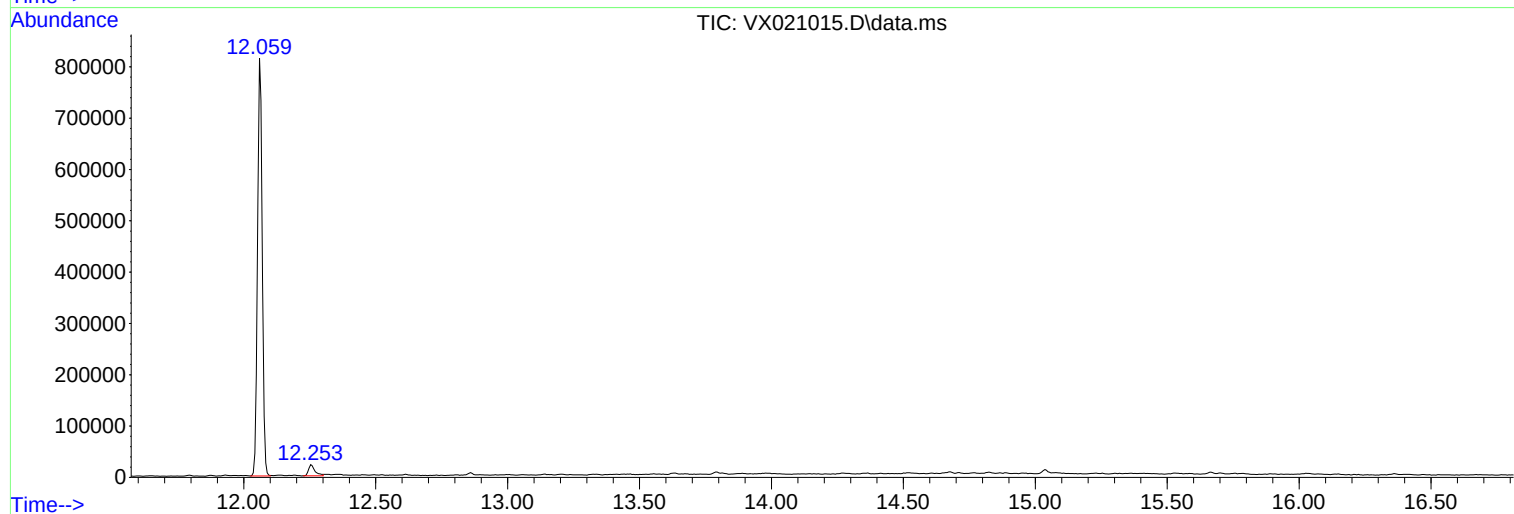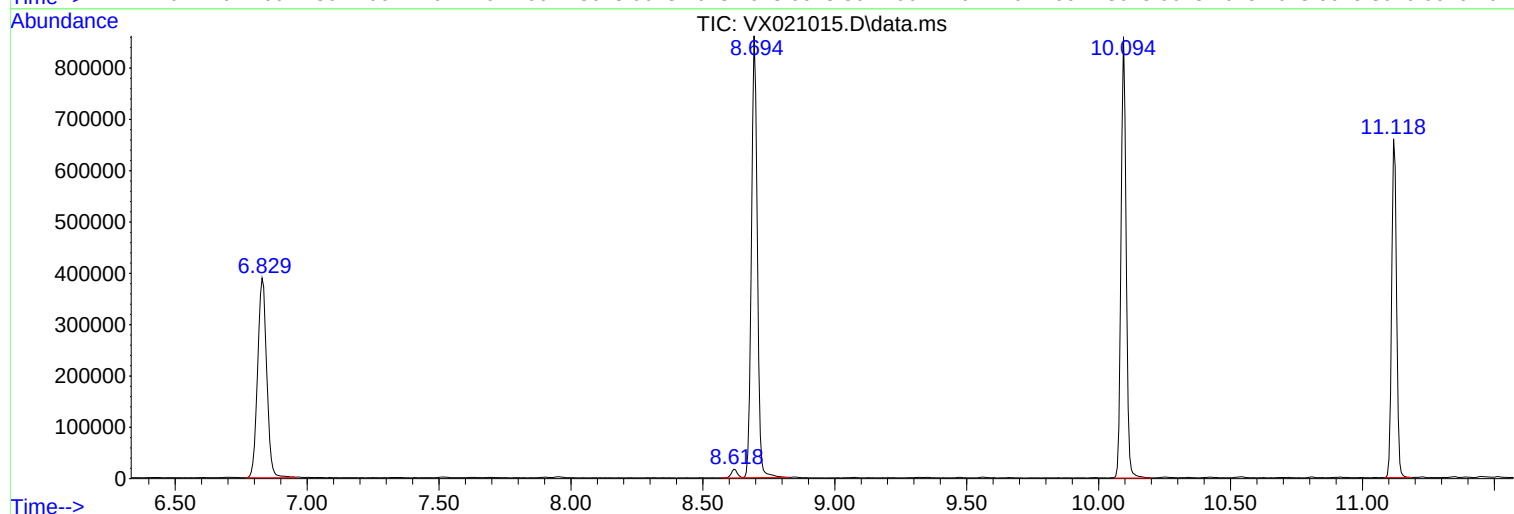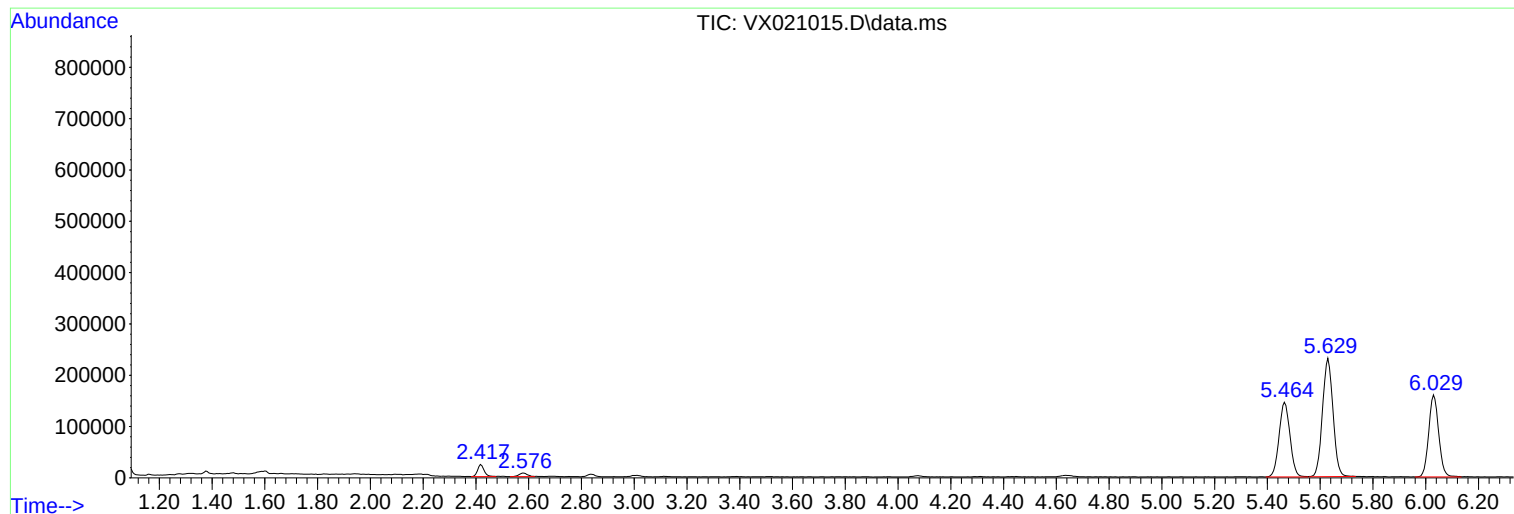

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030621\
Data File : VX021015.D
Acq On : 04 Mar 2021 15:36
Operator : JC/MD
Sample : M1552-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
435-416

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030621\
Data File : VX021015.D
Acq On : 04 Mar 2021 15:36
Operator : JC/MD
Sample : M1552-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
435-416

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------