
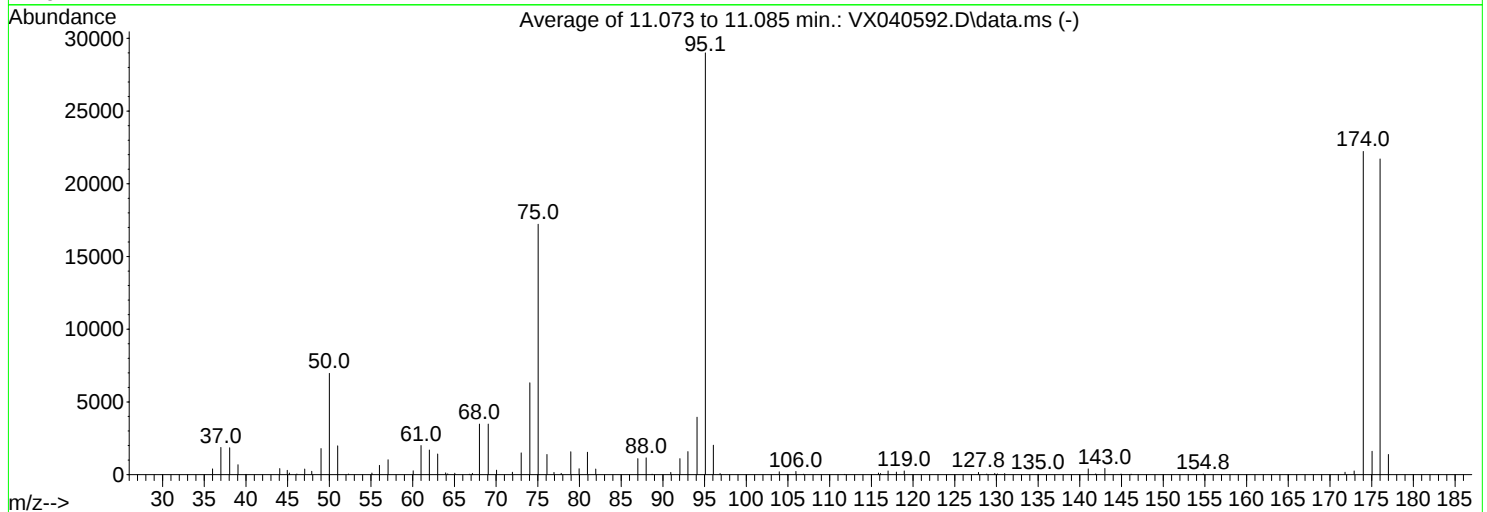


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030624\
Data File : VX040592.D
Acq On : 06 Mar 2024 08:20
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X030524W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Mar 05 13:21:29 2024

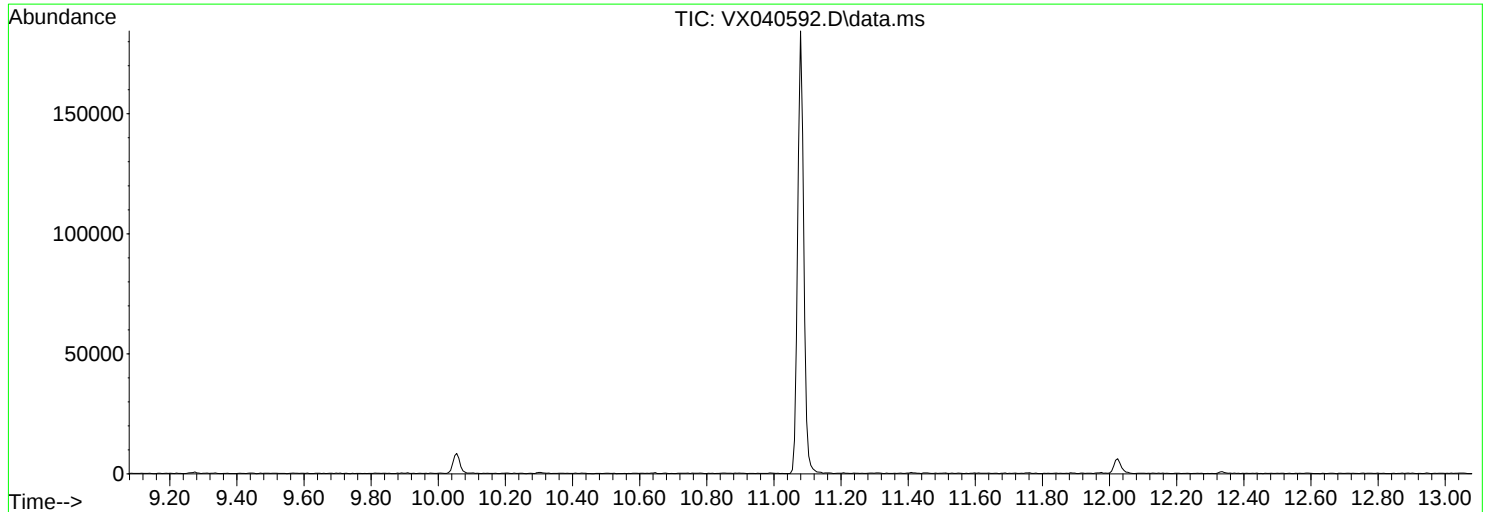

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.0	6966	PASS
75	95	30	60	59.4	17223	PASS
95	95	100	100	100.0	29005	PASS
96	95	5	9	7.0	2028	PASS
173	174	0.00	2	1.1	250	PASS
174	95	50	100	76.6	22227	PASS
175	174	5	9	7.2	1602	PASS
176	174	95	101	97.7	21709	PASS
177	176	5	9	6.4	1386	PASS