

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX030719\
 Data File : VX007878.D
 Acq On : 07 Mar 2019 12:36
 Operator : JC/SP
 Sample : K1560-09
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030619W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.642	67	80	85	rBV5	8671	24491	1.92%	0.333%
2	2.294	181	187	195	rBV	8936	15577	1.22%	0.212%
3	2.385	196	202	207	rVB4	7111	12836	1.01%	0.174%
4	2.513	218	223	229	rBV	8434	14499	1.14%	0.197%
5	3.056	309	312	321	rVB	7201	14837	1.16%	0.202%
6	3.154	322	328	335	rBV3	7569	22363	1.75%	0.304%
7	3.818	429	437	456	rVB2	12529	43950	3.44%	0.597%
8	4.592	554	564	574	rBV9	4831	15483	1.21%	0.210%
9	5.153	648	656	662	rBV3	4558	13218	1.04%	0.180%
10	5.501	700	713	729	rBV2	157751	461334	36.14%	6.269%
11	5.659	729	739	754	rVV	272974	775202	60.73%	10.535%
12	5.793	755	761	771	rVB9	4953	15069	1.18%	0.205%
13	6.068	794	806	815	rBV	167134	440561	34.52%	5.987%
14	6.860	925	936	949	rBV	395737	936040	73.33%	12.721%
15	7.458	1027	1034	1039	rBV5	6040	13537	1.06%	0.184%
16	8.311	1168	1174	1185	rBV	11346	19715	1.54%	0.268%
17	8.646	1224	1229	1233	rBV	18571	28503	2.23%	0.387%
18	8.713	1233	1240	1248	rVV	830994	1276400	100.00%	17.346%
19	8.781	1248	1251	1265	rVB	12576	22994	1.80%	0.312%
20	9.335	1334	1342	1345	rBV	8837	13891	1.09%	0.189%
21	9.494	1364	1368	1378	rBV	13372	19880	1.56%	0.270%
22	10.110	1463	1469	1480	rBV	769471	1054582	82.62%	14.331%
23	10.250	1489	1492	1500	rVB	12649	16983	1.33%	0.231%
24	10.360	1505	1510	1516	rVB	20876	29707	2.33%	0.404%
25	10.701	1560	1566	1575	rBV3	13450	26256	2.06%	0.357%
26	11.018	1612	1618	1623	rBV	13135	16117	1.26%	0.219%
27	11.134	1632	1637	1648	rBV	639437	822755	64.46%	11.181%
28	11.256	1652	1657	1661	rBV3	10702	18590	1.46%	0.253%
29	11.359	1670	1674	1678	rVV	12637	16032	1.26%	0.218%
30	11.420	1680	1684	1688	rVB2	11023	13717	1.07%	0.186%
31	11.506	1694	1698	1705	rVB2	20236	27268	2.14%	0.371%
32	11.768	1734	1741	1745	rBV3	16762	25379	1.99%	0.345%
33	11.804	1745	1747	1753	rVB	12093	13501	1.06%	0.183%
34	11.945	1764	1770	1776	rBV	11050	14565	1.14%	0.198%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX030719\
Data File : VX007878.D
Acq On : 07 Mar 2019 12:36
Operator : JC/SP
Sample : K1560-09
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030619W.M
Title : SW846 8260

35	12.024	1778	1783	1786	rBV	9957	12823	1.00%	0.174%
36	12.079	1786	1792	1805	rVB	776071	1010765	79.19%	13.736%
37	12.390	1838	1843	1849	rVB	20002	25997	2.04%	0.353%
38	13.341	1994	1999	2006	rVB2	10057	13083	1.02%	0.178%


Sum of corrected areas: 7358500

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX030719\
Data File : VX007878.D
Acq On : 07 Mar 2019 12:36
Operator : JC/SP
Sample : K1560-09
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X030619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

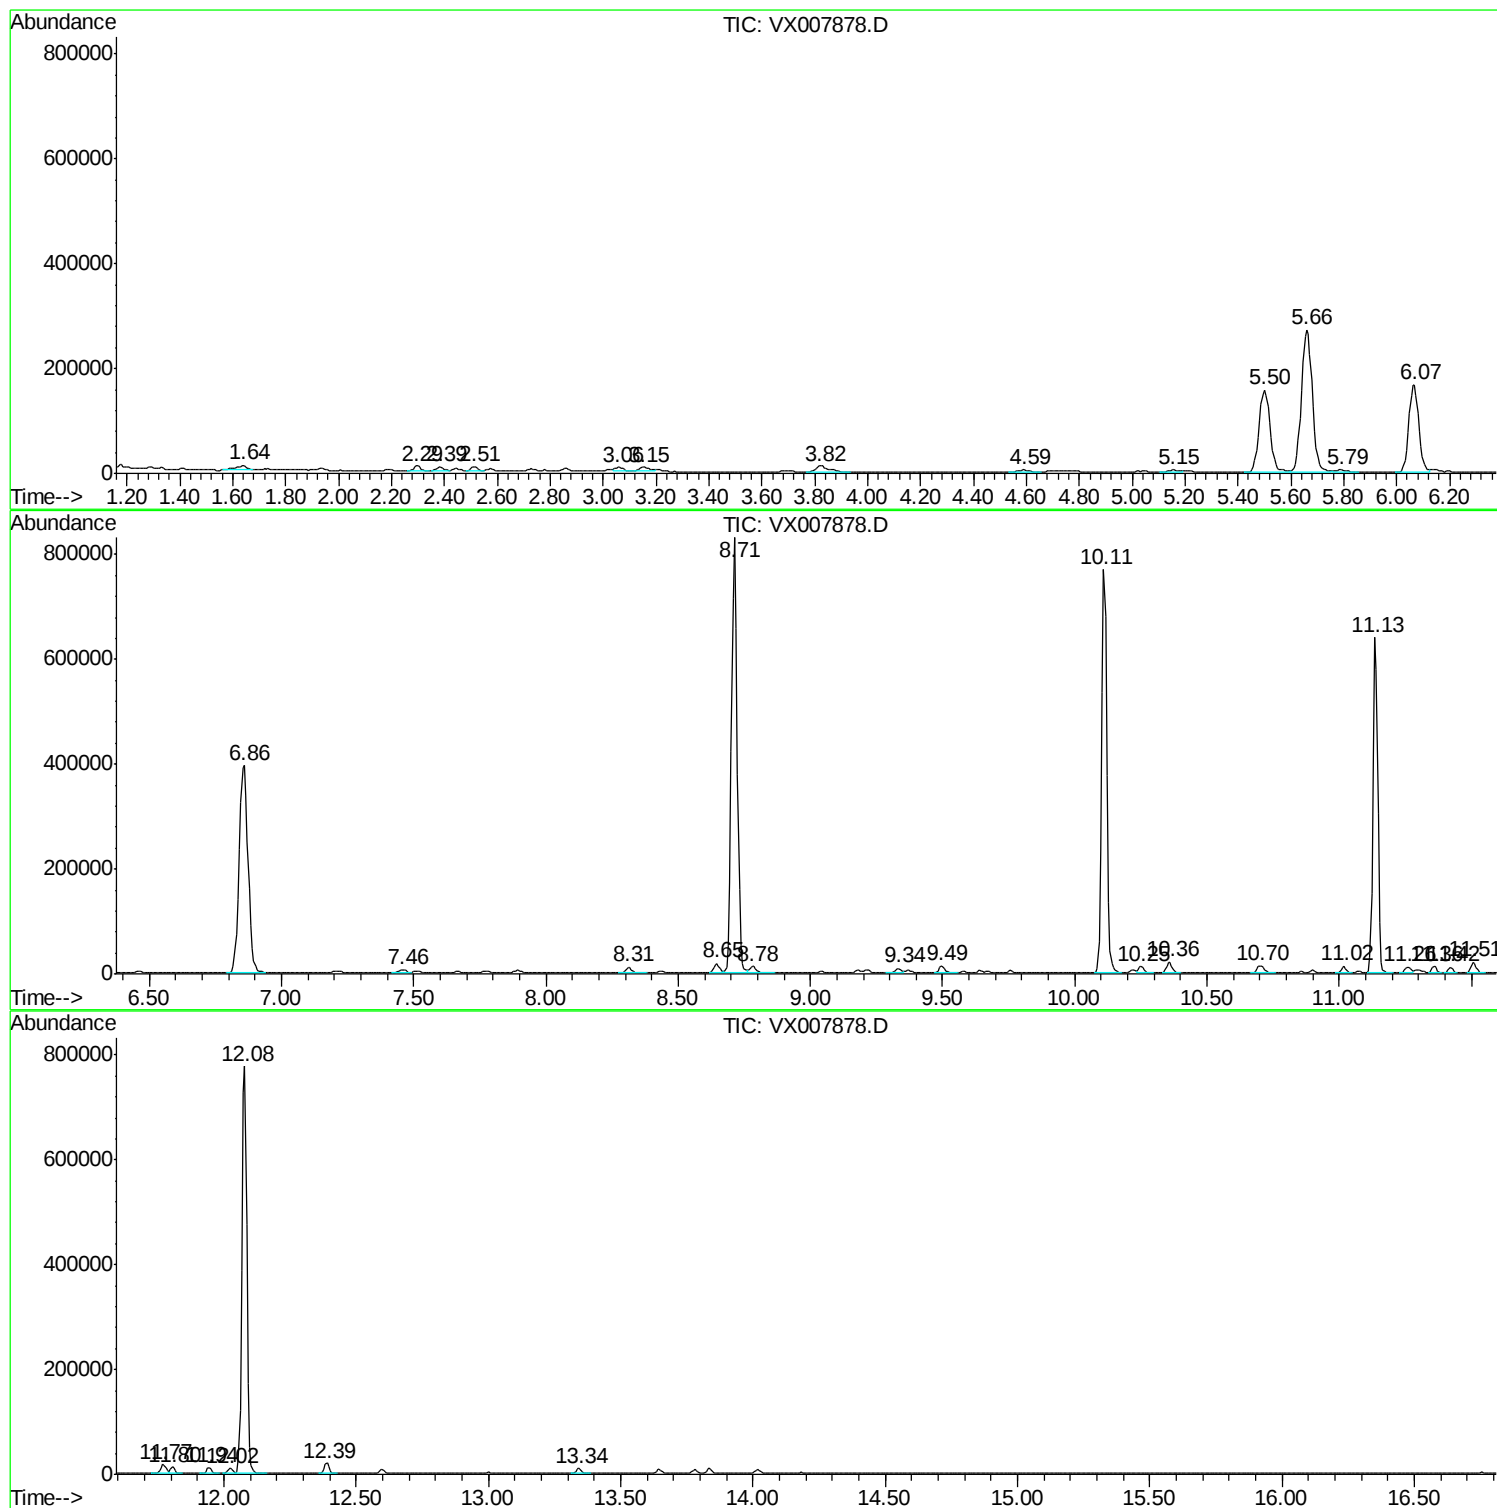

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX030719\
Data File : VX007878.D
Acq On : 07 Mar 2019 12:36
Operator : JC/SP
Sample : K1560-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X030619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX030719\
Data File : VX007878.D
Acq On : 07 Mar 2019 12:36
Operator : JC/SP
Sample : K1560-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X030619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc