


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX030719\
 Data File : VX007897.D
 Acq On : 07 Mar 2019 21:37
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X030619W.M
 Title : SW846 8260
 Last Update : Thu Mar 07 07:33:26 2019

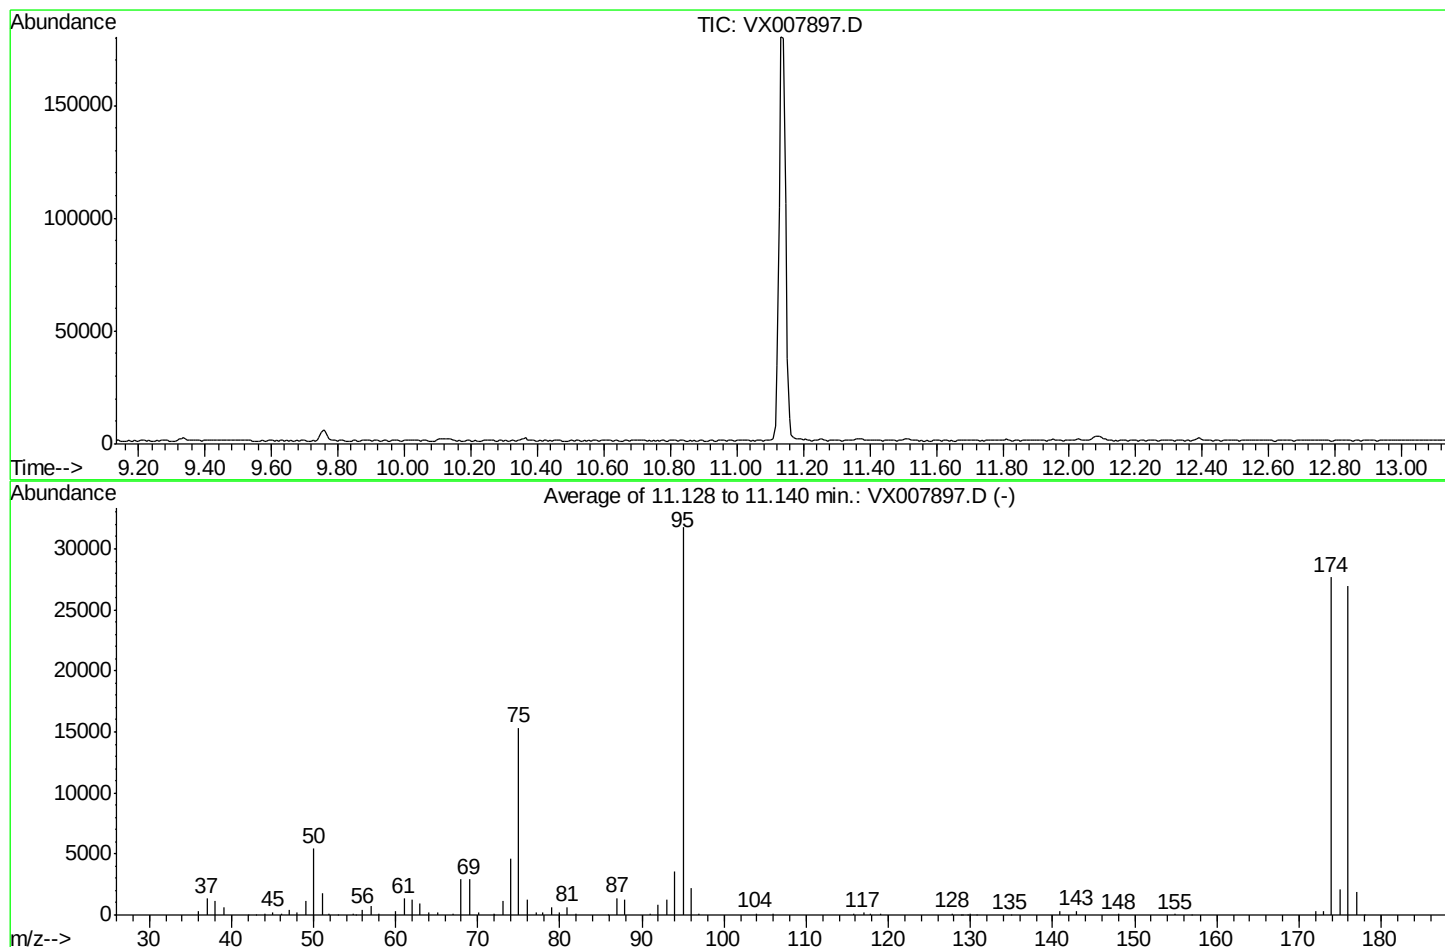

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	5446	PASS
75	95	30	60	48.2	15323	PASS
95	95	100	100	100.0	31762	PASS
96	95	5	9	6.9	2189	PASS
173	174	0.00	2	1.1	313	PASS
174	95	50	100	87.1	27680	PASS
175	174	5	9	7.6	2093	PASS
176	174	95	101	97.2	26912	PASS
177	176	5	9	6.9	1845	PASS