

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030721\
 Data File : VX021043.D
 Acq On : 05 Mar 2021 18:20
 Operator : JC/MD
 Sample : M1575-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IDW-GW806-AQ-030321

Quant Time: Mar 06 00:01:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 24 13:50:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.629	168	208936	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	391892	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	377313	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.065	152	170565	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	140320	49.72	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	99.44%		
35) Dibromofluoromethane	5.464	113	122347	51.38	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	102.76%		
50) Toluene-d8	8.694	98	488270	52.59	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	105.18%		
62) 4-Bromofluorobenzene	11.118	95	187716	54.68	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	109.36%		
Target Compounds						Qvalue
5) Bromomethane	1.640	94	197	Below Cal		86
11) Tert butyl alcohol	3.005	59	550	0.88 ug/l #		73
12) 1,1-Dichloroethene	2.358	96	915	0.39 ug/l		98
13) Acrolein	2.275	56	98	0.25 ug/l #		79
16) Acetone	2.417	43	11364	9.77 ug/l		100
18) Methyl Acetate	2.746	43	655	0.24 ug/l #		60
20) Methylene Chloride	2.840	84	890	0.32 ug/l #		82
25) 2-Butanone	4.640	43	2729	1.54 ug/l		93
27) cis-1,2-Dichloroethene	4.564	96	2862	0.95 ug/l		99
28) Bromochloromethane	5.170	49	5806	3.00 ug/l #		9
30) Chloroform	5.176	83	76610	16.80 ug/l		99
31) Cyclohexane	5.629	56	3934	0.96 ug/l #		1
36) 1,1-Dichloropropene	5.623	75	16041	4.31 ug/l #		48
37) Ethyl Acetate	4.640	43	2729	0.77 ug/l #		64
38) Carbon Tetrachloride	5.629	117	19955	5.53 ug/l #		17
42) 1,2-Dichloroethane	6.158	62	969	0.26 ug/l #		73
44) Trichloroethene	7.182	130	688	0.23 ug/l		96
46) Dibromomethane	7.876	93	529	0.28 ug/l #		2
47) Bromodichloromethane	7.876	83	19777	5.04 ug/l		99
48) Methyl methacrylate	7.635	41	1632	0.54 ug/l #		35
49) 1,4-Dioxane	7.723	88	68	0.96 ug/l #		1
51) 4-Methyl-2-Pentanone	8.617	43	2010	0.57 ug/l		97
52) Toluene	8.764	92	5153	0.74 ug/l		96
59) 2-Hexanone	9.470	43	779	0.30 ug/l		81
60) Dibromochloromethane	9.565	129	6388	2.20 ug/l		99
68) m/p-Xylenes	10.341	106	2538	0.48 ug/l		96
69) o-Xylene	10.682	106	1072	0.21 ug/l		98
74) N-amyl acetate	10.894	43	29778	5.46 ug/l #		1
76) 1,2,3-Trichloropropane	11.118	75	89718	24.45 ug/l #		39
81) trans-1,4-Dichloro-2-b...	11.118	75	89718	54.13 ug/l #		12
84) 1,2,4-Trimethylbenzene	11.788	105	2496	0.22 ug/l		90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030721\
Data File : VX021043.D
Acq On : 05 Mar 2021 18:20
Operator : JC/MD
Sample : M1575-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321

Quant Time: Mar 06 00:01:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 24 13:50:55 2021
Response via : Initial Calibration

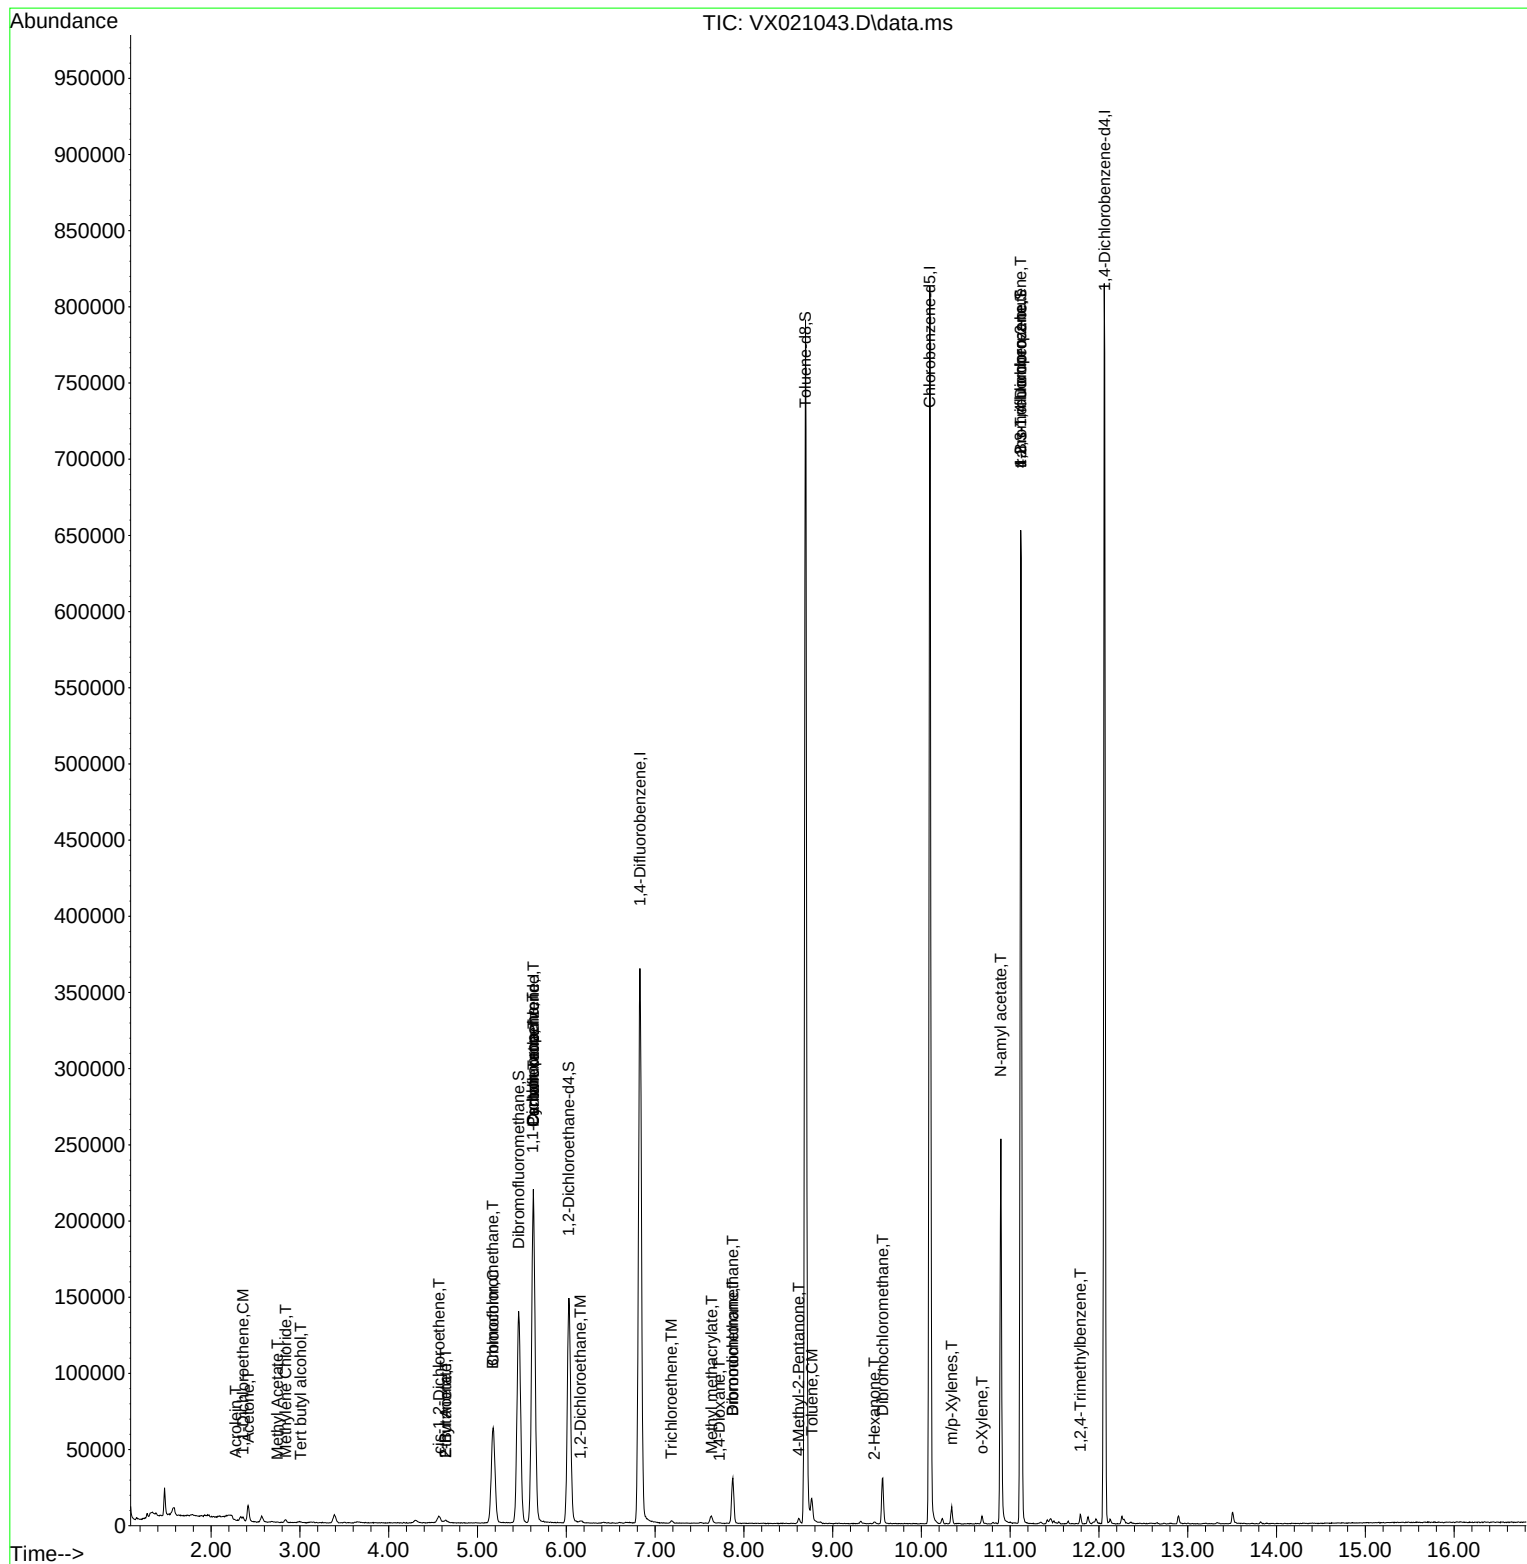



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.629 min Scan# 772

Delta R.T. 0.006 min

Lab File: VX021043.D





Acq: 05 Mar 2021 18:20

Tgt Ion: 168 Resp: 208936

Ion Ratio Lower Upper

168 100

99 55.5 45.8 68.6

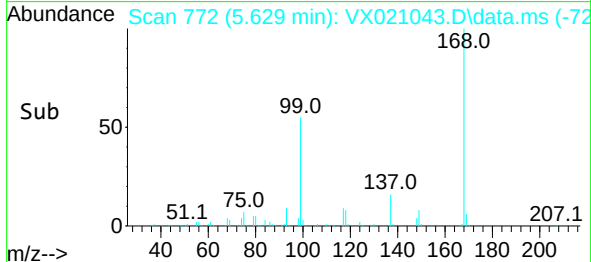

#5

Bromomethane

Concen: Below Cal

RT: 1.640 min Scan# 94

Delta R.T. 0.017 min

Lab File: VX021043.D




Acq: 05 Mar 2021 18:20


Tgt Ion: 94 Resp: 197

Ion Ratio Lower Upper

94 100

96 109.6 76.4 114.6




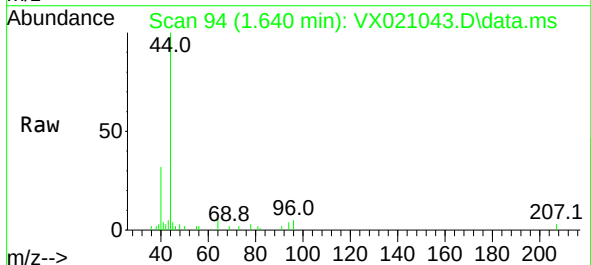




#11
Tert butyl alcohol
Concen: 0.88 ug/l
RT: 3.005 min Scan# 326
Delta R.T. -0.012 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion: 59 Resp: 550
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

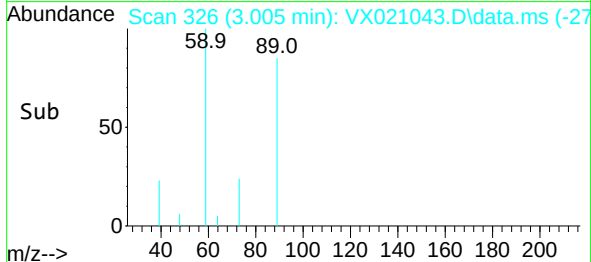

#12
1,1-Dichloroethene
Concen: 0.39 ug/l
RT: 2.358 min Scan# 216
Delta R.T. 0.006 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 96 Resp: 915
Ion Ratio Lower Upper
96 100
61 152.8 124.6 187.0
98 61.5 50.6 76.0




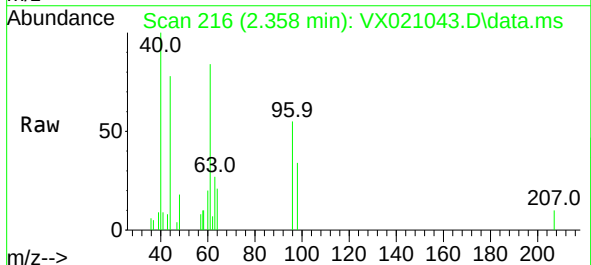




#13
Acrolein
Concen: 0.25 ug/l
RT: 2.275 min Scan# 202
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion: 56 Resp: 98
Ion Ratio Lower Upper
56 100
55 53.1 56.4 84.6#

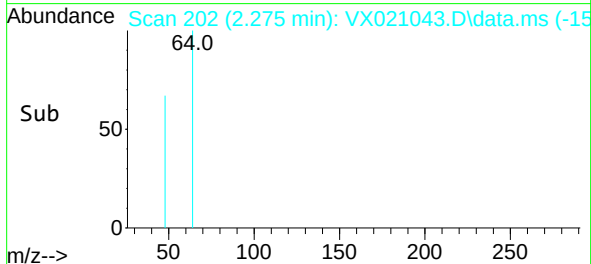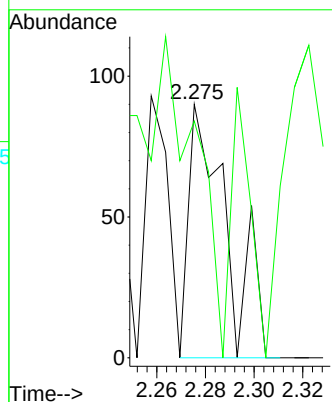

#16
Acetone
Concen: 9.77 ug/l
RT: 2.417 min Scan# 226
Delta R.T. -0.006 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 43 Resp: 11364
Ion Ratio Lower Upper
43 100
58 34.8 27.8 41.8



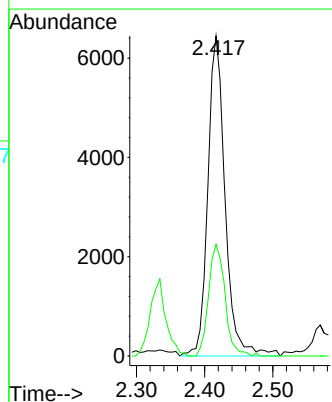



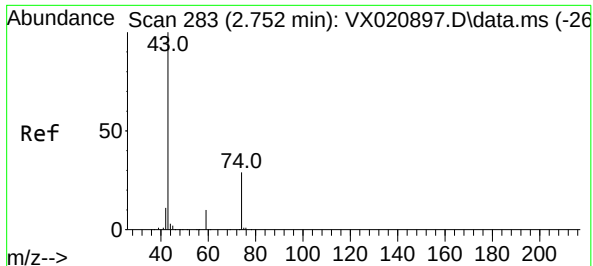

#18
Methyl Acetate
Concen: 0.24 ug/l
RT: 2.746 min Scan# 282
Delta R.T. -0.006 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion: 43 Resp: 655
Ion Ratio Lower Upper
43 100
74 6.6 21.9 32.9#

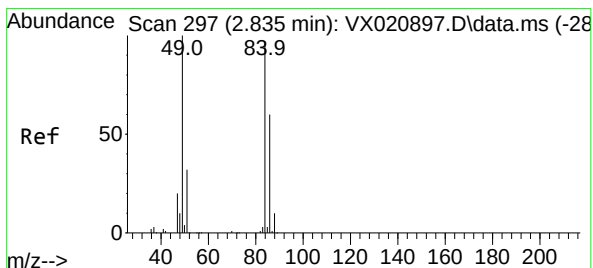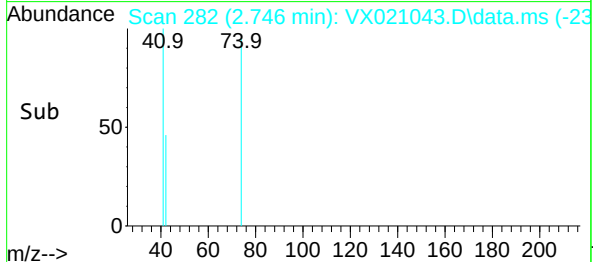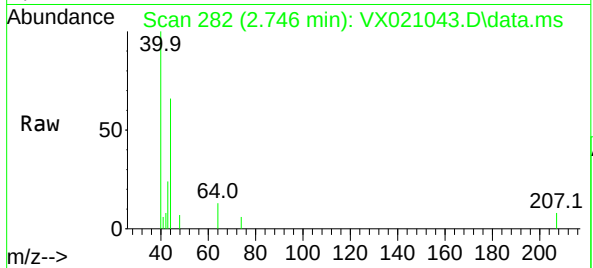

#20
Methylene Chloride
Concen: 0.32 ug/l
RT: 2.840 min Scan# 298
Delta R.T. 0.006 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 84 Resp: 890
Ion Ratio Lower Upper
84 100
49 95.2 88.6 132.8
51 21.8 27.0 40.6#
86 46.7 50.3 75.5#


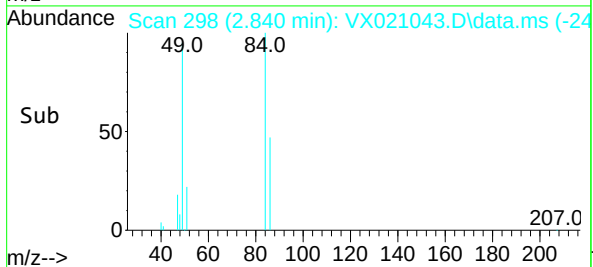

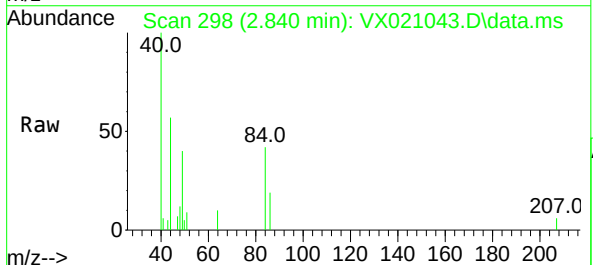


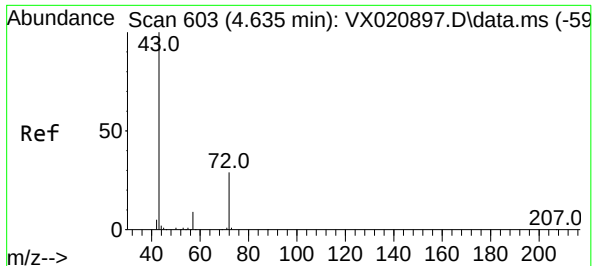

#25
2-Butanone
Concen: 1.54 ug/l
RT: 4.640 min Scan# 604
Delta R.T. 0.006 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion: 43 Resp: 2729
Ion Ratio Lower Upper
43 100
72 26.0 23.7 35.5

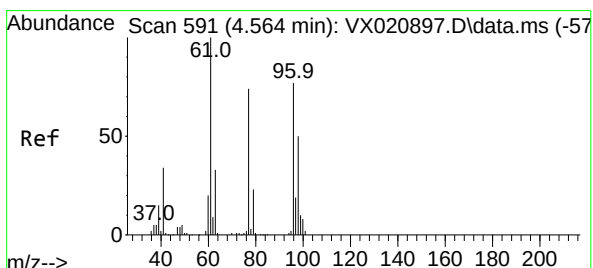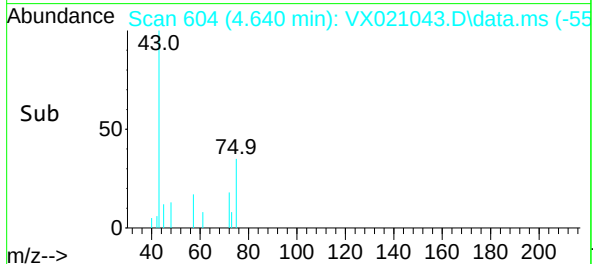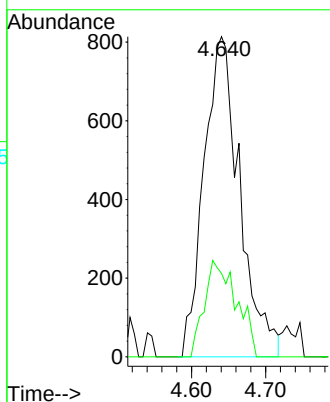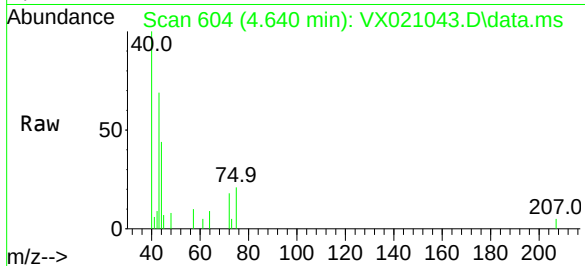

#27
cis-1,2-Dichloroethene
Concen: 0.95 ug/l
RT: 4.564 min Scan# 591
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 96 Resp: 2862
Ion Ratio Lower Upper
96 100
61 141.9 0.0 285.6
98 63.8 0.0 129.6


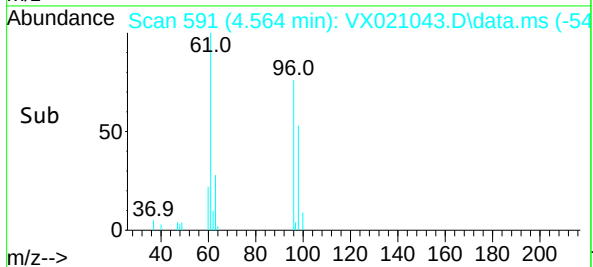
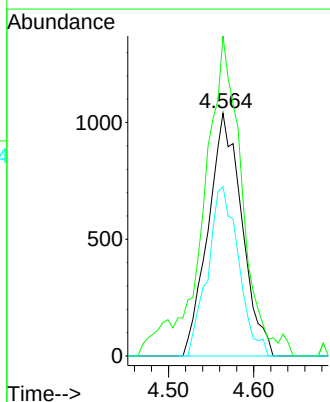
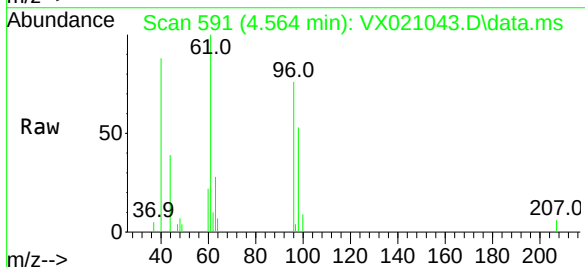


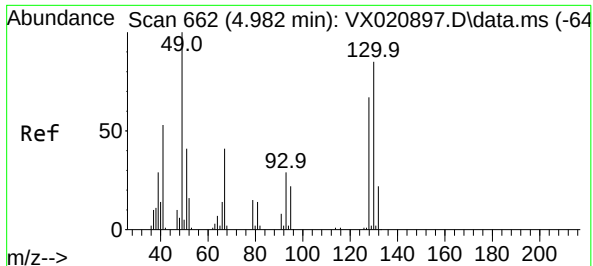

#28
Bromochloromethane
Concen: 3.00 ug/l
RT: 5.170 min Scan# 694
Delta R.T. 0.188 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion: 49 Resp: 5806
Ion Ratio Lower Upper
49 100
129 0.0 0.0 4.0
130 0.0 68.2 102.2#

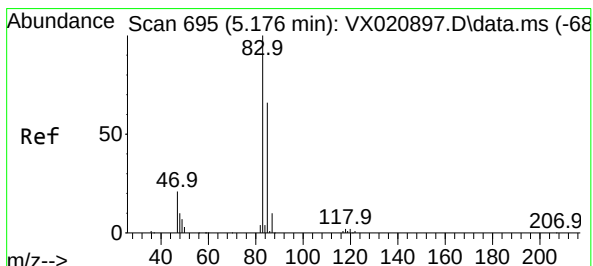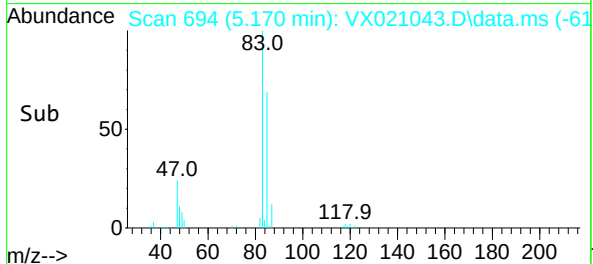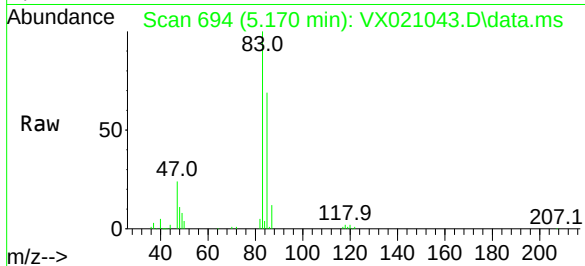

#30
Chloroform
Concen: 16.80 ug/l
RT: 5.176 min Scan# 695
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20


Tgt Ion: 83 Resp: 76610
Ion Ratio Lower Upper
83 100
85 65.4 52.0 78.0

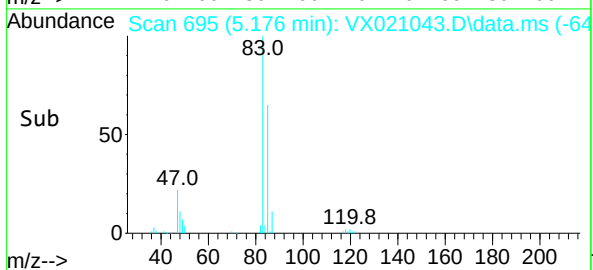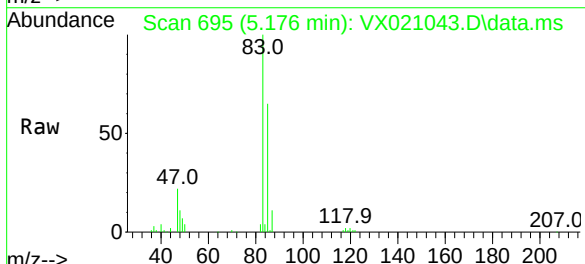






#31
Cyclohexane
Concen: 0.96 ug/l
RT: 5.629 min Scan# 772
Delta R.T. 0.082 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20


Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321





Tgt Ion: 56 Resp: 3934
Ion Ratio Lower Upper
56 100
69 193.3 25.3 37.9#
84 160.3 71.4 107.0#

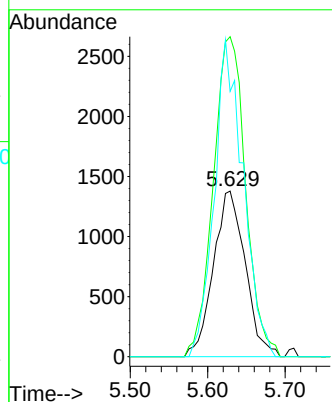


#33
1,2-Dichloroethane-d4
Concen: 49.72 ug/l
RT: 6.029 min Scan# 840
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Tgt Ion: 65 Resp: 140320
Ion Ratio Lower Upper
65 100
67 53.0 0.0 105.4

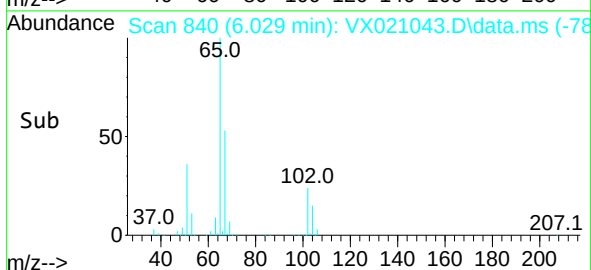






#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.829 min Scan# 976
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20


Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321





Tgt Ion:114 Resp: 391892
Ion Ratio Lower Upper
114 100
63 19.7 0.0 40.8
88 16.3 0.0 32.8

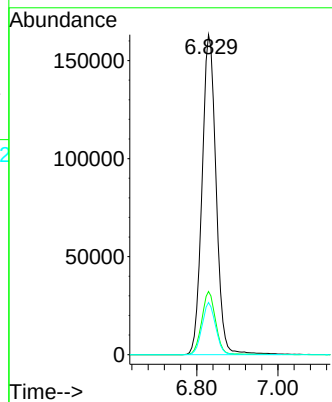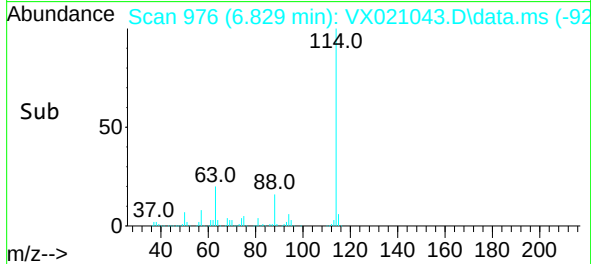


#35
Dibromofluoromethane
Concen: 51.38 ug/l
RT: 5.464 min Scan# 744
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

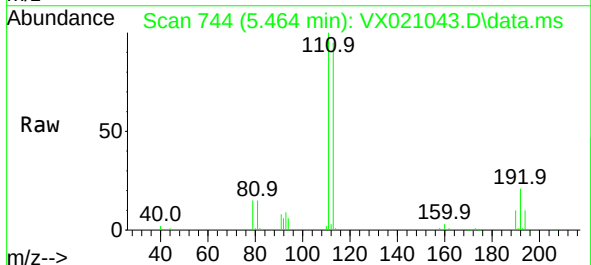


Tgt Ion:113 Resp: 122347
Ion Ratio Lower Upper
113 100
111 103.0 81.9 122.9
192 20.4 16.7 25.1








#36
1,1-Dichloropropene
Concen: 4.31 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.147 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321



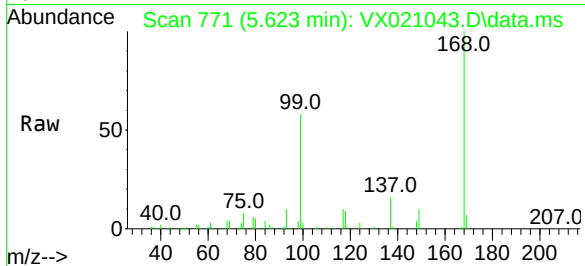



Tgt Ion: 75 Resp: 16041
Ion Ratio Lower Upper
75 100
110 8.2 18.1 54.4#
77 0.0 25.3 37.9#

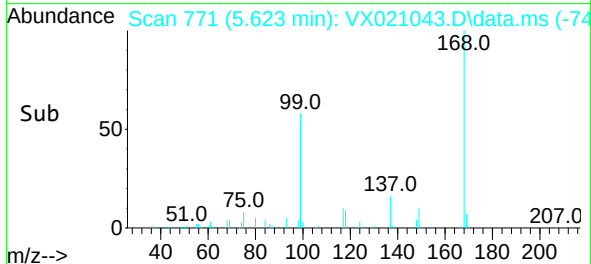

#37
Ethyl Acetate
Concen: 0.77 ug/l
RT: 4.640 min Scan# 604
Delta R.T. -0.153 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 43 Resp: 2729
Ion Ratio Lower Upper
43 100
61 0.0 12.8 19.2#
70 0.0 10.5 15.7#




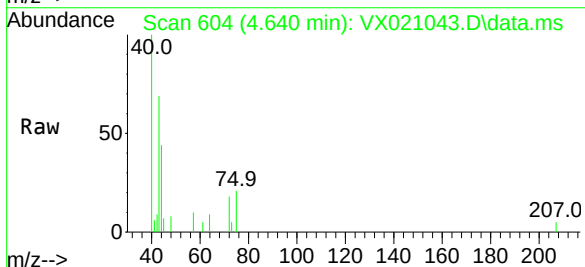


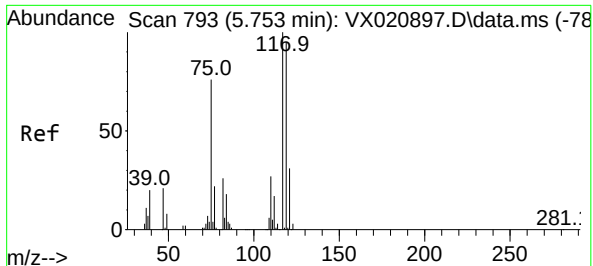

#38
Carbon Tetrachloride
Concen: 5.53 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.124 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion:117 Resp: 19955
Ion Ratio Lower Upper
117 100
119 5.7 76.2 114.2#
121 0.0 24.8 37.2#

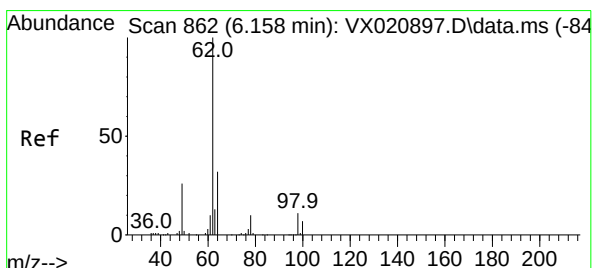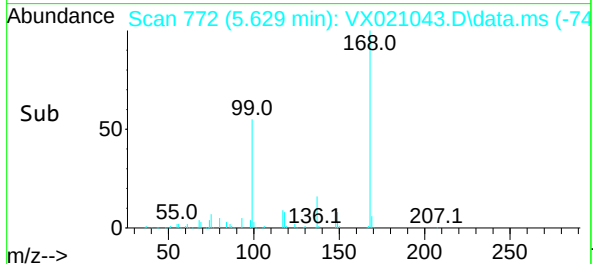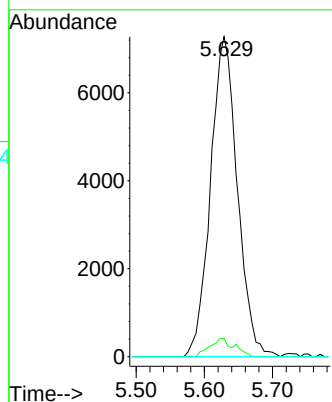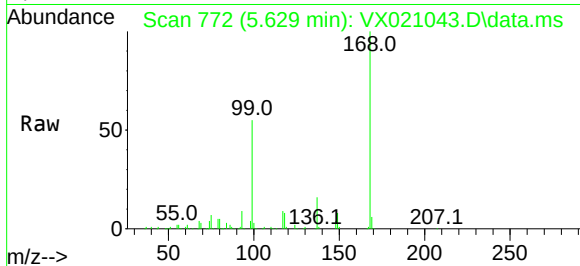

#42
1,2-Dichloroethane
Concen: 0.26 ug/l
RT: 6.158 min Scan# 862
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 62 Resp: 969
Ion Ratio Lower Upper
62 100
98 0.0 0.0 20.2


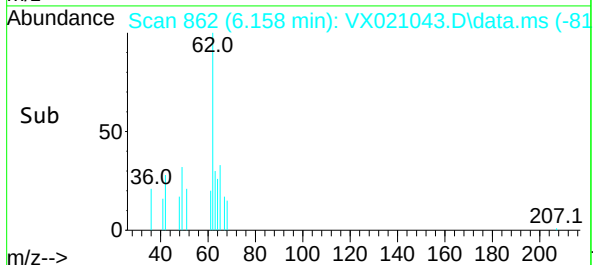

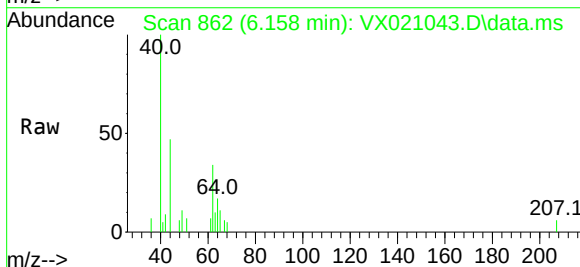


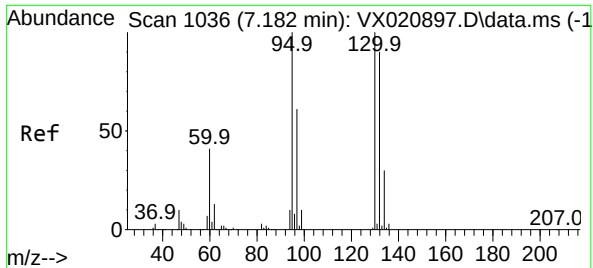

#44
Trichloroethene
Concen: 0.23 ug/l
RT: 7.182 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion:130 Resp: 688
Ion Ratio Lower Upper
130 100
95 95.1 0.0 198.0

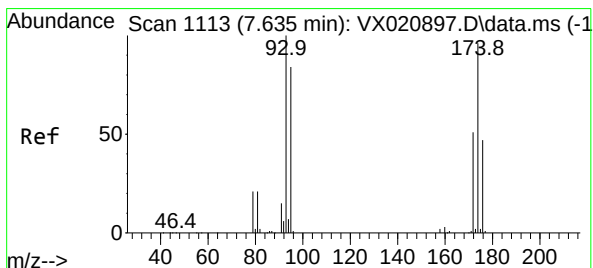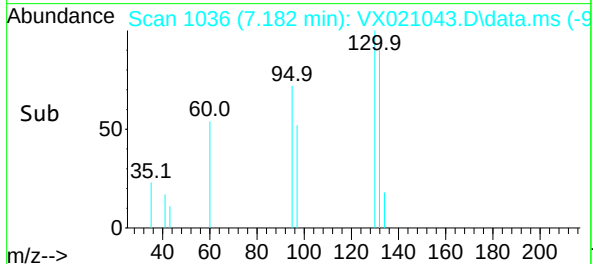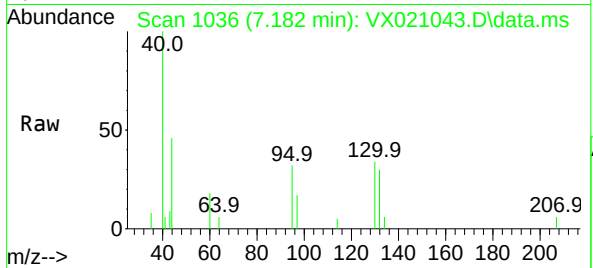

#46
Dibromomethane
Concen: 0.28 ug/l
RT: 7.876 min Scan# 1154
Delta R.T. 0.241 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 93 Resp: 529
Ion Ratio Lower Upper
93 100
95 0.0 66.8 100.2#
174 0.0 83.1 124.7#


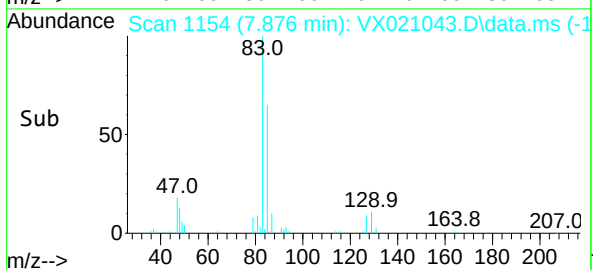

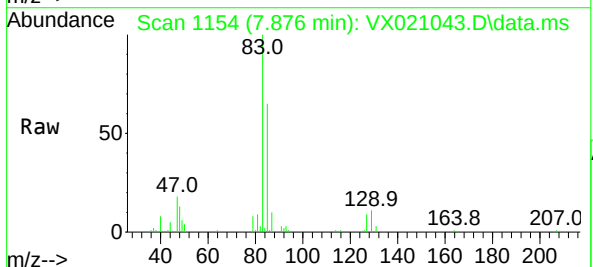




#47
Bromodichloromethane
Concen: 5.04 ug/l
RT: 7.876 min Scan# 1154
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion: 83 Resp: 19777
Ion Ratio Lower Upper
83 100
85 65.2 51.4 77.0
127 8.7 6.8 10.2

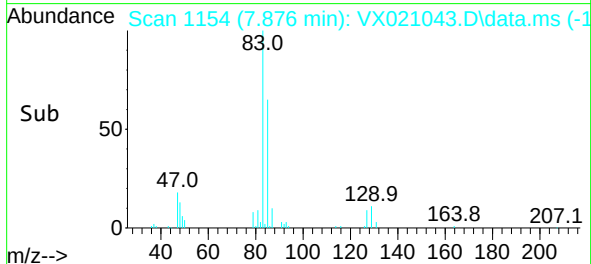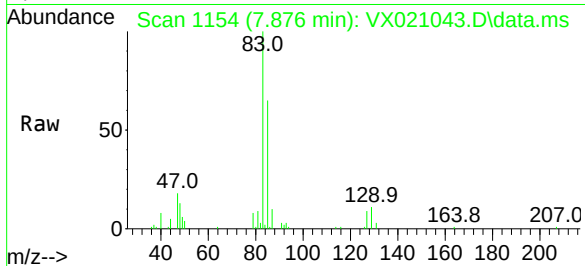

#48
Methyl methacrylate
Concen: 0.54 ug/l
RT: 7.635 min Scan# 1113
Delta R.T. -0.112 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 41 Resp: 1632
Ion Ratio Lower Upper
41 100
69 0.0 76.0 114.0#
39 48.9 44.6 67.0

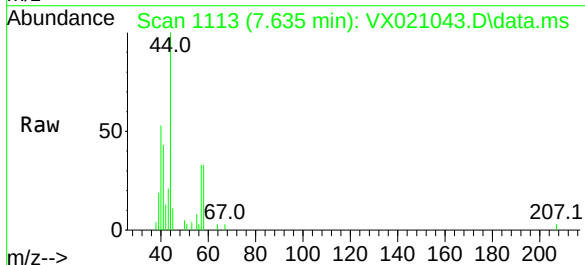



#49

1,4-Dioxane

Concen: 0.96 ug/l

RT: 7.723 min Scan# 1128





Delta R.T. 0.012 min

Lab File: VX021043.D

Acq: 05 Mar 2021 18:20

Tgt Ion:	88	Resp:	68
Ion	Ratio	Lower	Upper
88	100		
43	261.8	23.2	34.8#
58	0.0	55.0	82.4#

Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321

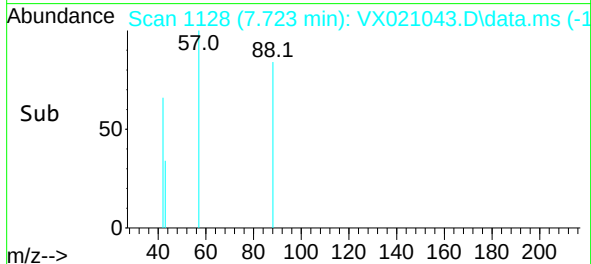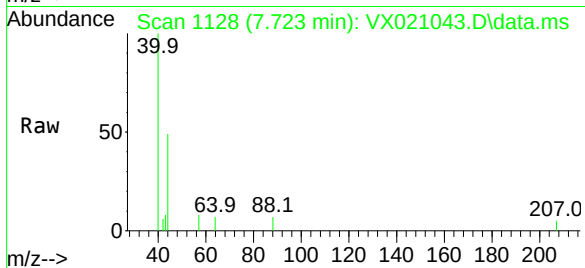

#50

Toluene-d8

Concen: 52.59 ug/l




RT: 8.694 min Scan# 1293


Delta R.T. -0.000 min

Lab File: VX021043.D

Acq: 05 Mar 2021 18:20

Tgt Ion:	98	Resp:	488270
Ion	Ratio	Lower	Upper
98	100		
100	66.6	51.9	77.9




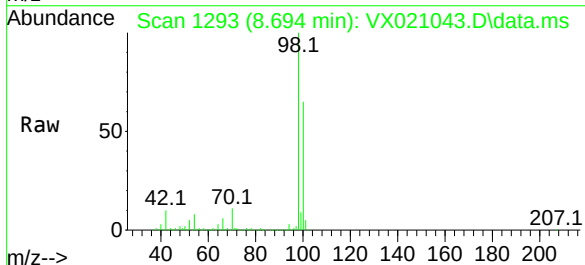




#51
4-Methyl-2-Pentanone
Concen: 0.57 ug/l
RT: 8.617 min Scan# 1280
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion: 43 Resp: 2010
Ion Ratio Lower Upper
43 100
58 42.4 35.4 53.0

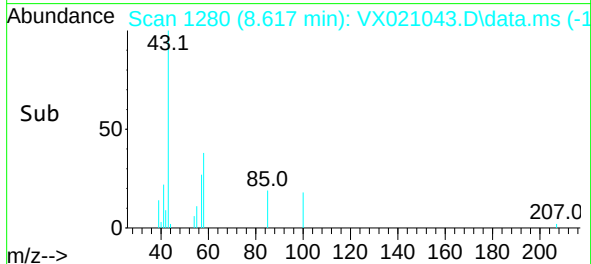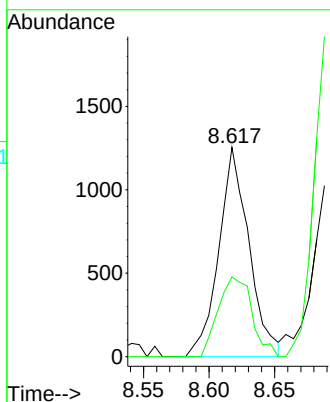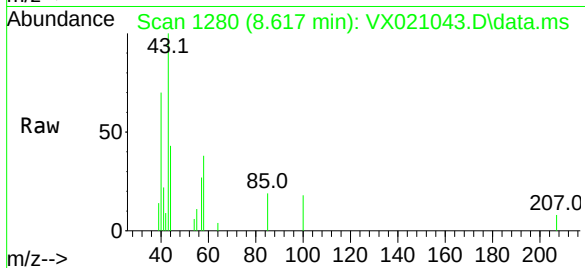

#52
Toluene
Concen: 0.74 ug/l
RT: 8.764 min Scan# 1305
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 92 Resp: 5153
Ion Ratio Lower Upper
92 100
91 166.4 137.1 205.7



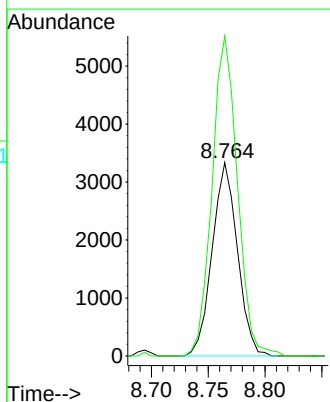
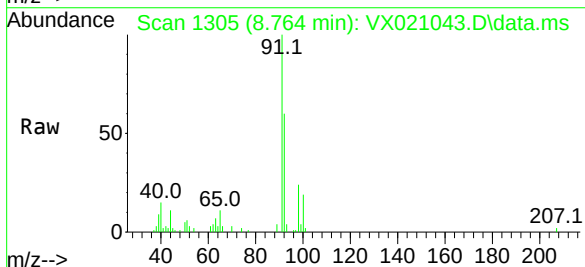


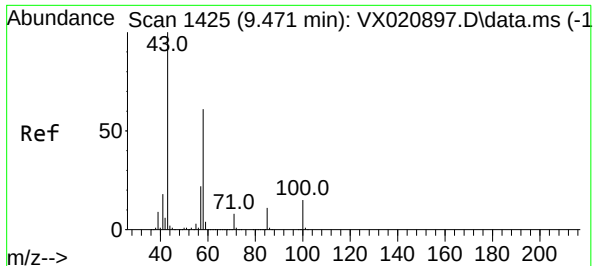

#59
2-Hexanone
Concen: 0.30 ug/l
RT: 9.470 min Scan# 1425
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion: 43 Resp: 779
Ion Ratio Lower Upper
43 100
58 47.2 30.9 92.8

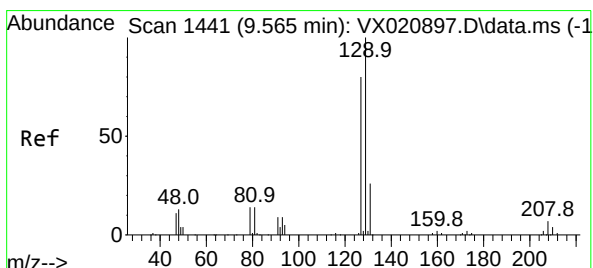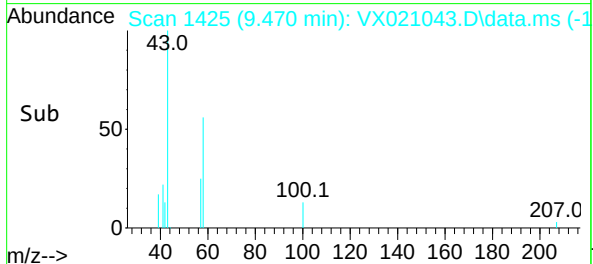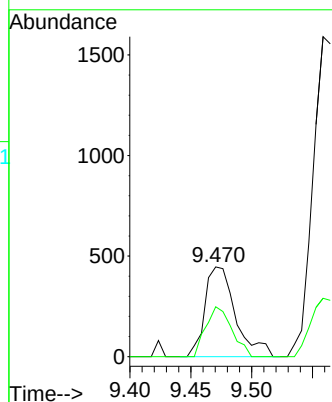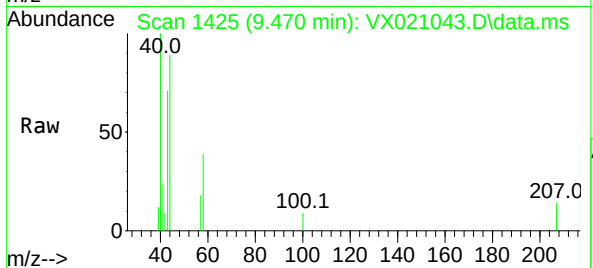

#60
Dibromochloromethane
Concen: 2.20 ug/l
RT: 9.565 min Scan# 1441
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 129 Resp: 6388
Ion Ratio Lower Upper
129 100
127 75.5 38.4 115.2


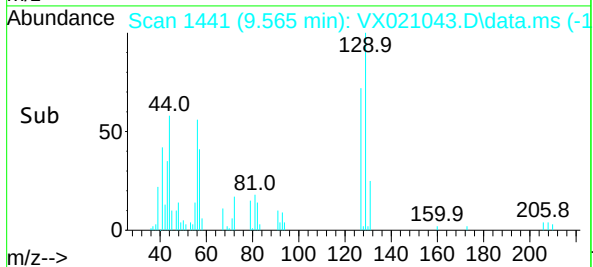
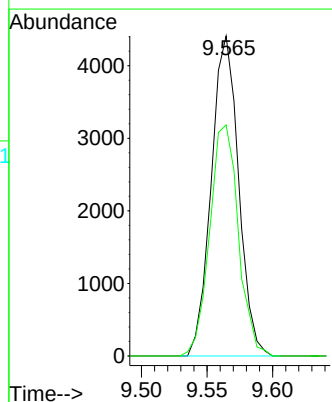
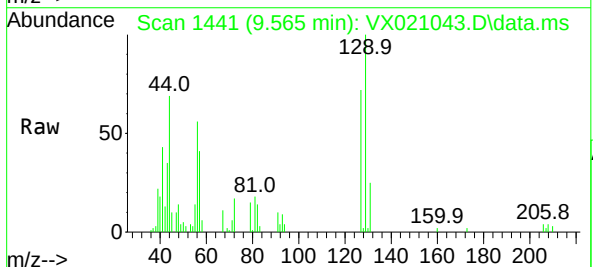


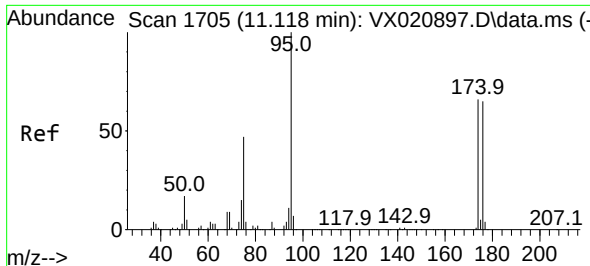

#62
4-Bromofluorobenzene
Concen: 54.68 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion: 95 Resp: 187716
Ion Ratio Lower Upper
95 100
174 75.6 0.0 154.6
176 76.8 0.0 155.8

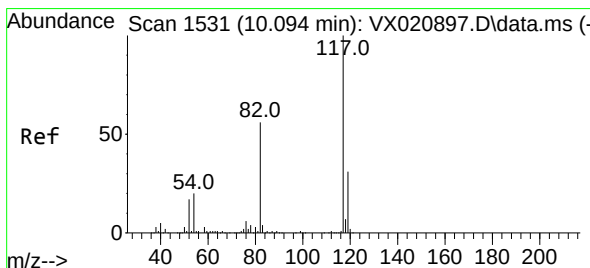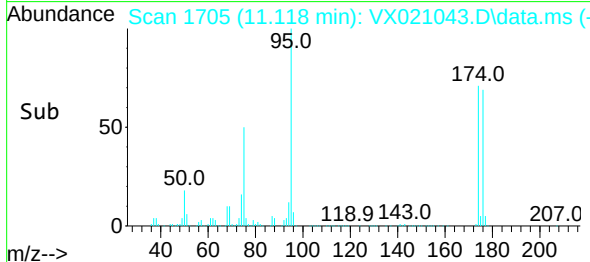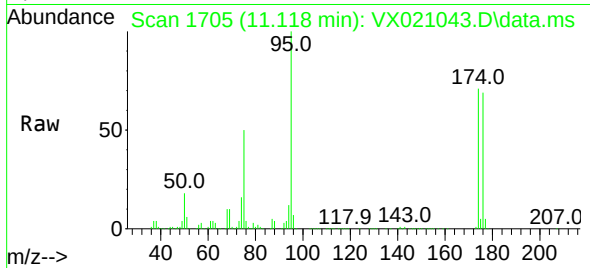

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 117 Resp: 377313
Ion Ratio Lower Upper
117 100
82 56.5 47.4 71.2
119 31.5 26.6 39.8


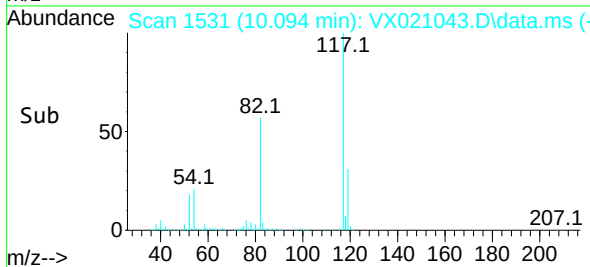

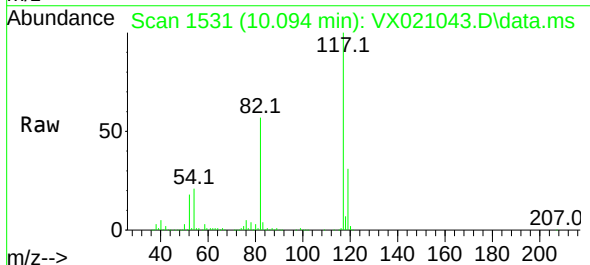


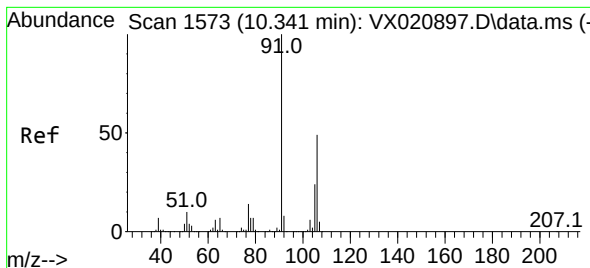

#68
m/p-Xylenes
Concen: 0.48 ug/l
RT: 10.341 min Scan# 1573
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion:106 Resp: 2538
Ion Ratio Lower Upper
106 100
91 198.0 162.8 244.2

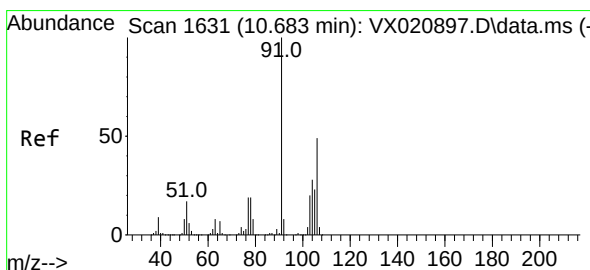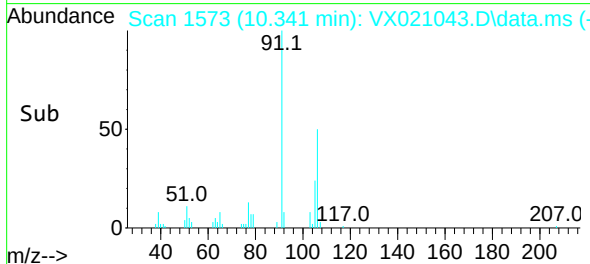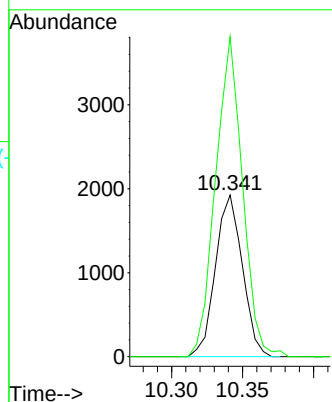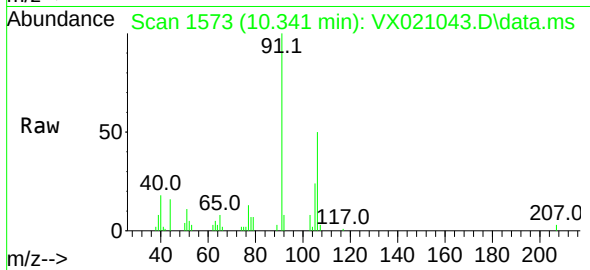

#69
o-Xylene
Concen: 0.21 ug/l
RT: 10.682 min Scan# 1631
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion:106 Resp: 1072
Ion Ratio Lower Upper
106 100
91 212.7 108.1 324.2


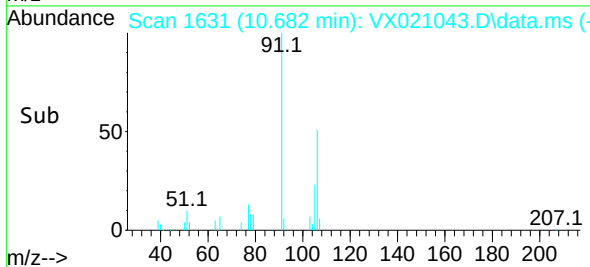
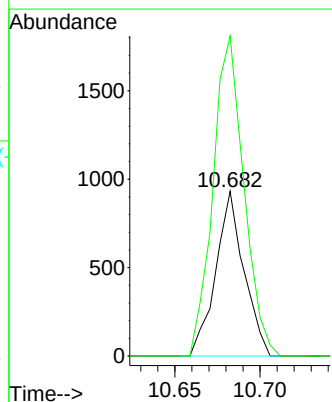
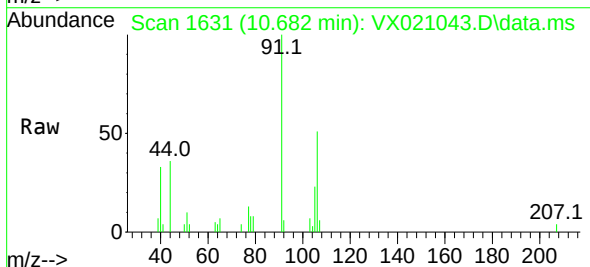




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.065 min Scan# 1866
Delta R.T. -0.000 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion:152 Resp: 170565
Ion Ratio Lower Upper
152 100
115 59.2 41.1 123.3
150 162.1 0.0 349.0

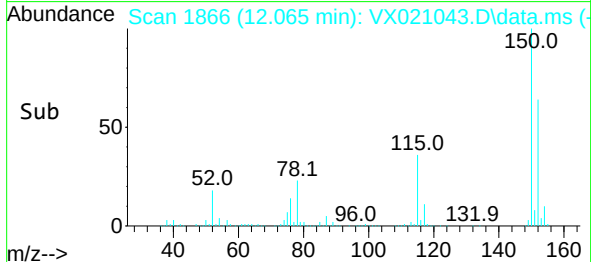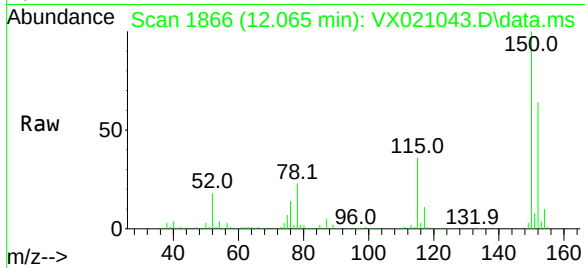

#74
N-ethyl acetate
Concen: 5.46 ug/l
RT: 10.894 min Scan# 1667
Delta R.T. 0.017 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 43 Resp: 29778
Ion Ratio Lower Upper
43 100
70 139.1 39.0 58.6#
55 89.6 21.5 32.3#
61 0.0 22.1 33.1#



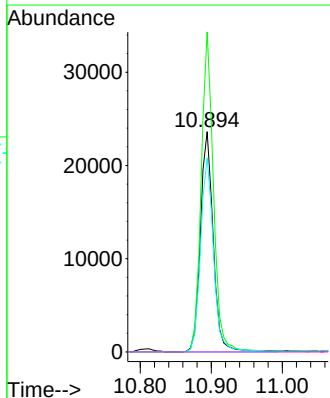
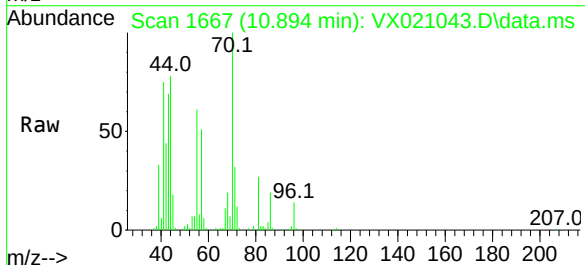


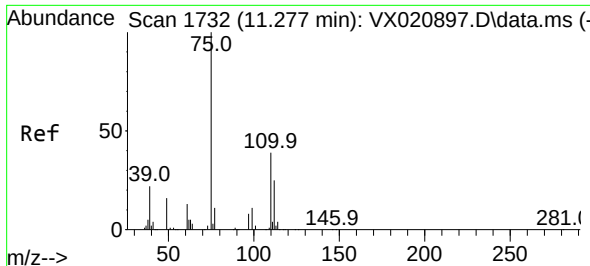

#76
1,2,3-Trichloropropane
Concen: 24.45 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.159 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20




Instrument :
MSVOA_X
ClientSampleId :
IDW-GW806-AQ-030321


Tgt Ion: 75 Resp: 89718
Ion Ratio Lower Upper
75 100
77 1.2 19.1 57.5#

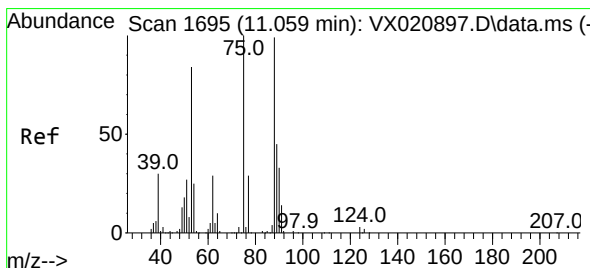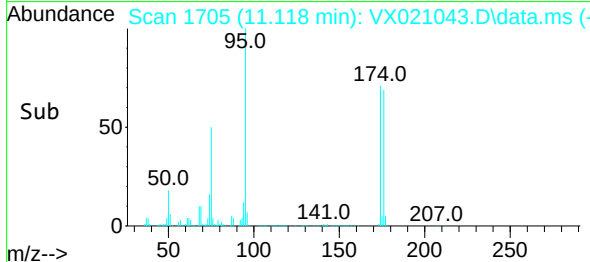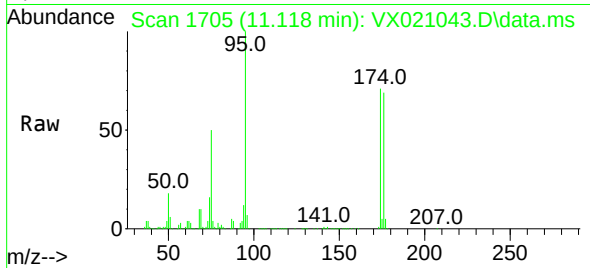

#81
trans-1,4-Dichloro-2-butene
Concen: 54.13 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. 0.059 min
Lab File: VX021043.D
Acq: 05 Mar 2021 18:20

Tgt Ion: 75 Resp: 89718
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

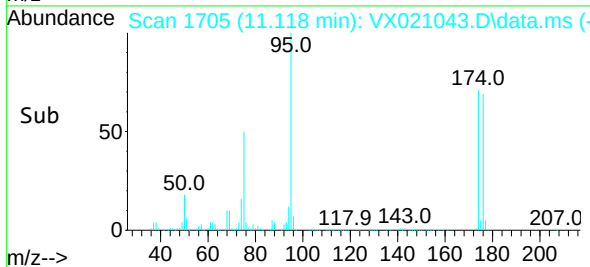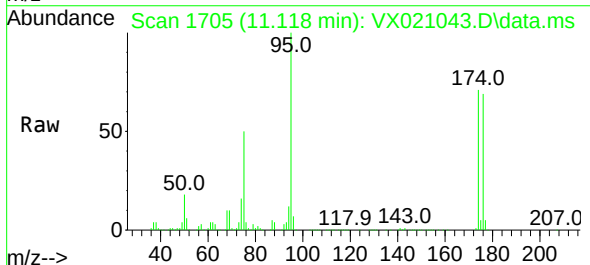

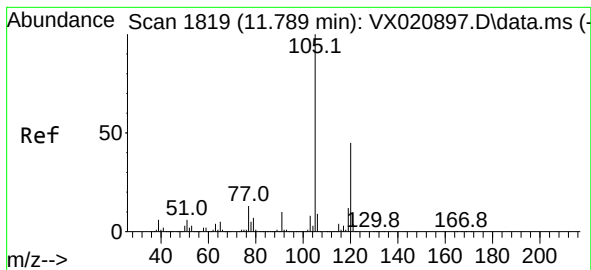

#84

1,2,4-Trimethylbenzene

Concen: 0.22 ug/l

RT: 11.788 min Scan# 1819

Delta R.T. -0.000 min

Lab File: VX021043.D

Acq: 05 Mar 2021 18:20

Tgt Ion:105 Resp: 2496

Ion Ratio Lower Upper

105 100

120 51.2 22.4 67.3

