

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030721\
 Data File : VX021035.D
 Acq On : 05 Mar 2021 15:25
 Operator : JC/MD
 Sample : M1584-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-VPB-RW6-GW-798-800

Quant Time: Mar 05 23:59:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 24 13:50:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.635	168	220947	50.00	ug/l	0.01
34) 1,4-Difluorobenzene	6.835	114	417761	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	403328	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.065	152	174914	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	150613	50.47	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 100.94%	
35) Dibromofluoromethane	5.464	113	128678	50.70	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 101.40%	
50) Toluene-d8	8.694	98	525026	53.05	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 106.10%	
62) 4-Bromofluorobenzene	11.118	95	193209	52.80	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 105.60%	
Target Compounds						
						Qvalue
16) Acetone	2.417	43	4224	3.43	ug/l	94
44) Trichloroethene	7.188	130	22909	7.32	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030721\
Data File : VX021035.D
Acq On : 05 Mar 2021 15:25
Operator : JC/MD
Sample : M1584-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-798-800


Quant Time: Mar 05 23:59:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 24 13:50:55 2021
Response via : Initial Calibration

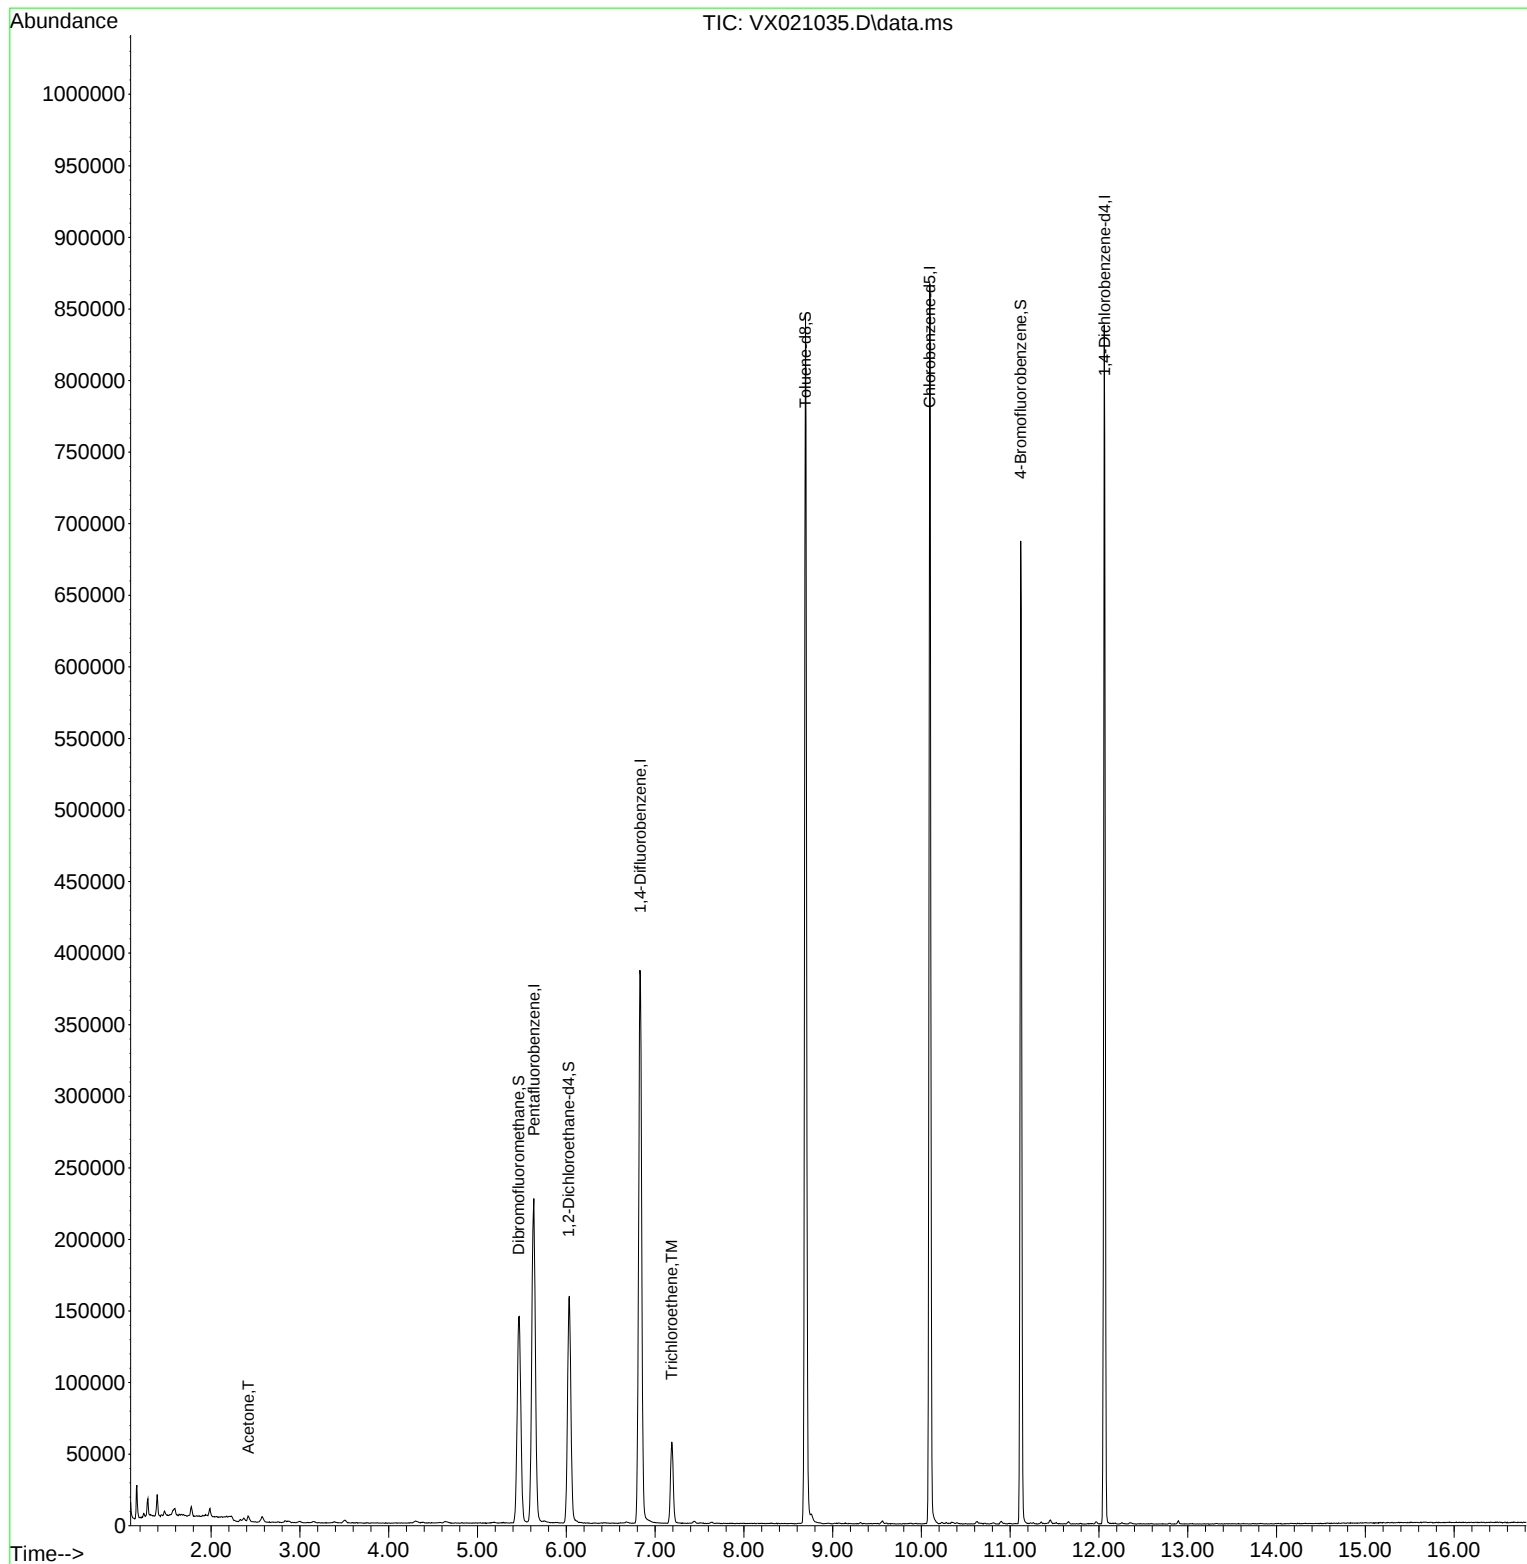






#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.635 min Scan# 773
Delta R.T. 0.012 min
Lab File: VX021035.D
Acq: 05 Mar 2021 15:25

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-798-800



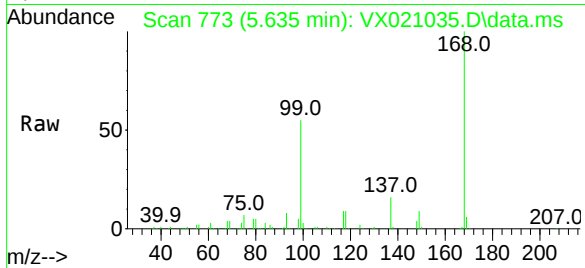



Tgt Ion:168 Resp: 220947
Ion Ratio Lower Upper
168 100
99 54.7 45.8 68.6

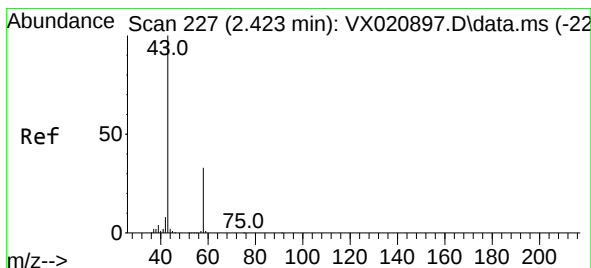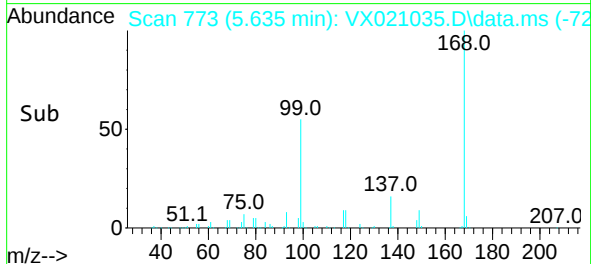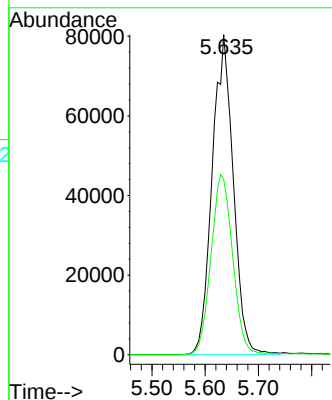

#16
Acetone
Concen: 3.43 ug/l
RT: 2.417 min Scan# 226
Delta R.T. -0.006 min
Lab File: VX021035.D
Acq: 05 Mar 2021 15:25

Tgt Ion: 43 Resp: 4224
Ion Ratio Lower Upper
43 100
58 31.5 27.8 41.8


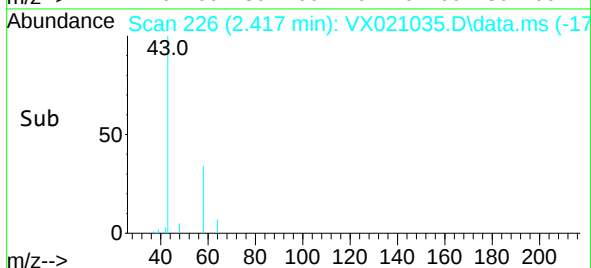
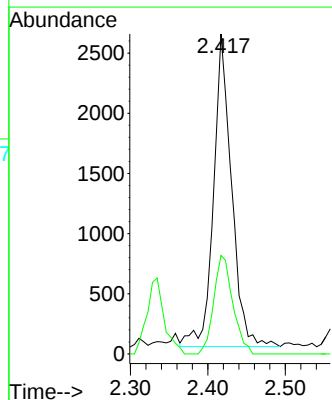
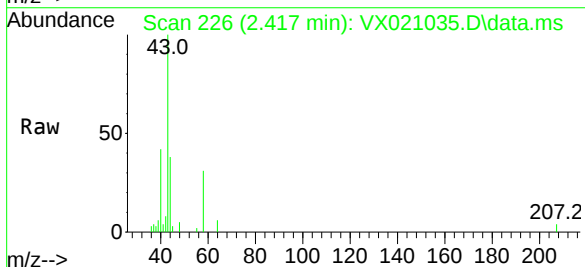


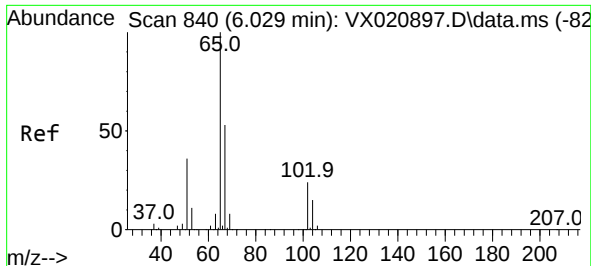

#33
1,2-Dichloroethane-d4
Concen: 50.47 ug/l
RT: 6.029 min Scan# 840
Delta R.T. -0.000 min
Lab File: VX021035.D
Acq: 05 Mar 2021 15:25




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-798-800


Tgt Ion: 65 Resp: 150613
Ion Ratio Lower Upper
65 100
67 52.4 0.0 105.4

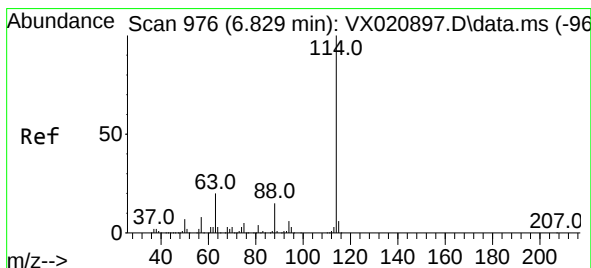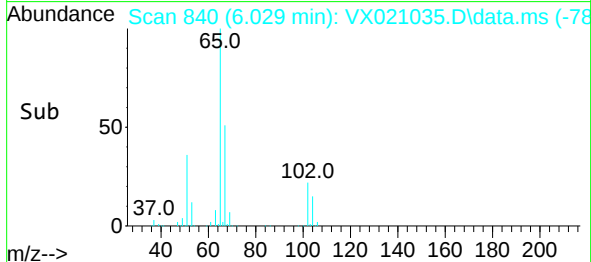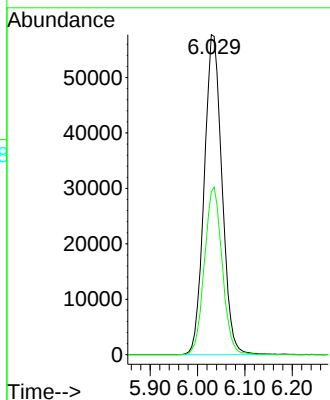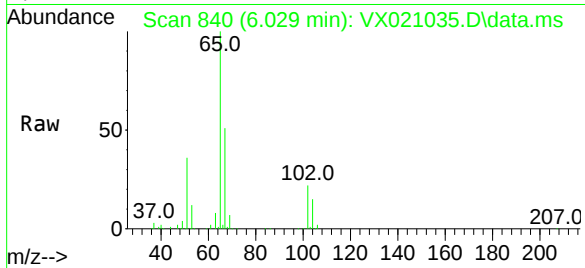

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.835 min Scan# 977
Delta R.T. 0.006 min
Lab File: VX021035.D
Acq: 05 Mar 2021 15:25


Tgt Ion: 114 Resp: 417761
Ion Ratio Lower Upper
114 100
63 19.3 0.0 40.8
88 16.4 0.0 32.8

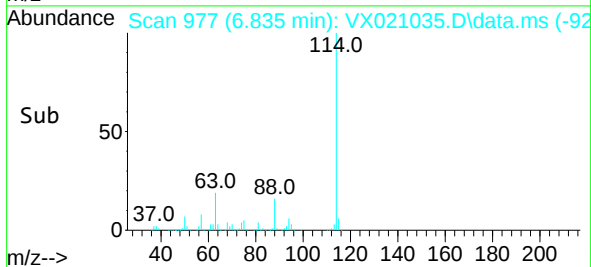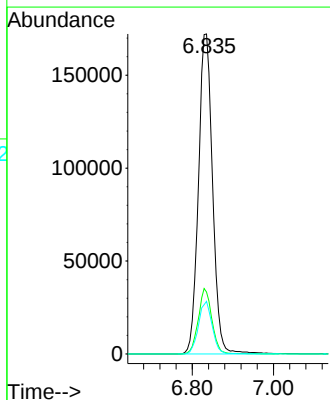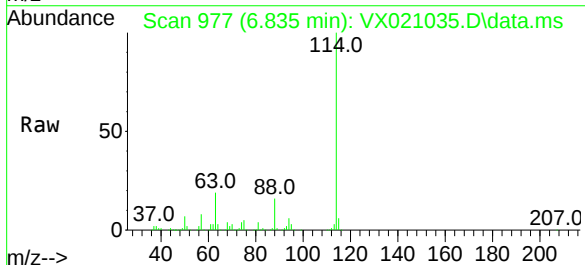



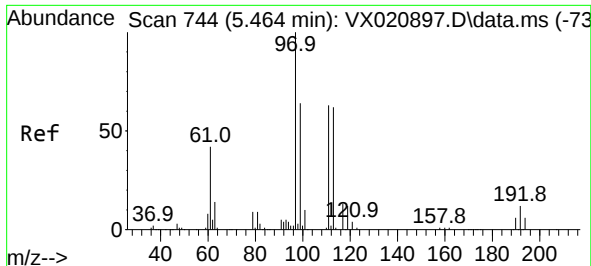


#35
Dibromofluoromethane
Concen: 50.70 ug/l
RT: 5.464 min Scan# 744
Delta R.T. -0.000 min
Lab File: VX021035.D
Acq: 05 Mar 2021 15:25


Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-798-800

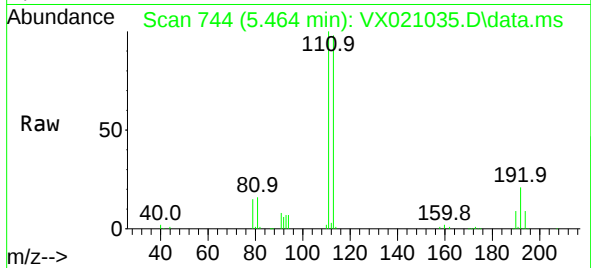



Tgt Ion:113 Resp: 128678
Ion Ratio Lower Upper
113 100
111 103.1 81.9 122.9
192 21.0 16.7 25.1

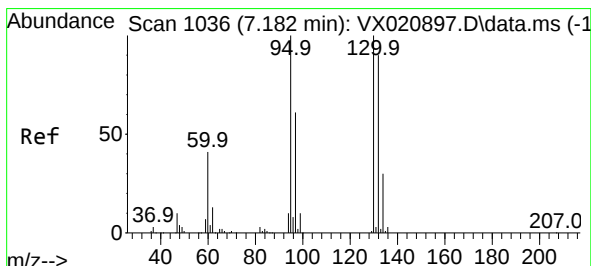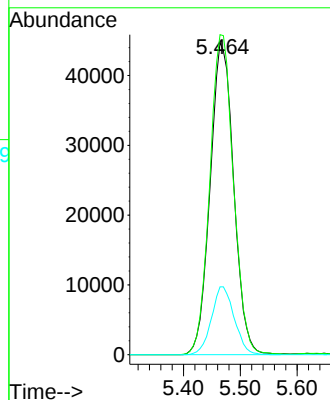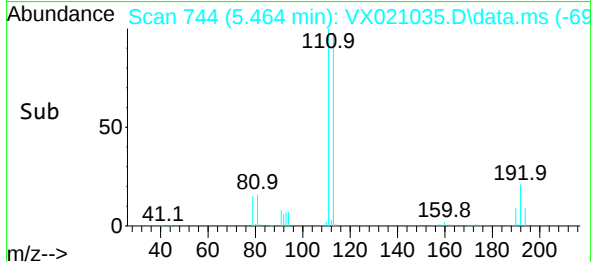


#44
Trichloroethene
Concen: 7.32 ug/l
RT: 7.188 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VX021035.D
Acq: 05 Mar 2021 15:25

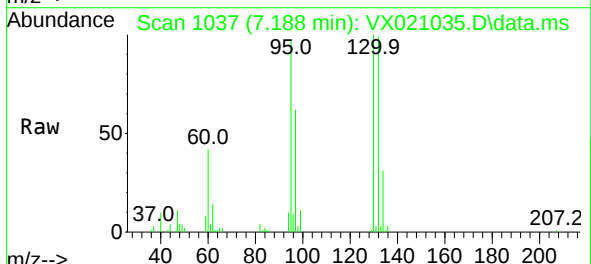

Tgt Ion:130 Resp: 22909
Ion Ratio Lower Upper
130 100
95 96.6 0.0 198.0



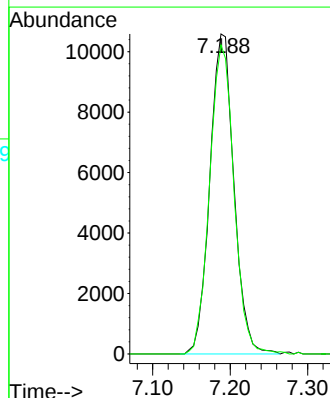
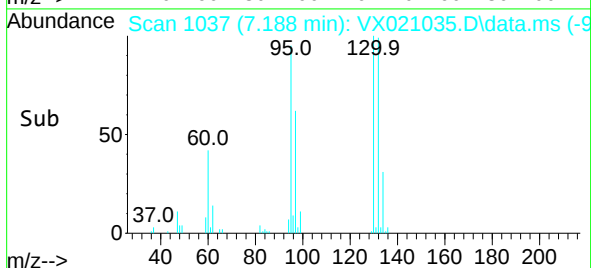


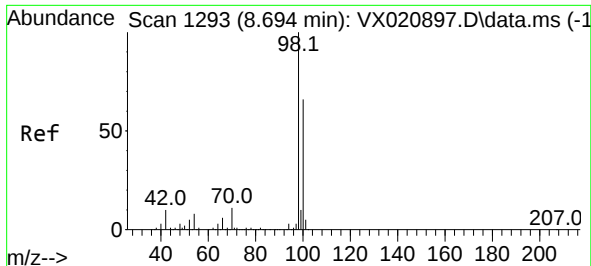

#50
Toluene-d8
Concen: 53.05 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. -0.000 min
Lab File: VX021035.D
Acq: 05 Mar 2021 15:25




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-798-800


Tgt Ion: 98 Resp: 525026
Ion Ratio Lower Upper
98 100
100 66.1 51.9 77.9

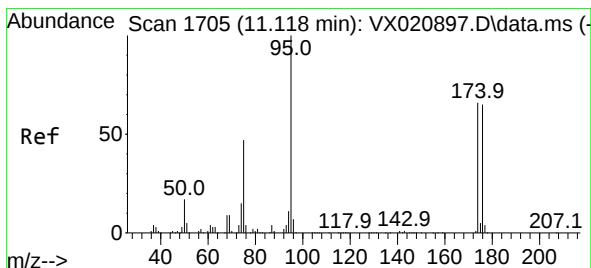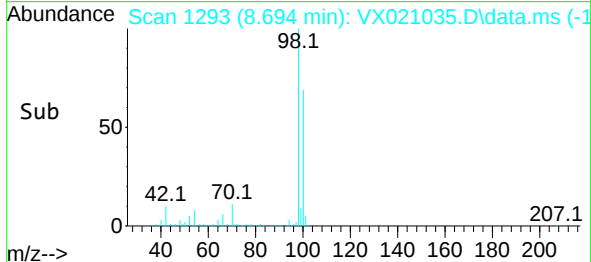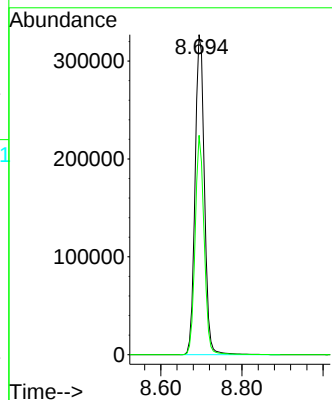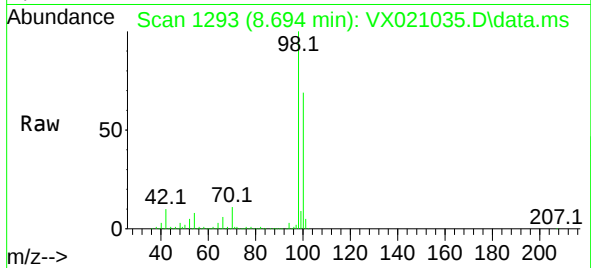

#62
4-Bromofluorobenzene
Concen: 52.80 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021035.D
Acq: 05 Mar 2021 15:25

Tgt Ion: 95 Resp: 193209
Ion Ratio Lower Upper
95 100
174 76.7 0.0 154.6
176 73.6 0.0 155.8


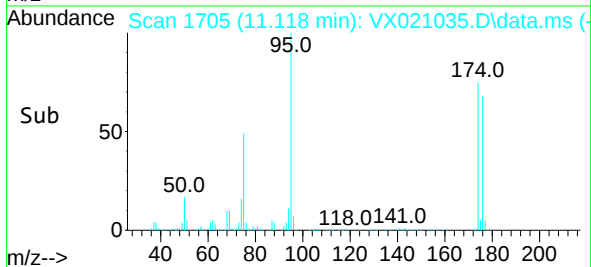
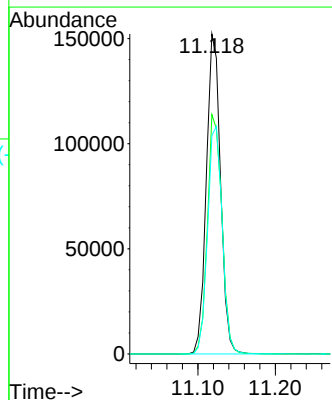
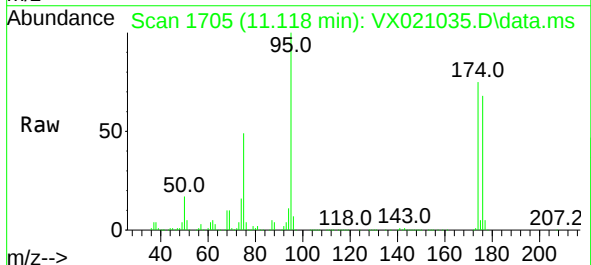


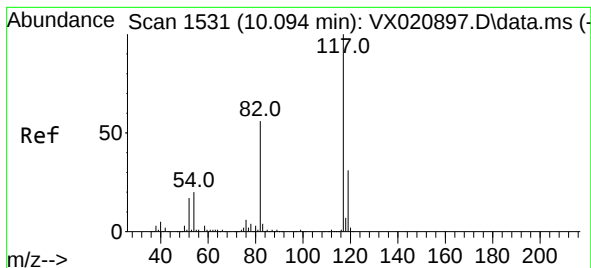

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. -0.000 min
Lab File: VX021035.D
Acq: 05 Mar 2021 15:25

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-798-800

Tgt Ion:117 Resp: 403328
Ion Ratio Lower Upper
117 100
82 58.5 47.4 71.2
119 33.3 26.6 39.8

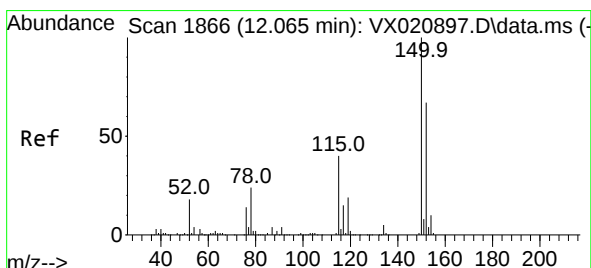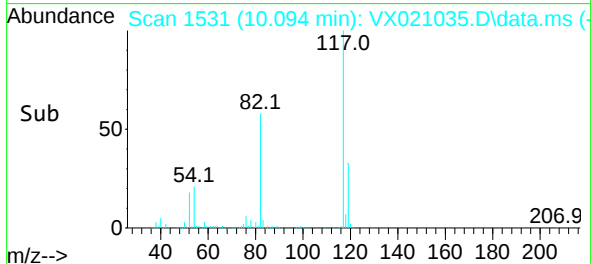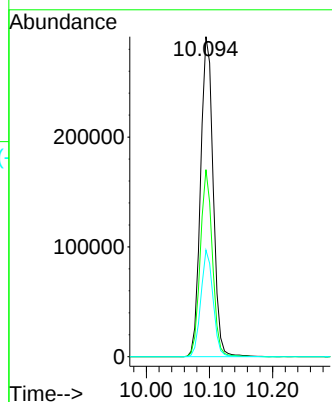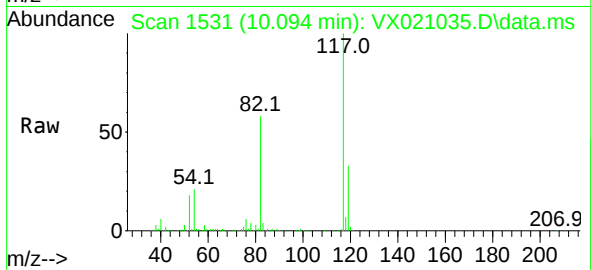

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.065 min Scan# 1866
Delta R.T. -0.000 min
Lab File: VX021035.D
Acq: 05 Mar 2021 15:25

Tgt Ion:152 Resp: 174914
Ion Ratio Lower Upper
152 100
115 58.3 41.1 123.3
150 154.1 0.0 349.0

