

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
 Data File : VX040607.D
 Acq On : 06 Mar 2024 16:35
 Operator : JC/MD
 Sample : VX0307MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK660

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	11	13	16	rBB2	652	585	0.08%	0.010%
2	1.264	27	29	32	rVB	864	831	0.11%	0.015%
3	1.368	42	46	59	rVB	104576	111673	15.01%	1.975%
4	1.666	91	95	108	rVB	69670	102990	13.84%	1.822%
5	2.306	193	200	210	rBV	162891	259405	34.87%	4.588%
6	2.447	221	223	225	rVB2	317	271	0.04%	0.005%
7	2.514	229	234	239	rVB3	2397	4018	0.54%	0.071%
8	2.788	274	279	286	rBV3	1122	2278	0.31%	0.040%
9	2.989	308	312	313	rBV2	173	192	0.03%	0.003%
10	3.099	324	330	335	rBV3	1515	2321	0.31%	0.041%
11	3.367	370	374	376	rBV	241	225	0.03%	0.004%
12	3.605	410	413	414	rBV	284	243	0.03%	0.004%
13	3.916	462	464	466	rBV	210	189	0.03%	0.003%
14	4.458	543	553	567	rBV2	61436	178600	24.01%	3.159%
15	4.763	600	603	604	rBV2	195	265	0.04%	0.005%
16	4.800	607	609	612	rVB2	293	297	0.04%	0.005%
17	4.824	612	613	616	rBV	230	225	0.03%	0.004%
18	4.897	623	625	627	rBV	225	201	0.03%	0.004%
19	5.062	639	652	666	rBV	99637	310535	41.74%	5.492%
20	5.184	670	672	676	rVB2	397	432	0.06%	0.008%
21	5.221	676	678	680	rBV	333	381	0.05%	0.007%
22	5.385	700	705	713	rBV2	817	1839	0.25%	0.033%
23	5.452	713	716	717	rBV2	611	623	0.08%	0.011%
24	5.550	730	732	735	rBV3	388	557	0.07%	0.010%
25	5.641	745	747	748	rBV2	248	202	0.03%	0.004%
26	5.970	788	801	818	rBV2	250734	743908	100.00%	13.158%
27	6.428	874	876	879	rVB	209	211	0.03%	0.004%
28	6.531	891	893	897	rVB2	191	237	0.03%	0.004%
29	6.672	912	916	919	rBV	209	244	0.03%	0.004%
30	6.763	921	931	947	rBV	154779	371655	49.96%	6.574%
31	6.964	962	964	966	rBV2	195	216	0.03%	0.004%
32	7.117	983	989	996	rVB6	2452	5937	0.80%	0.105%
33	7.306	1011	1020	1030	rBV	151517	332269	44.67%	5.877%
34	7.580	1063	1065	1066	rBV	240	195	0.03%	0.003%
35	7.696	1080	1084	1085	rBV	346	235	0.03%	0.004%
36	7.830	1102	1106	1107	rBV	195	223	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
 Data File : VX040607.D
 Acq On : 06 Mar 2024 16:35
 Operator : JC/MD
 Sample : VX0307MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK660

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.940	1121	1124	1127	rBV2	677	877	0.12%	0.016%
38	8.031	1135	1139	1142	rBV2	164	213	0.03%	0.004%
39	8.098	1148	1150	1151	rBV	395	228	0.03%	0.004%
40	8.165	1158	1161	1163	rBV2	198	231	0.03%	0.004%
41	8.324	1181	1187	1203	rBV	112972	182813	24.57%	3.233%
42	8.488	1211	1214	1215	rBV2	388	532	0.07%	0.009%
43	8.543	1221	1223	1226	rBV	297	317	0.04%	0.006%
44	8.574	1226	1228	1232	rVB3	381	434	0.06%	0.008%
45	8.647	1234	1240	1250	rBV	375352	586801	78.88%	10.379%
46	8.952	1284	1290	1303	rBV	82622	123988	16.67%	2.193%
47	9.128	1317	1319	1324	rVB2	288	455	0.06%	0.008%
48	9.189	1324	1329	1333	rBV2	271	590	0.08%	0.010%
49	9.275	1339	1343	1347	rBV4	1886	2739	0.37%	0.048%
50	9.384	1355	1361	1377	rBV	297207	423239	56.89%	7.486%
51	9.573	1391	1392	1396	rVB2	180	203	0.03%	0.004%
52	9.616	1396	1399	1401	rBV	336	430	0.06%	0.008%
53	9.720	1413	1416	1420	rBV2	241	368	0.05%	0.007%
54	9.842	1431	1436	1439	rBV3	528	788	0.11%	0.014%
55	9.921	1445	1449	1451	rBV2	200	196	0.03%	0.003%
56	10.055	1465	1471	1486	rBV	348762	465207	62.54%	8.228%
57	10.195	1491	1494	1498	rBV3	1758	2425	0.33%	0.043%
58	10.305	1507	1512	1518	rBV2	2067	2921	0.39%	0.052%
59	10.500	1540	1544	1546	rVB2	176	204	0.03%	0.004%
60	10.646	1564	1568	1569	rBV2	1756	1786	0.24%	0.032%
61	10.823	1596	1597	1599	rVV	307	186	0.03%	0.003%
62	10.884	1605	1607	1611	rVV2	281	327	0.04%	0.006%
63	10.963	1616	1620	1629	rVB3	2213	3277	0.44%	0.058%
64	11.085	1637	1640	1645	rVV2	1193	1674	0.23%	0.030%
65	11.189	1652	1657	1668	rVV	283923	368314	49.51%	6.514%
66	11.299	1672	1675	1676	rBV	173	203	0.03%	0.004%
67	11.451	1697	1700	1704	rBV2	2129	2841	0.38%	0.050%
68	11.567	1715	1719	1720	rBV2	238	233	0.03%	0.004%
69	11.756	1744	1750	1755	rBV4	2549	3651	0.49%	0.065%
70	11.847	1763	1765	1768	rVB	296	251	0.03%	0.004%
71	11.890	1768	1772	1775	rBV	308	431	0.06%	0.008%
72	11.969	1782	1785	1789	rBV	3640	4789	0.64%	0.085%
73	12.024	1789	1794	1801	rVV	353020	459722	61.80%	8.131%
74	12.262	1832	1833	1837	rBV	186	199	0.03%	0.004%
75	12.317	1837	1842	1853	rVV	417904	539914	72.58%	9.550%
76	12.433	1859	1861	1863	rVB2	305	205	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
 Data File : VX040607.D
 Acq On : 06 Mar 2024 16:35
 Operator : JC/MD
 Sample : VX0307MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK660

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

77	12.549	1877	1880	1884	rBV2	192	293	0.04%	0.005%
78	12.823	1923	1925	1929	rBV2	168	249	0.03%	0.004%
79	12.969	1947	1949	1952	rBV2	165	227	0.03%	0.004%
80	13.024	1952	1958	1959	rVV2	265	354	0.05%	0.006%
81	13.115	1967	1973	1979	rBV3	4511	6159	0.83%	0.109%
82	13.195	1982	1986	1988	rBV	172	239	0.03%	0.004%
83	13.231	1988	1992	1995	rBV2	234	319	0.04%	0.006%
84	13.414	2020	2022	2026	rBV2	178	226	0.03%	0.004%
85	13.536	2039	2042	2043	rBV	225	244	0.03%	0.004%
86	13.591	2047	2051	2057	rVV2	5710	7431	1.00%	0.131%
87	13.780	2077	2082	2090	rBV	7699	9407	1.26%	0.166%
88	13.963	2107	2112	2117	rVB2	5117	6712	0.90%	0.119%
89	14.048	2125	2126	2130	rBV2	179	195	0.03%	0.003%
90	14.128	2137	2139	2142	rBV	285	198	0.03%	0.004%
91	14.627	2217	2221	2222	rBV2	201	230	0.03%	0.004%
92	14.755	2239	2242	2244	rBV	292	290	0.04%	0.005%
93	14.969	2274	2277	2278	rBV2	293	321	0.04%	0.006%
94	15.316	2332	2334	2336	rBV	184	236	0.03%	0.004%
95	15.438	2352	2354	2356	rVB	379	226	0.03%	0.004%
96	15.578	2375	2377	2378	rBV2	243	225	0.03%	0.004%
97	15.926	2432	2434	2436	rVB2	373	283	0.04%	0.005%
98	15.975	2439	2442	2443	rBV2	351	331	0.04%	0.006%
99	16.249	2486	2487	2490	rBV	297	200	0.03%	0.004%
100	16.755	2568	2570	2572	rBV2	281	296	0.04%	0.005%




Sum of corrected areas: 5653801

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
Data File : VX040607.D
Acq On : 06 Mar 2024 16:35
Operator : JC/MD
Sample : VX0307MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK660

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

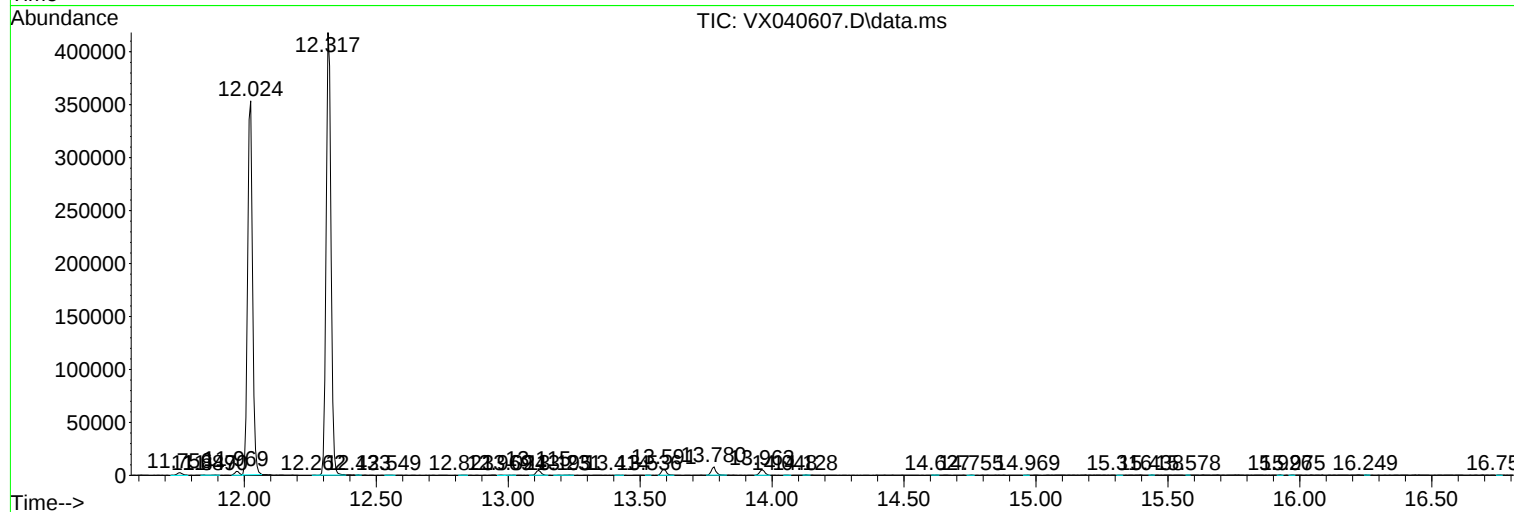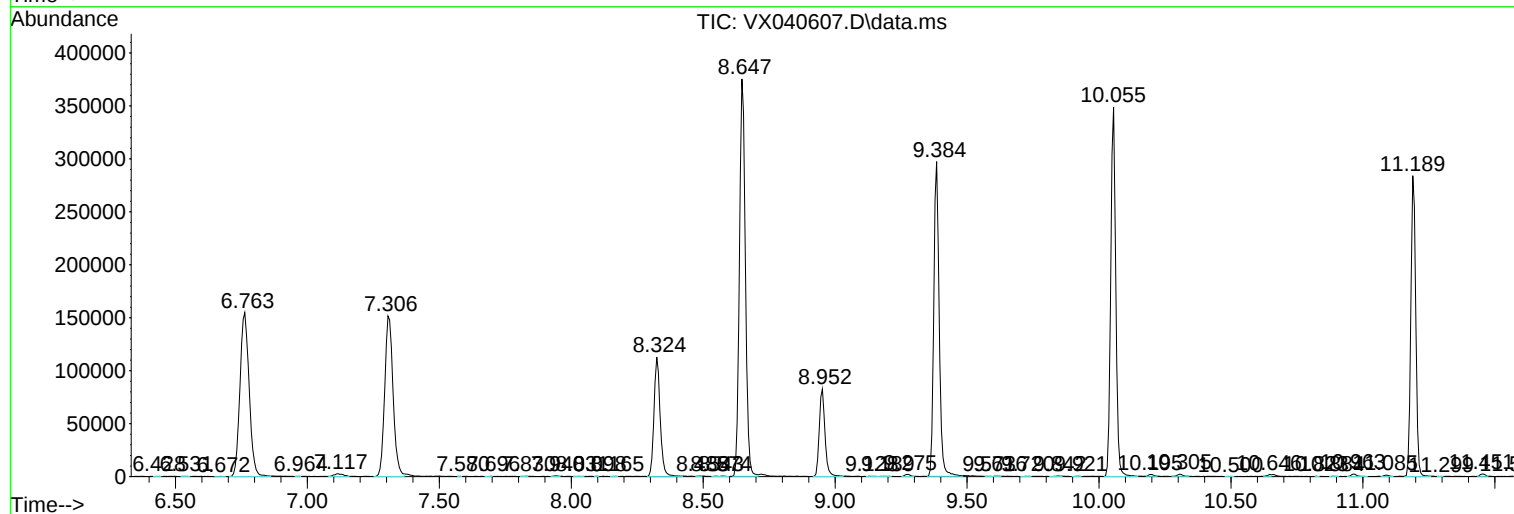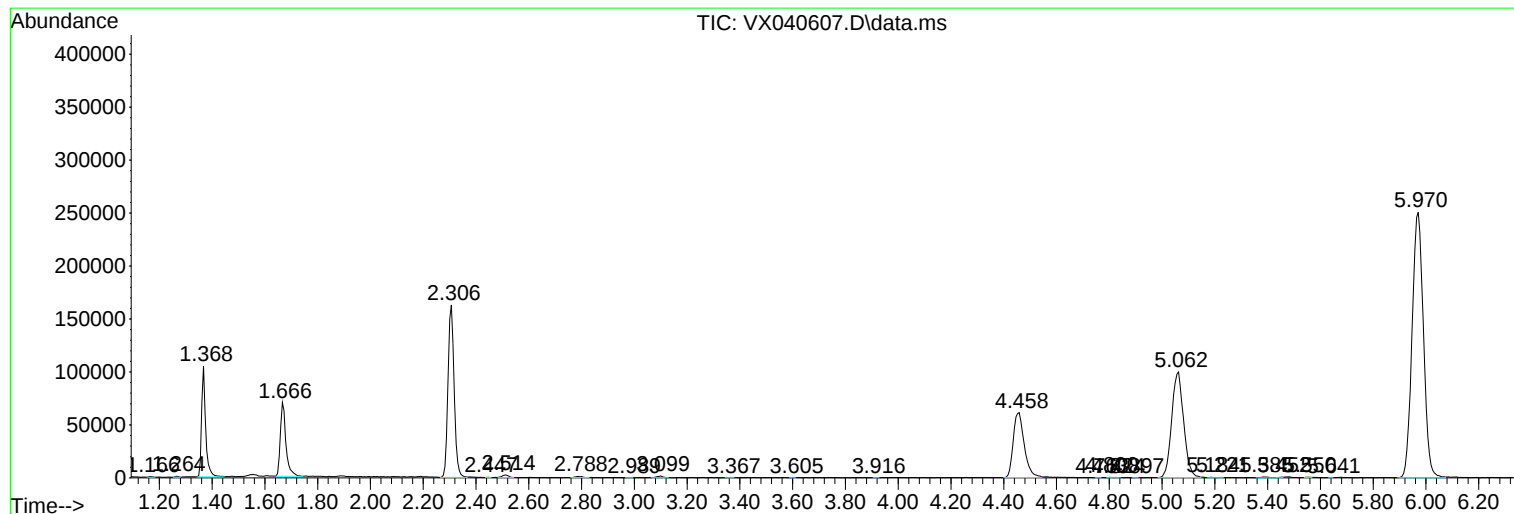

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
Data File : VX040607.D
Acq On : 06 Mar 2024 16:35
Operator : JC/MD
Sample : VX0307MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK660

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
Data File : VX040607.D
Acq On : 06 Mar 2024 16:35
Operator : JC/MD
Sample : VX0307MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK660

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc