

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
 Data File : VX040608.D
 Acq On : 06 Mar 2024 16:58
 Operator : JC/MD
 Sample : VX0307WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

Signal : TIC: VX040608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.173	11	14	17	rBV3	909	944	0.13%	0.017%
2	1.264	27	29	33	rBV3	951	843	0.11%	0.015%
3	1.294	33	34	36	rVV2	507	322	0.04%	0.006%
4	1.368	42	46	54	rBV	104392	109218	14.75%	1.939%
5	1.666	91	95	107	rBV	73880	102461	13.83%	1.819%
6	1.886	128	131	136	rVB2	1719	2308	0.31%	0.041%
7	2.306	193	200	209	rBV	165863	258559	34.91%	4.590%
8	2.514	229	234	237	rBV2	1911	3003	0.41%	0.053%
9	2.575	242	244	246	rBV	252	210	0.03%	0.004%
10	2.709	263	266	267	rBV	377	413	0.06%	0.007%
11	2.788	274	279	288	rVB4	1477	2746	0.37%	0.049%
12	3.087	323	328	330	rBV3	1379	1790	0.24%	0.032%
13	3.398	376	379	380	rVB	248	201	0.03%	0.004%
14	3.544	399	403	405	rBV2	168	215	0.03%	0.004%
15	3.599	410	412	417	rBV	313	522	0.07%	0.009%
16	3.703	425	429	433	rVB2	206	340	0.05%	0.006%
17	3.800	442	445	447	rVB2	228	259	0.03%	0.005%
18	3.843	450	452	454	rBV	169	186	0.03%	0.003%
19	3.977	472	474	479	rBV2	234	429	0.06%	0.008%
20	4.135	498	500	502	rVB	246	186	0.03%	0.003%
21	4.166	502	505	508	rBV	236	356	0.05%	0.006%
22	4.452	543	552	568	rBV	61194	176589	23.84%	3.135%
23	4.769	602	604	607	rVB	260	300	0.04%	0.005%
24	5.056	640	651	668	rVV2	97937	307359	41.50%	5.457%
25	5.263	682	685	688	rBV	231	364	0.05%	0.006%
26	5.349	697	699	700	rBV	248	209	0.03%	0.004%
27	5.672	748	752	755	rBV2	640	1164	0.16%	0.021%
28	5.739	760	763	766	rVB2	189	227	0.03%	0.004%
29	5.970	789	801	818	rBV2	247401	740701	100.00%	13.150%
30	6.166	831	833	837	rVB2	289	282	0.04%	0.005%
31	6.226	840	843	846	rVB2	294	427	0.06%	0.008%
32	6.275	846	851	853	rBV2	307	548	0.07%	0.010%
33	6.397	868	871	872	rBV	248	196	0.03%	0.003%
34	6.562	895	898	901	rBV	271	229	0.03%	0.004%
35	6.611	903	906	910	rBV2	305	445	0.06%	0.008%
36	6.763	921	931	946	rBV2	156997	379006	51.17%	6.729%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
 Data File : VX040608.D
 Acq On : 06 Mar 2024 16:58
 Operator : JC/MD
 Sample : VX0307WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
 Title : VOC Analysis

37	7.117	982	989	997	rVB7	3202	7184	0.97%	0.128%
38	7.306	1011	1020	1030	rBV	150074	333907	45.08%	5.928%
39	7.763	1091	1095	1096	rBV	322	275	0.04%	0.005%
40	7.830	1102	1106	1111	rVB3	706	1123	0.15%	0.020%
41	7.933	1121	1123	1126	rBV3	232	277	0.04%	0.005%
42	8.324	1181	1187	1201	rBV	107599	178887	24.15%	3.176%
43	8.464	1209	1210	1212	rBV	242	198	0.03%	0.004%
44	8.494	1212	1215	1220	rBV4	453	636	0.09%	0.011%
45	8.580	1224	1229	1233	rVB3	1383	2157	0.29%	0.038%
46	8.647	1234	1240	1248	rBV	364750	578177	78.06%	10.265%
47	8.891	1278	1280	1284	rBV	209	280	0.04%	0.005%
48	8.952	1284	1290	1301	rBV	81057	121583	16.41%	2.159%
49	9.159	1318	1324	1326	rVV2	872	1132	0.15%	0.020%
50	9.275	1339	1343	1348	rVB2	2013	3039	0.41%	0.054%
51	9.384	1355	1361	1376	rBV	296391	415147	56.05%	7.370%
52	9.616	1396	1399	1400	rBV2	676	660	0.09%	0.012%
53	9.653	1403	1405	1409	rBV2	230	311	0.04%	0.006%
54	9.848	1432	1437	1438	rBV2	417	632	0.09%	0.011%
55	9.878	1441	1442	1446	rVB2	259	288	0.04%	0.005%
56	10.055	1465	1471	1485	rBV	336451	472233	63.75%	8.384%
57	10.195	1491	1494	1501	rVB	3128	3833	0.52%	0.068%
58	10.305	1507	1512	1519	rBV3	2700	3971	0.54%	0.071%
59	10.457	1534	1537	1539	rVV2	142	190	0.03%	0.003%
60	10.659	1563	1570	1575	rBV4	2874	6134	0.83%	0.109%
61	10.835	1597	1599	1601	rBV	211	202	0.03%	0.004%
62	10.915	1609	1612	1613	rBV2	190	206	0.03%	0.004%
63	10.963	1616	1620	1624	rVB2	3151	3906	0.53%	0.069%
64	11.037	1629	1632	1634	rBV2	288	419	0.06%	0.007%
65	11.091	1638	1641	1644	rBV3	1082	1390	0.19%	0.025%
66	11.189	1652	1657	1664	rBV	282039	363639	49.09%	6.456%
67	11.366	1684	1686	1688	rBV2	241	293	0.04%	0.005%
68	11.457	1696	1701	1706	rBV2	2715	3902	0.53%	0.069%
69	11.671	1734	1736	1741	rVB	185	248	0.03%	0.004%
70	11.719	1741	1744	1746	rBV	201	203	0.03%	0.004%
71	11.756	1746	1750	1755	rVB2	2979	3568	0.48%	0.063%
72	11.811	1755	1759	1760	rBV2	161	194	0.03%	0.003%
73	11.975	1781	1786	1788	rBV	3251	4062	0.55%	0.072%
74	12.024	1788	1794	1806	rVB	350200	465766	62.88%	8.269%
75	12.317	1837	1842	1851	rBV	407958	535591	72.31%	9.509%
76	12.579	1881	1885	1889	rVV	292	367	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
Data File : VX040608.D
Acq On : 06 Mar 2024 16:58
Operator : JC/MD
Sample : VX0307WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Title : VOC Analysis

77	12.707	1905	1906	1909	rVB2	232	236	0.03%	0.004%
78	12.768	1912	1916	1918	rVB	183	230	0.03%	0.004%
79	13.006	1952	1955	1957	rVB2	214	271	0.04%	0.005%
80	13.115	1969	1973	1978	rBV3	2867	4005	0.54%	0.071%
81	13.262	1995	1997	2002	rBV	243	269	0.04%	0.005%
82	13.542	2041	2043	2046	rVV2	313	265	0.04%	0.005%
83	13.591	2047	2051	2057	rVB4	3504	5014	0.68%	0.089%
84	13.676	2063	2065	2070	rVB	233	318	0.04%	0.006%
85	13.780	2075	2082	2087	rBV	3134	4573	0.62%	0.081%
86	13.859	2092	2095	2099	rVB2	197	363	0.05%	0.006%
87	13.902	2099	2102	2103	rBV	244	264	0.04%	0.005%
88	13.963	2108	2112	2118	rVB	3301	3959	0.53%	0.070%
89	14.438	2188	2190	2191	rBV	299	203	0.03%	0.004%
90	14.877	2260	2262	2264	rBV2	198	201	0.03%	0.004%
91	14.932	2269	2271	2275	rBV	252	328	0.04%	0.006%
92	14.981	2275	2279	2280	rBV2	213	235	0.03%	0.004%
93	15.085	2295	2296	2298	rBV2	203	204	0.03%	0.004%
94	15.389	2344	2346	2349	rBV2	281	277	0.04%	0.005%
95	16.109	2462	2464	2465	rBV	466	292	0.04%	0.005%
96	16.304	2495	2496	2500	rVB2	333	285	0.04%	0.005%
97	16.401	2509	2512	2514	rBV2	285	376	0.05%	0.007%
98	16.578	2539	2541	2544	rVB3	281	200	0.03%	0.004%
99	16.609	2544	2546	2549	rVB2	202	204	0.03%	0.004%
100	16.694	2558	2560	2562	rBV2	293	253	0.03%	0.004%




Sum of corrected areas: 5632592

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
Data File : VX040608.D
Acq On : 06 Mar 2024 16:58
Operator : JC/MD
Sample : VX0307WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK661

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

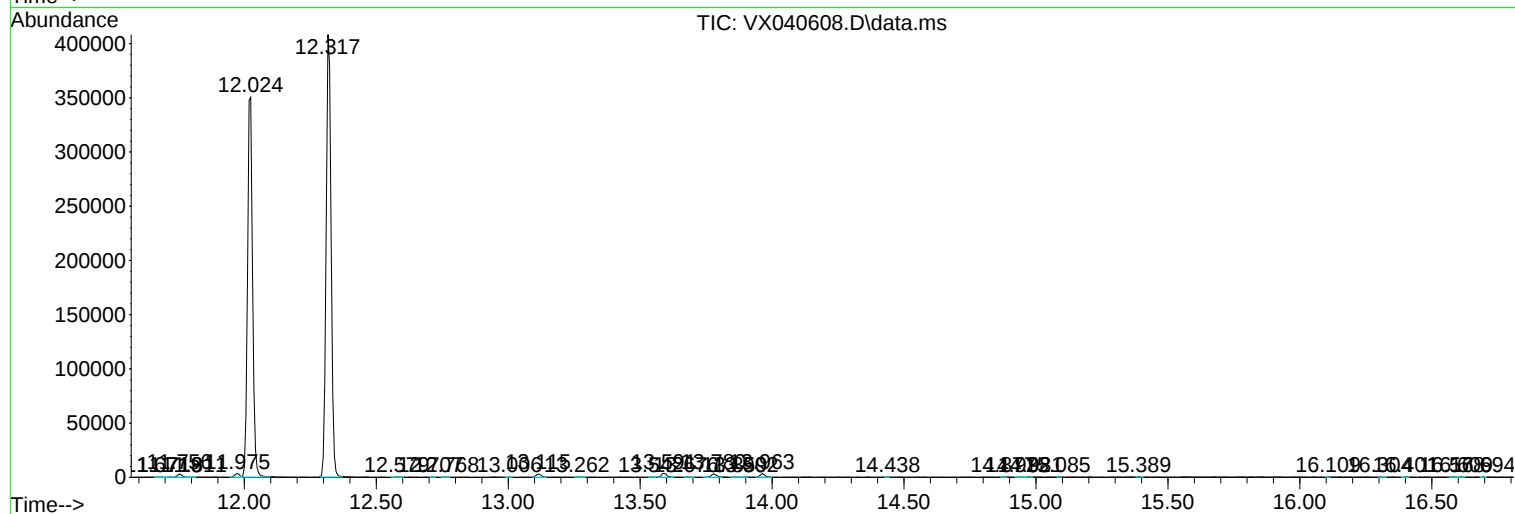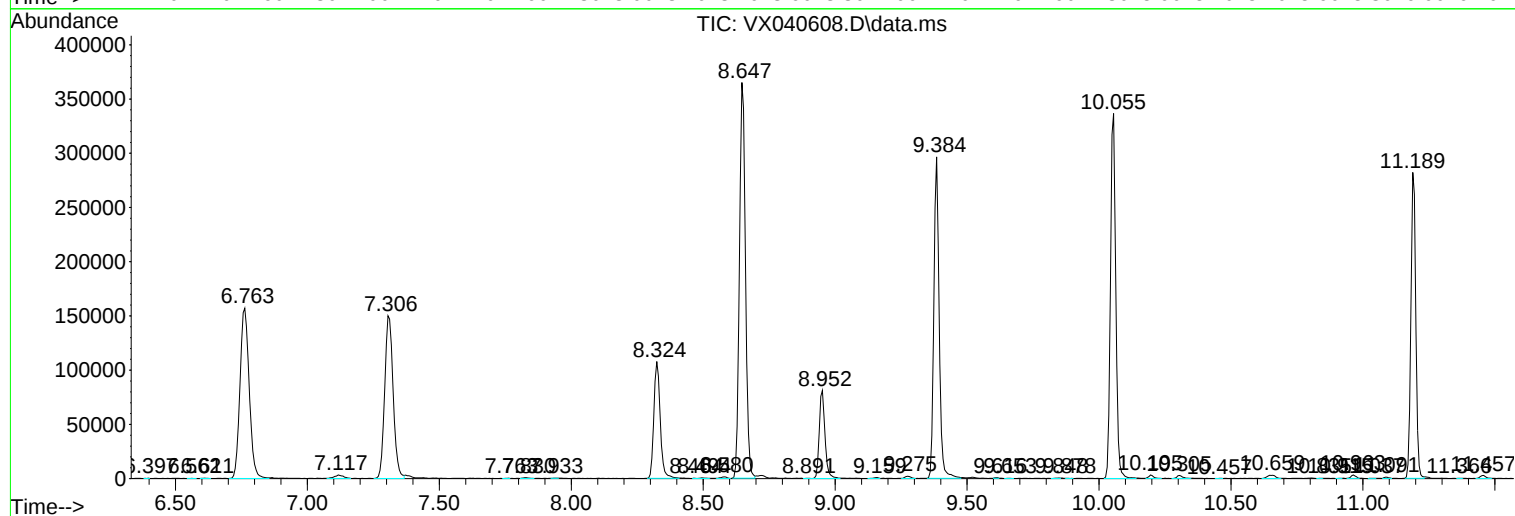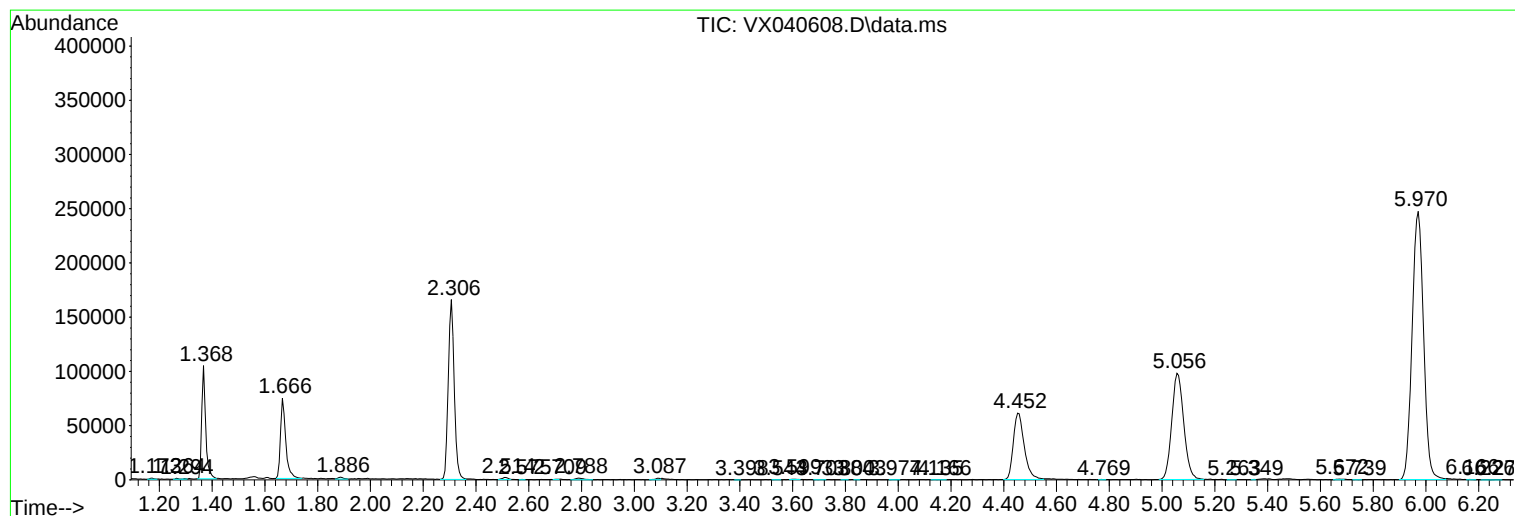

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
Data File : VX040608.D
Acq On : 06 Mar 2024 16:58
Operator : JC/MD
Sample : VX0307WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK661

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030724\
Data File : VX040608.D
Acq On : 06 Mar 2024 16:58
Operator : JC/MD
Sample : VX0307WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK661

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML030724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc