

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030821\
 Data File : VX021072.D
 Acq On : 08 Mar 2021 19:21
 Operator : JC/MD
 Sample : M1596-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WEST-DITCH-OUT-20210305

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M

Title : SW846 8260

Signal : TIC: VX021072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.587	77	85	92	rVB3	6109	14877	1.15%	0.188%
2	4.564	577	591	608	rBV	77807	220132	17.03%	2.785%
3	5.464	732	744	759	rBV	143890	409416	31.68%	5.180%
4	5.629	760	772	786	rBV	223562	618066	47.82%	7.820%
5	6.029	830	840	854	rBV	152260	401616	31.07%	5.082%
6	6.829	965	976	1000	rBV	381316	902282	69.81%	11.417%
7	7.188	1027	1037	1051	rBV2	468047	992170	76.76%	12.554%
8	8.694	1286	1293	1315	rBV	836070	1292518	100.00%	16.354%
9	10.094	1525	1531	1547	rBV	852030	1149089	88.90%	14.539%
10	11.118	1699	1705	1717	rBV	654355	862546	66.73%	10.914%
11	12.059	1860	1865	1878	rBV	841245	1040602	80.51%	13.167%




Sum of corrected areas: 7903314

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030821\
Data File : VX021072.D
Acq On : 08 Mar 2021 19:21
Operator : JC/MD
Sample : M1596-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WEST-DITCH-OUT-20210305

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

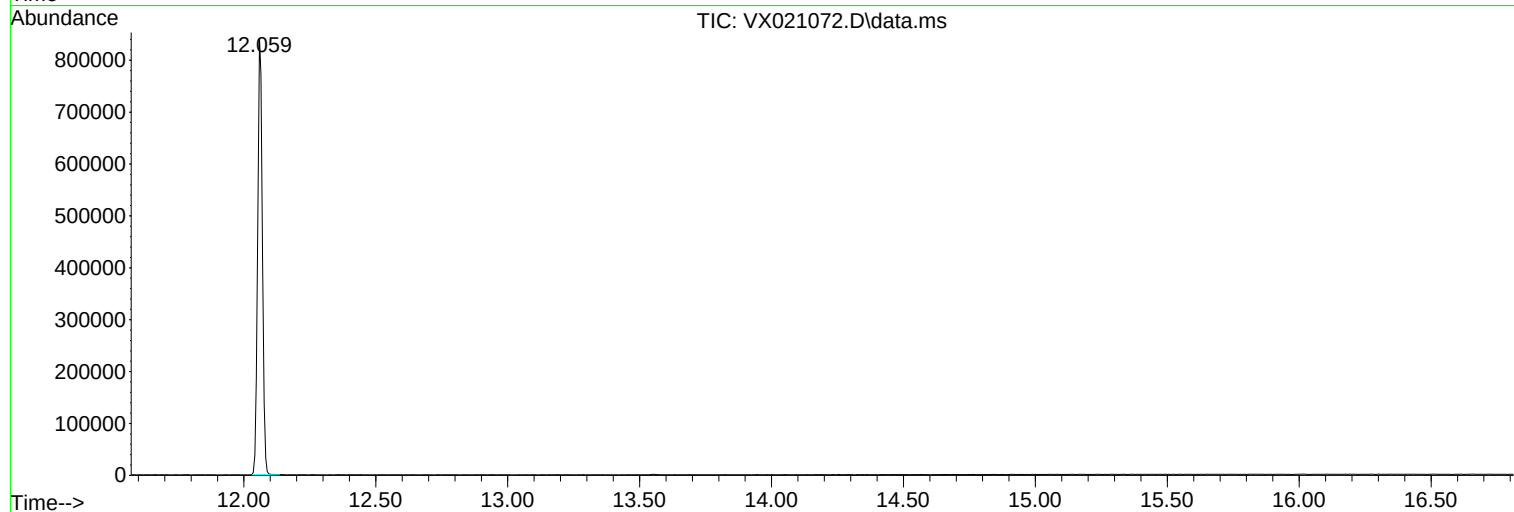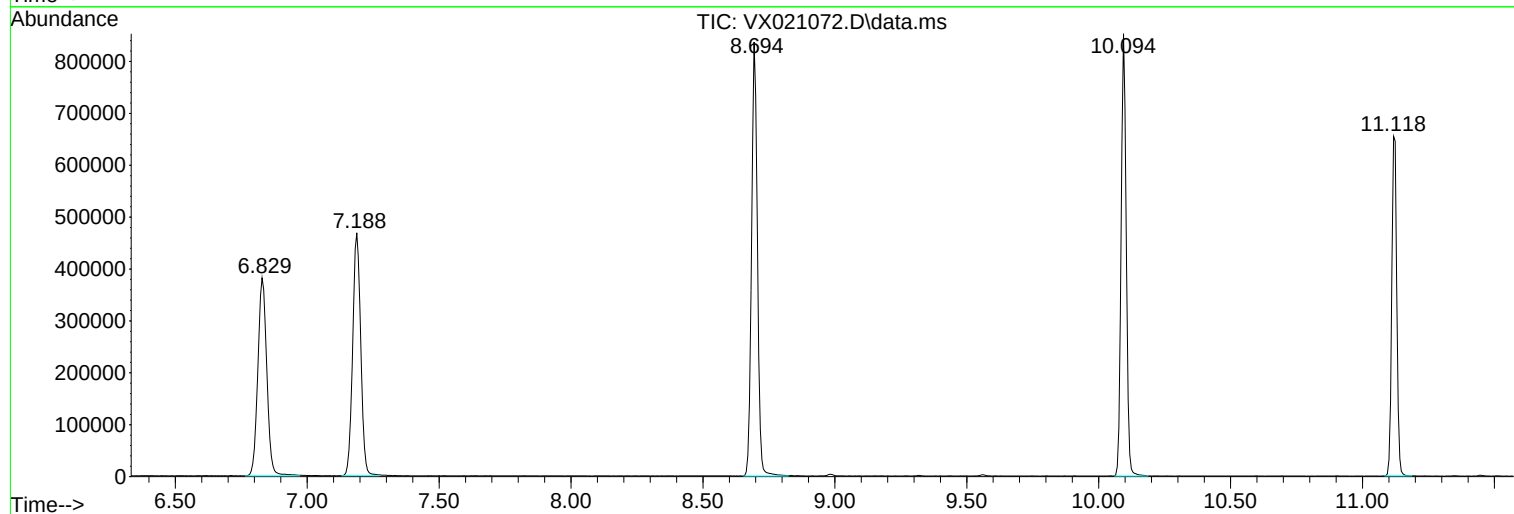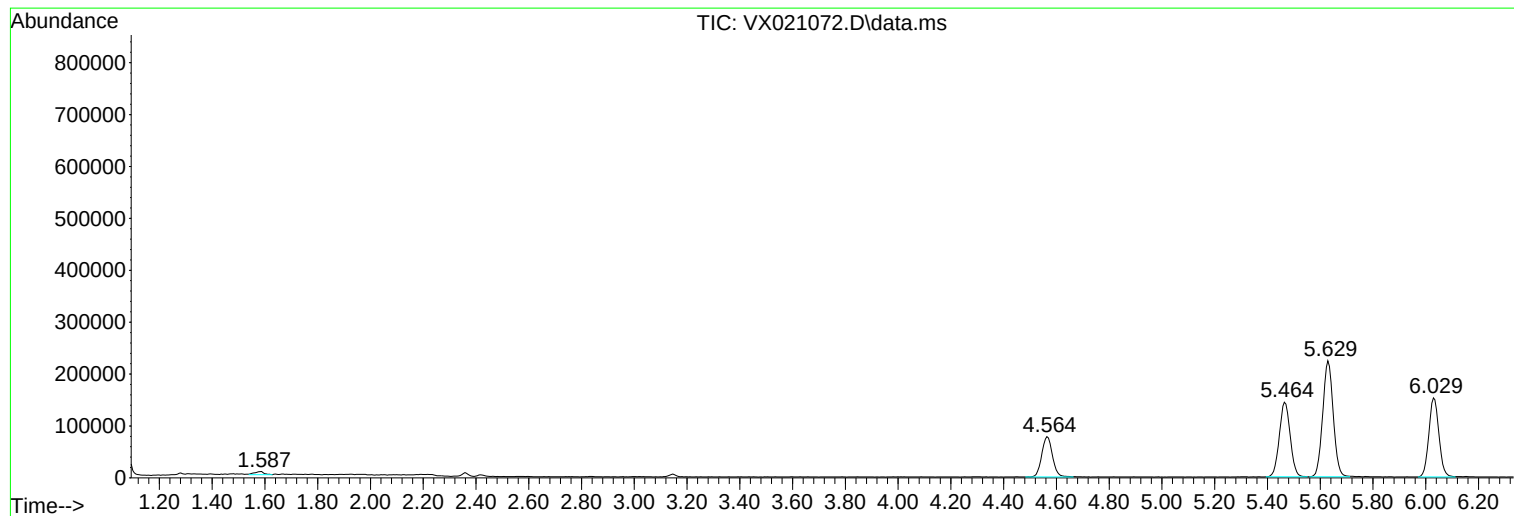

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030821\
Data File : VX021072.D
Acq On : 08 Mar 2021 19:21
Operator : JC/MD
Sample : M1596-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WEST-DITCH-OUT-20210305

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030821\
Data File : VX021072.D
Acq On : 08 Mar 2021 19:21
Operator : JC/MD
Sample : M1596-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WEST-DITCH-OUT-20210305

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
