
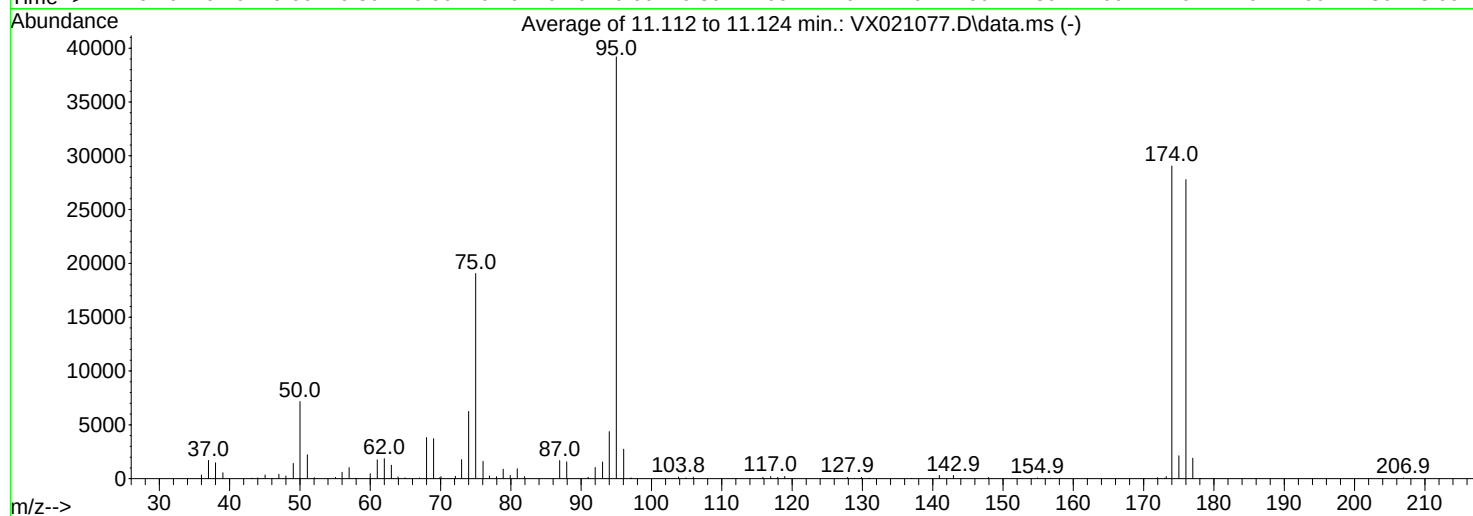


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030821\
Data File : VX021077.D
Acq On : 08 Mar 2021 21:39
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022421W.M
Title : SW846 8260
Last Update : Wed Feb 24 13:50:55 2021

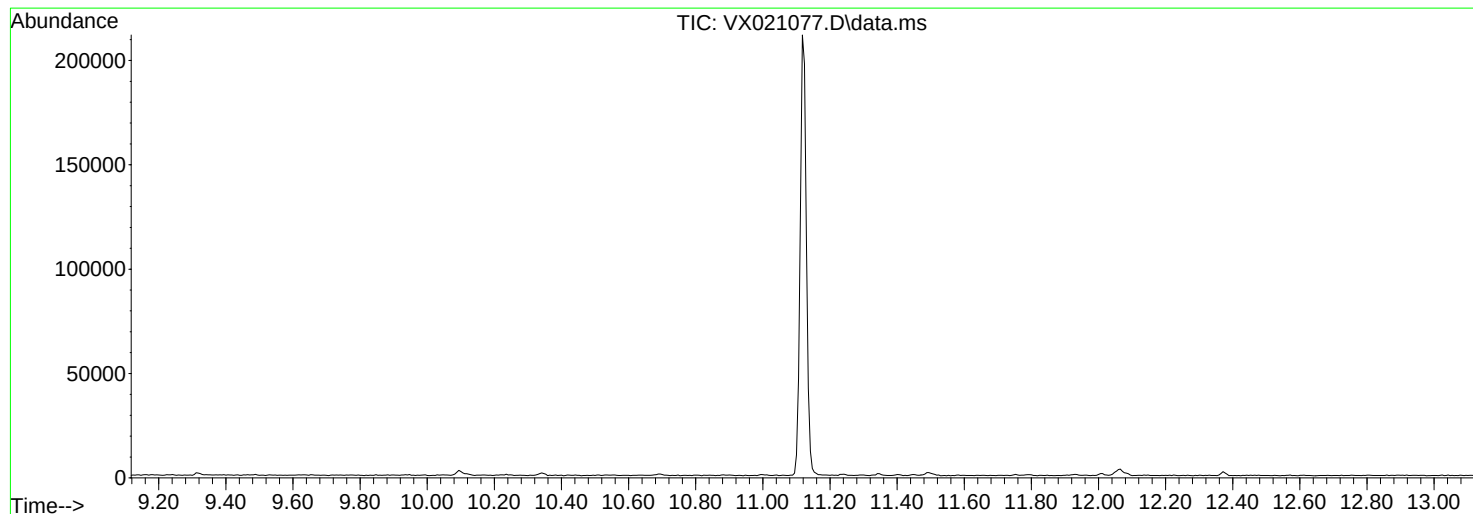

AutoFind: Scans 1704, 1705, 1706; Background Corrected with Scan 1698

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	7167	PASS
75	95	30	60	48.6	19065	PASS
95	95	100	100	100.0	39192	PASS
96	95	5	9	7.0	2738	PASS
173	174	0.00	2	0.7	196	PASS
174	95	50	100	74.1	29056	PASS
175	174	5	9	7.3	2130	PASS
176	174	95	101	95.6	27786	PASS
177	176	5	9	6.8	1899	PASS