



Bromomethane

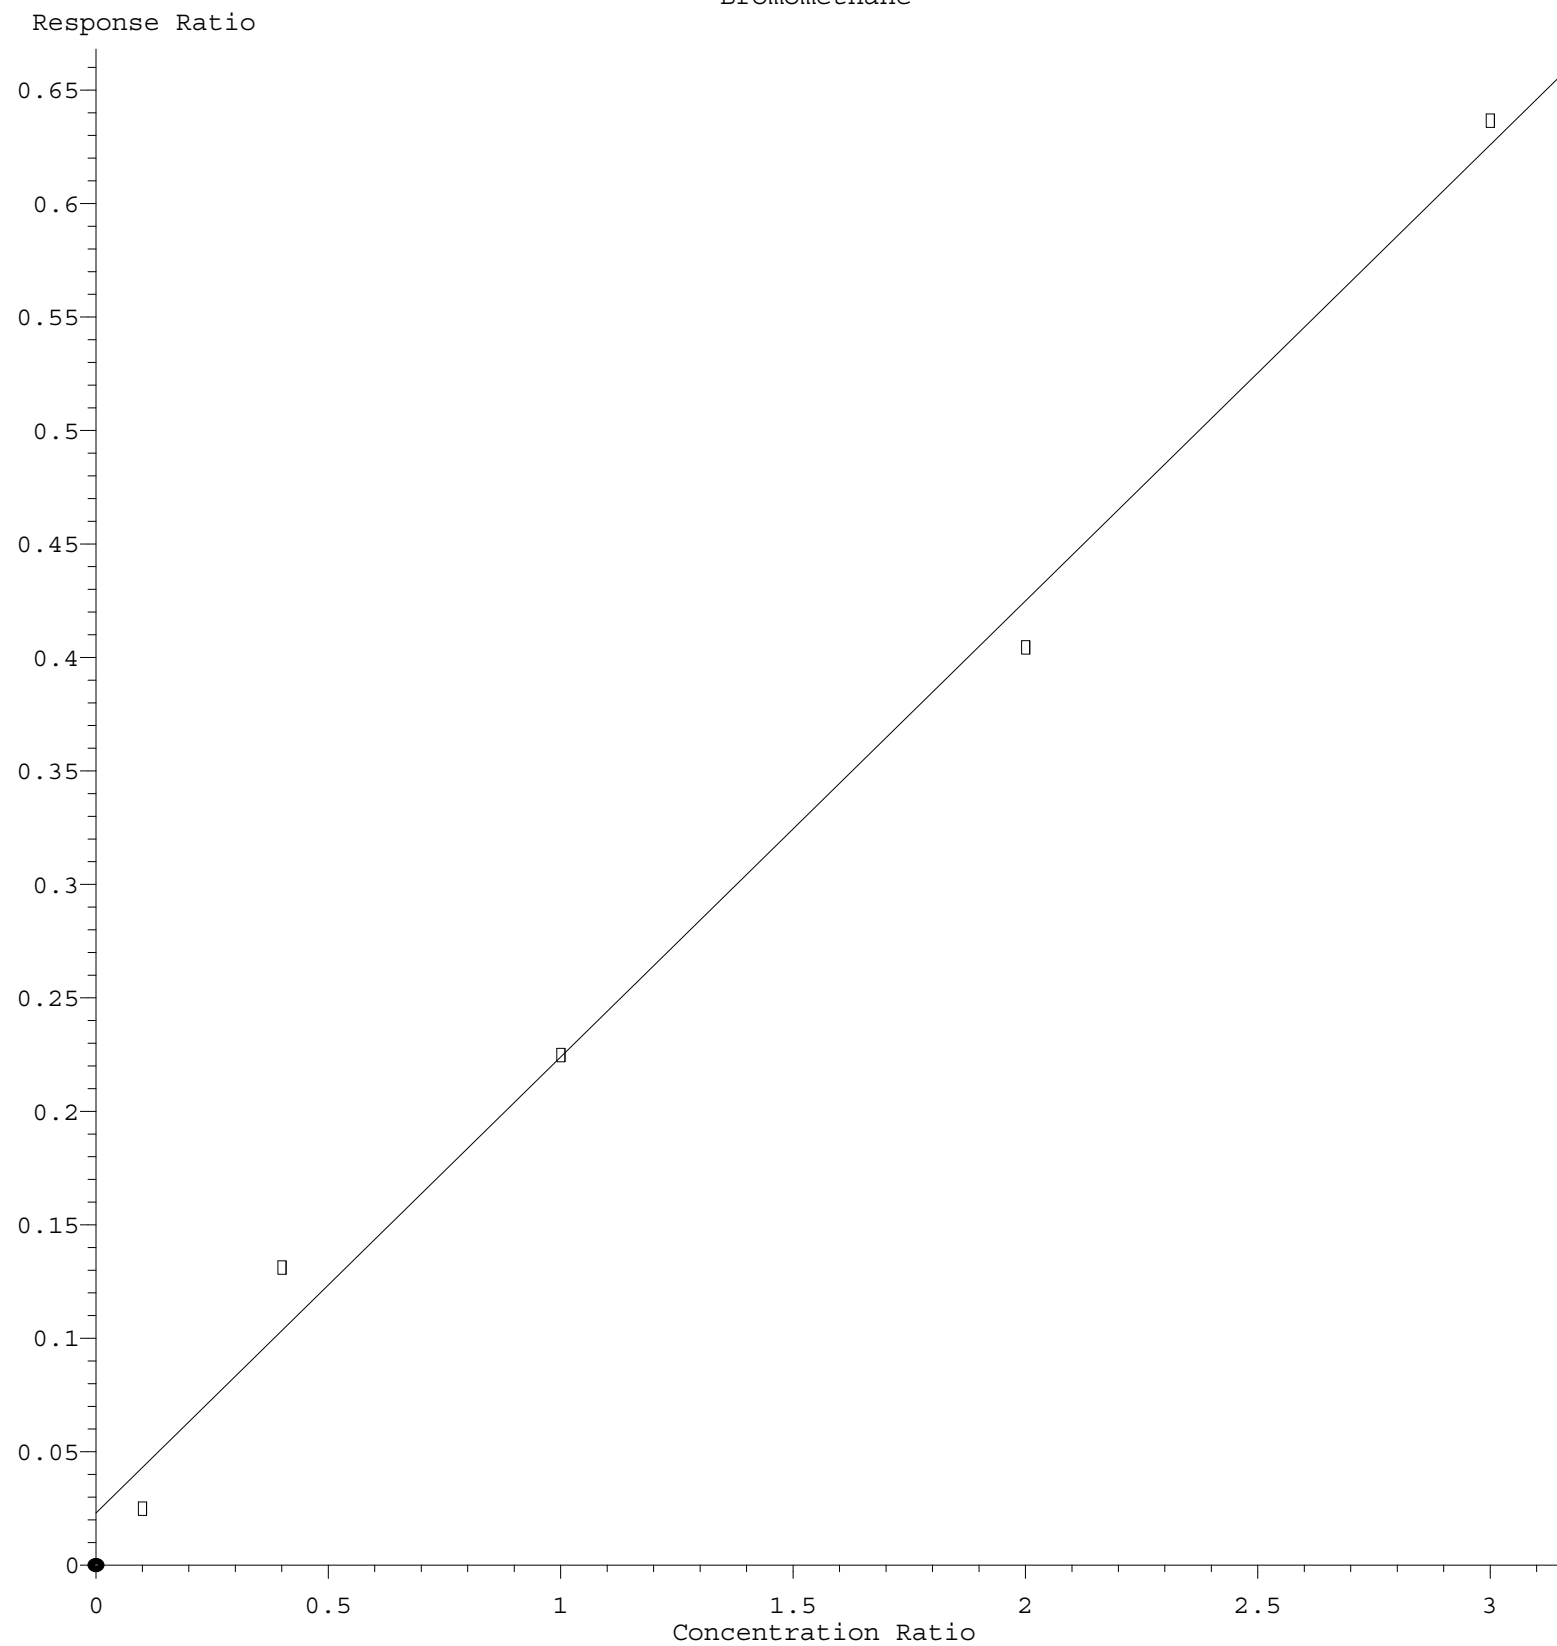

$\text{Response} = 2.010\text{e-}001 * \text{Amt} + 2.301\text{e-}002$
 Coef of Det (r^2) = 0.992965 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X030822W.M
 Calibration Table Last Updated: Tue Mar 08 15:54:34 2022

Chloroethane


Response Ratio

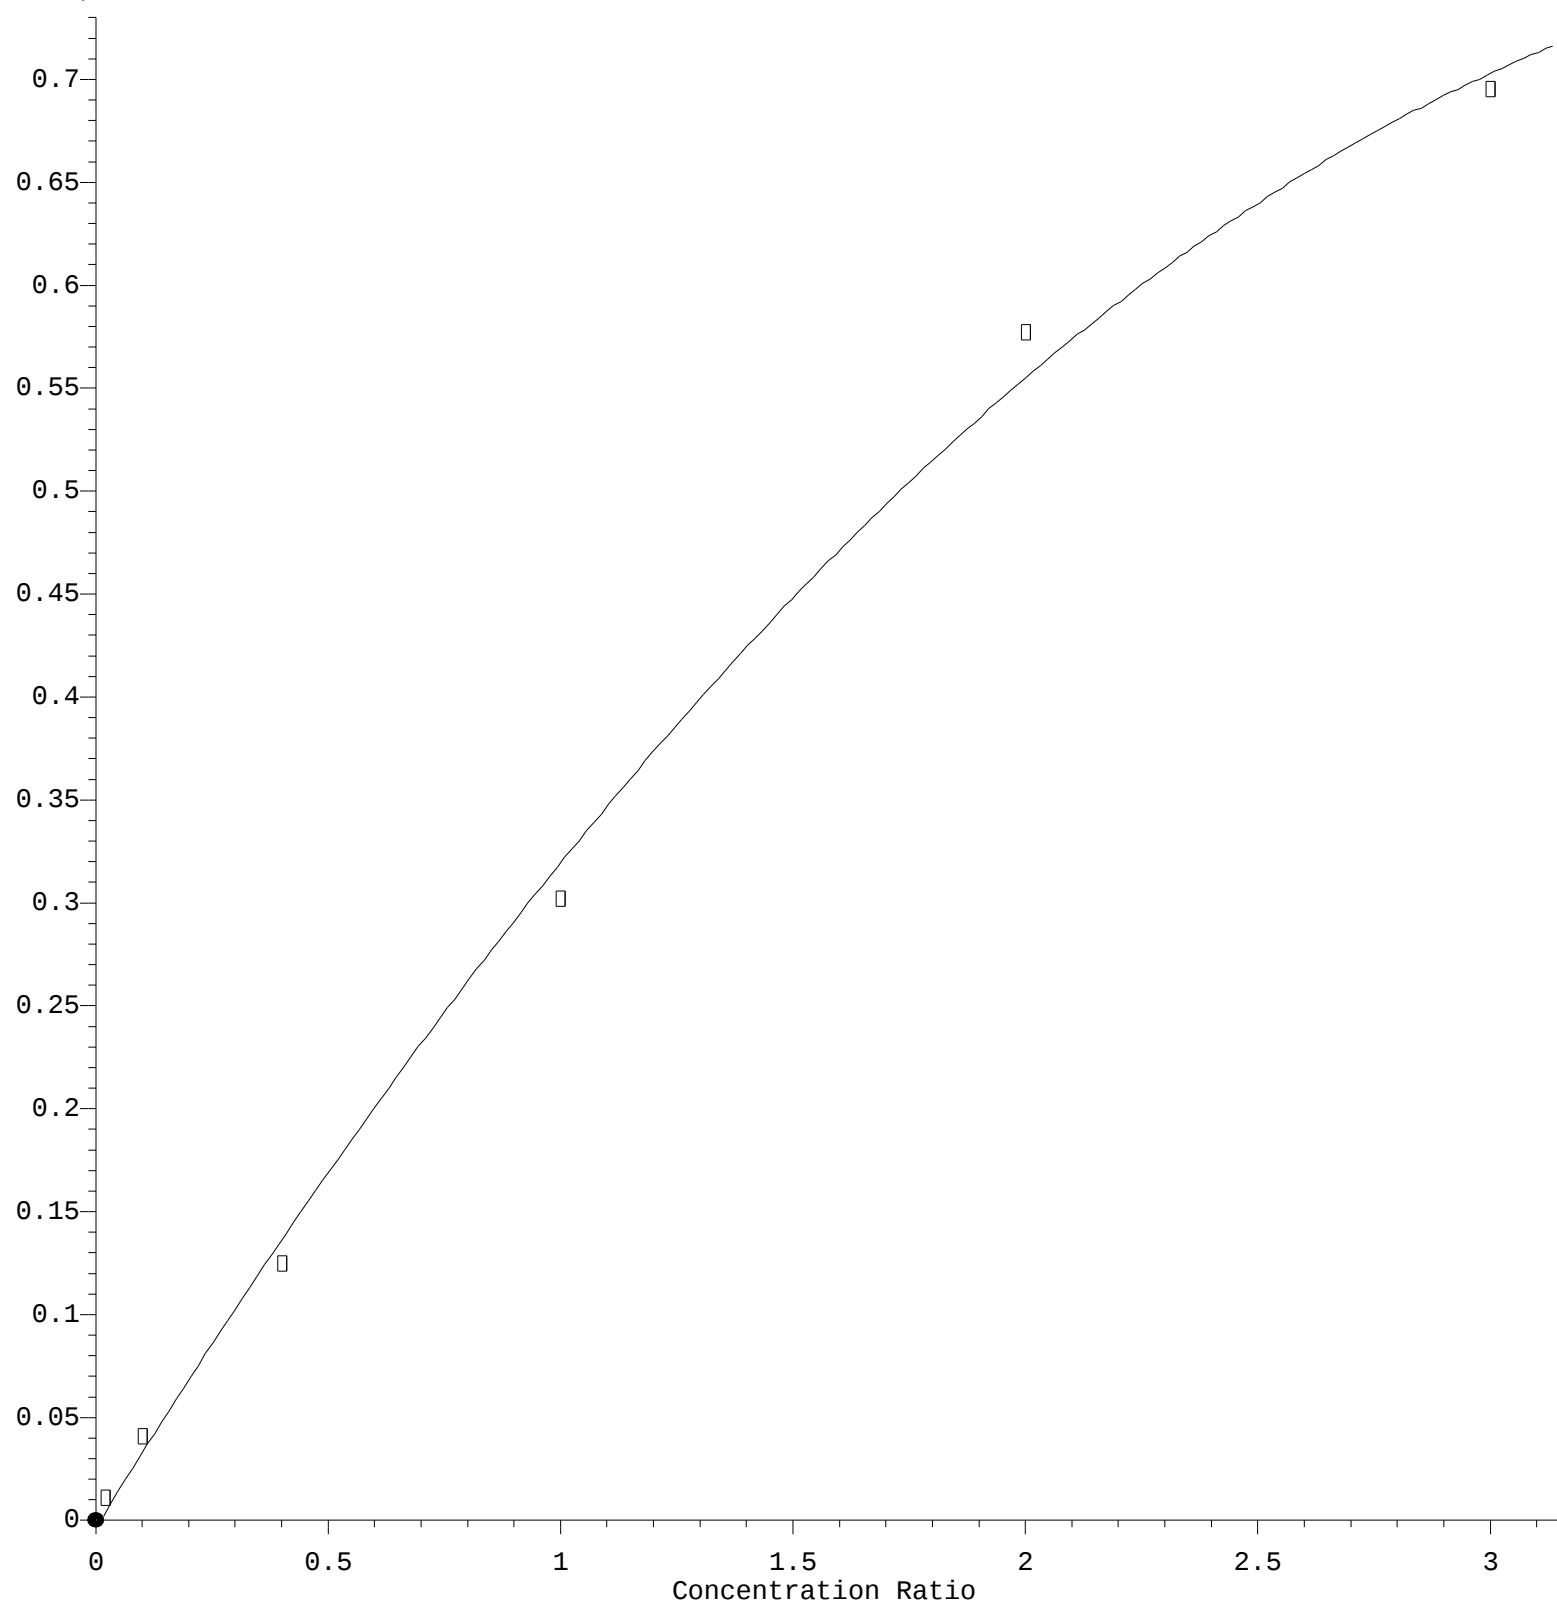

$R = -4.370e-002 A^2 + 3.665e-001 A - 3.355e-003$
 Coef of Det (r^2) = 0.997367 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
 Calibration Table Last Updated: Tue Mar 08 15:54:34 2022

Acetone

Response Ratio

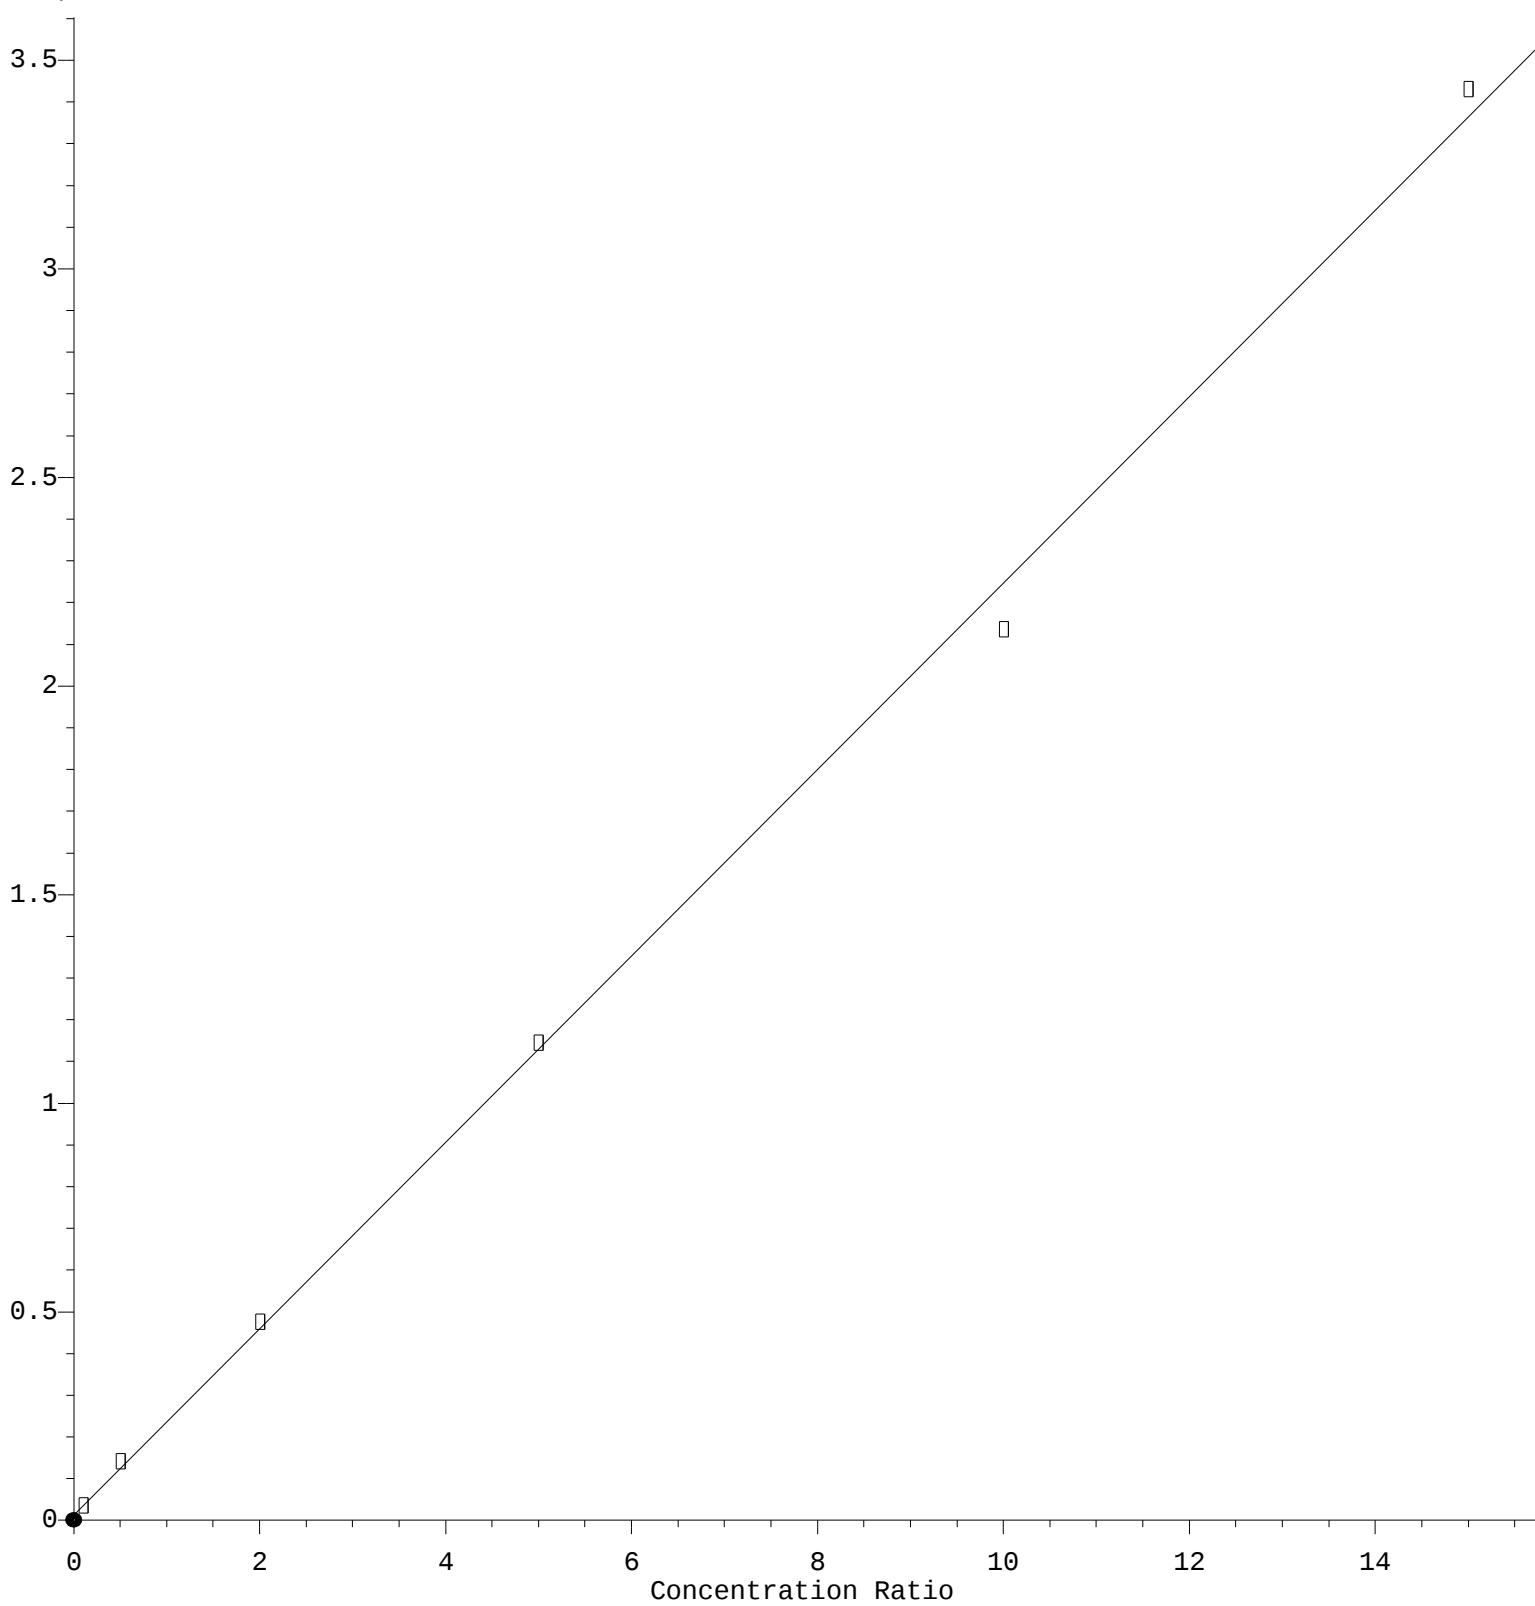

$$\text{Response} = 2.234\text{e-}001 * \text{Amt} + 1.306\text{e-}002$$

Coef of Det (r^2) = 0.998004 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M

Calibration Table Last Updated: Tue Mar 08 15:54:34 2022