

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030822\
 Data File : VX027336.D
 Acq On : 08 Mar 2022 17:11
 Operator : JC/MD
 Sample : VX0308WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0308WBL01

Quant Time: Mar 09 00:15:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 08 15:54:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	402897	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	670299	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	609435	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	279011	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	233351	49.666	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	99.340%
35) Dibromofluoromethane	5.391	113	213930	49.462	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.920%
50) Toluene-d8	8.653	98	792199	48.516	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	97.040%
62) 4-Bromofluorobenzene	11.085	95	290953	46.752	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	93.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030822\
Data File : VX027336.D
Acq On : 08 Mar 2022 17:11
Operator : JC/MD
Sample : VX0308WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0308WBL01

Quant Time: Mar 09 00:15:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X030822W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 08 15:54:34 2022
Response via : Initial Calibration




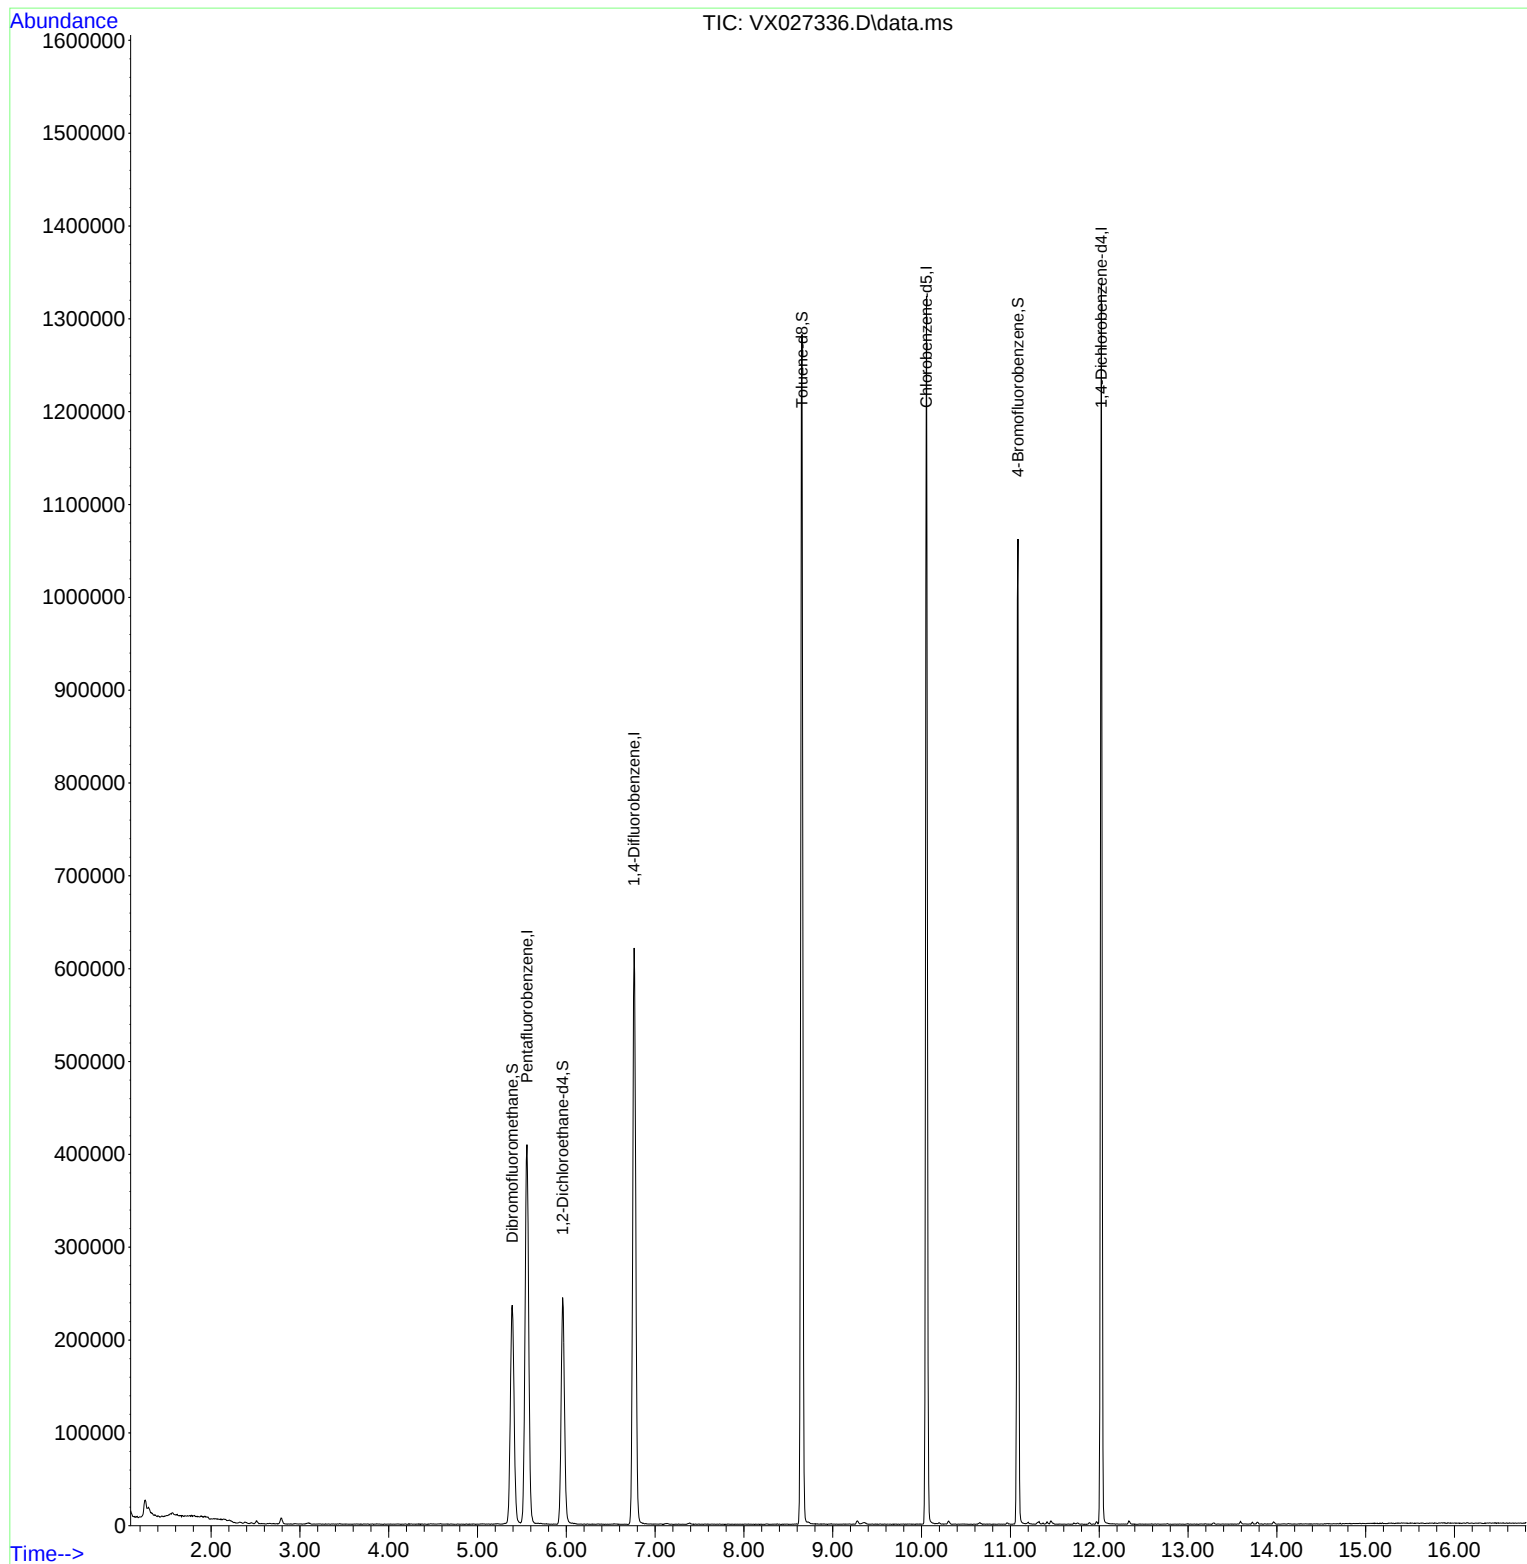


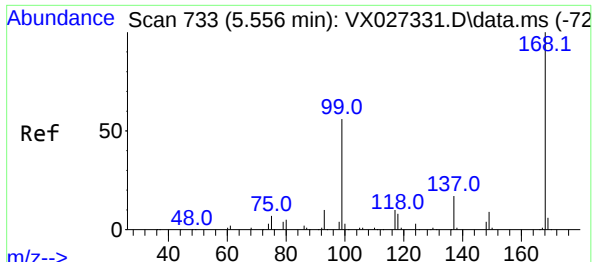

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX027336.D
Acq: 08 Mar 2022 17:11




Instrument :
MSVOA_X
ClientSampleId :
VX0308WBL01


Tgt Ion:168 Resp: 402897
Ion Ratio Lower Upper
168 100
99 56.5 41.7 62.5

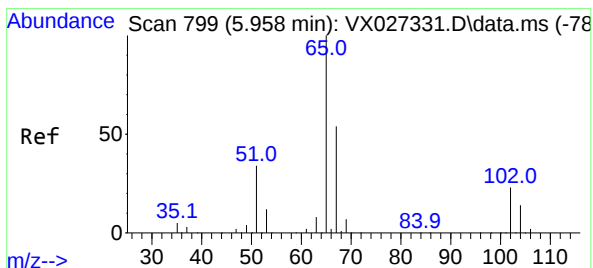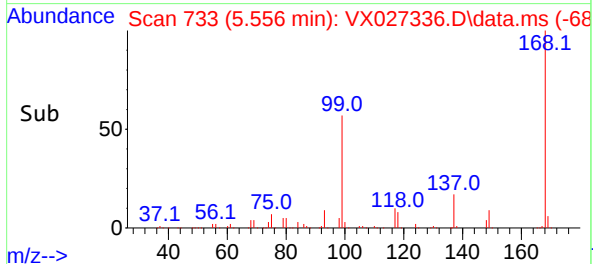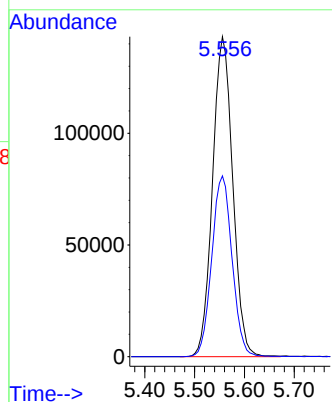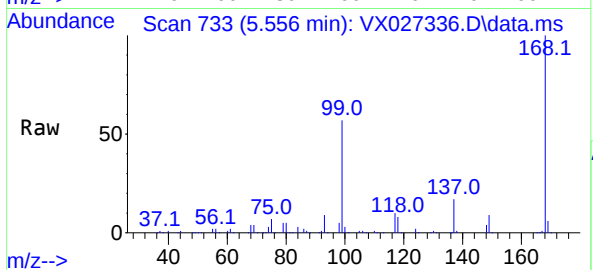

#33
1,2-Dichloroethane-d4
Concen: 49.666 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027336.D
Acq: 08 Mar 2022 17:11

Tgt Ion: 65 Resp: 233351
Ion Ratio Lower Upper
65 100
67 52.6 0.0 107.4


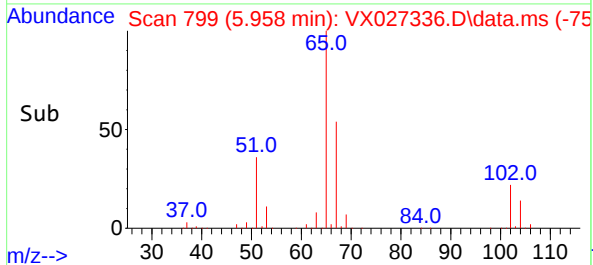
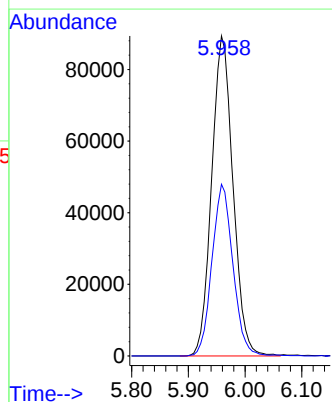
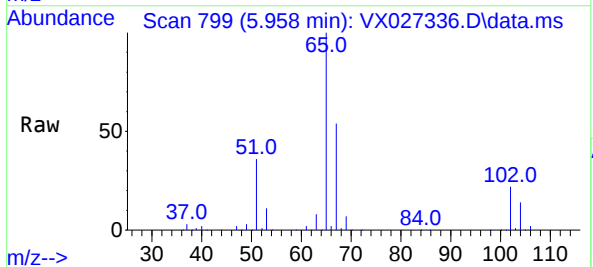


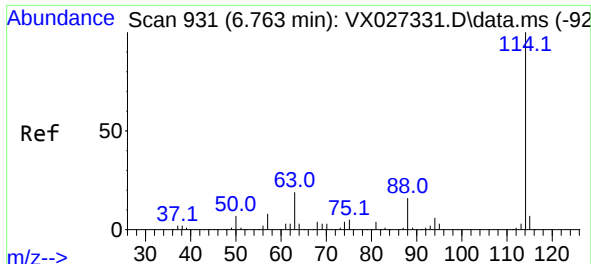

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX027336.D
Acq: 08 Mar 2022 17:11




Instrument :
MSVOA_X
ClientSampleId :
VX0308WBL01


Tgt Ion:114 Resp: 670299
Ion Ratio Lower Upper
114 100
63 19.3 0.0 36.8
88 16.4 0.0 32.4

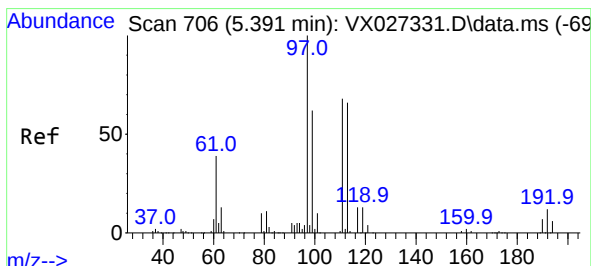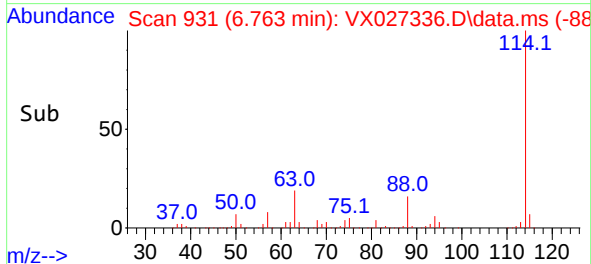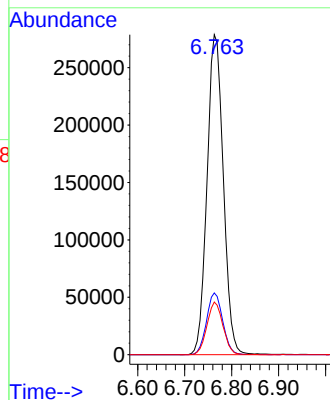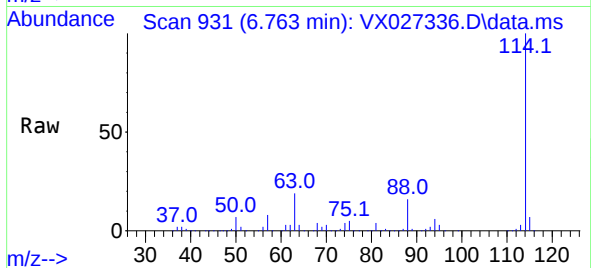

#35
Dibromofluoromethane
Concen: 49.462 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX027336.D
Acq: 08 Mar 2022 17:11

Tgt Ion:113 Resp: 213930
Ion Ratio Lower Upper
113 100
111 101.4 82.8 124.2
192 20.3 16.9 25.3


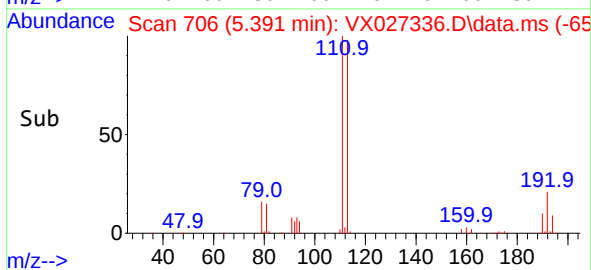
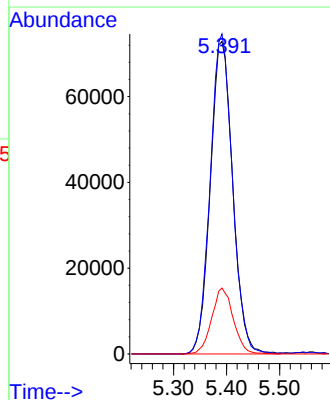
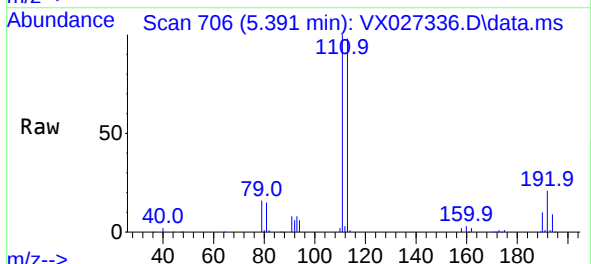


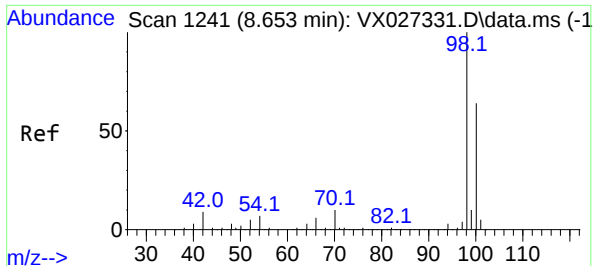

#50
Toluene-d8
Concen: 48.516 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX027336.D
Acq: 08 Mar 2022 17:11




Instrument :
MSVOA_X
ClientSampleId :
VX0308WBL01


Tgt Ion: 98 Resp: 792199
Ion Ratio Lower Upper
98 100
100 65.2 52.6 78.8

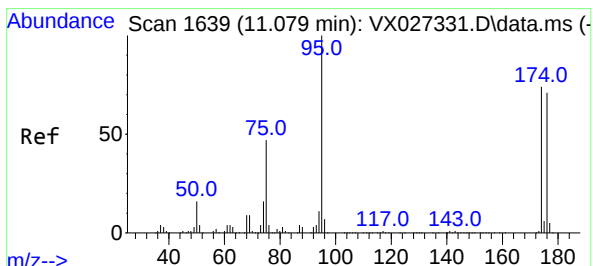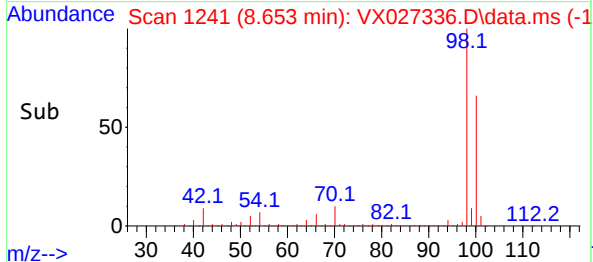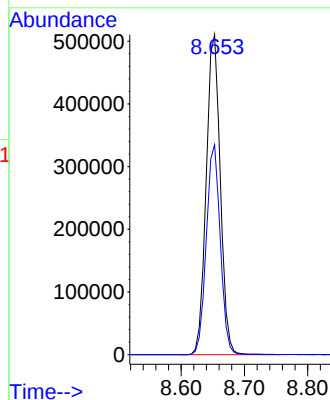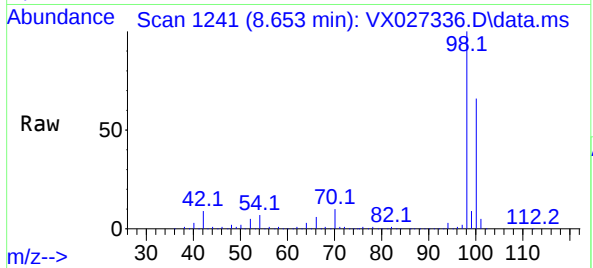

#62
4-Bromofluorobenzene
Concen: 46.752 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX027336.D
Acq: 08 Mar 2022 17:11

Tgt Ion: 95 Resp: 290953
Ion Ratio Lower Upper
95 100
174 79.4 0.0 163.0
176 77.0 0.0 155.0


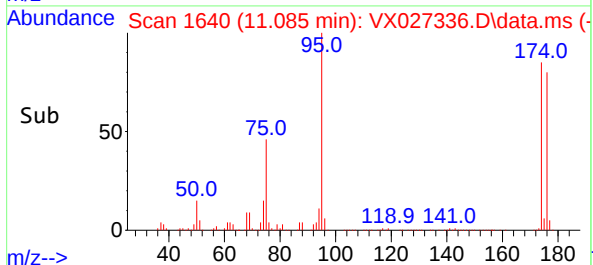
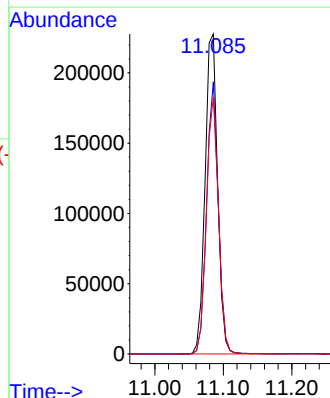
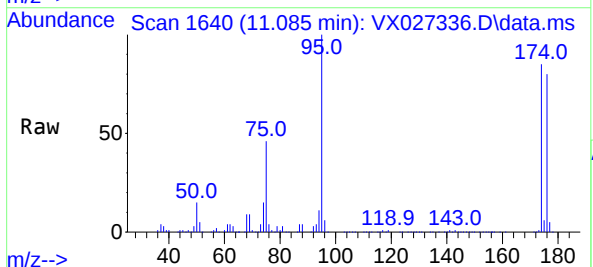


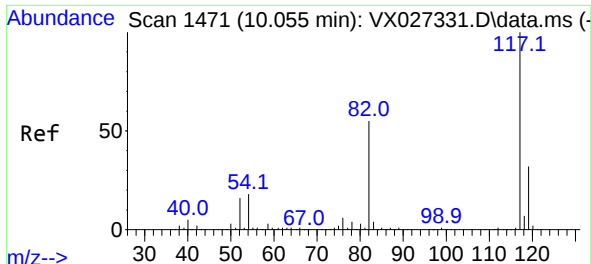

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX027336.D
Acq: 08 Mar 2022 17:11

Instrument :
MSVOA_X
ClientSampleId :
VX0308WBL01

Tgt Ion:117 Resp: 609435
Ion Ratio Lower Upper
117 100
82 55.1 41.8 62.8
119 31.8 24.8 37.2

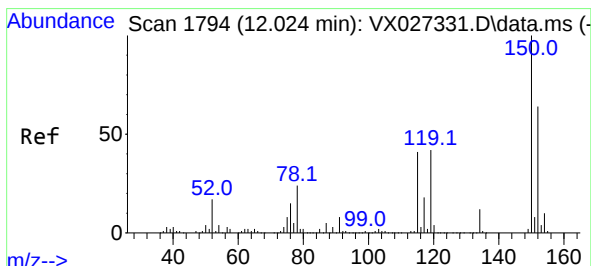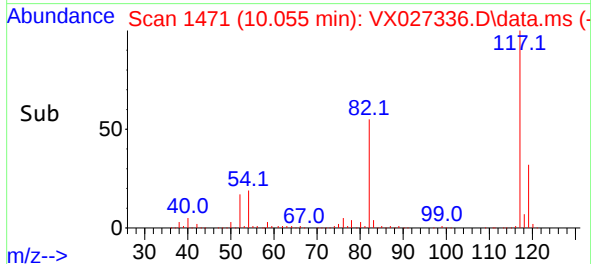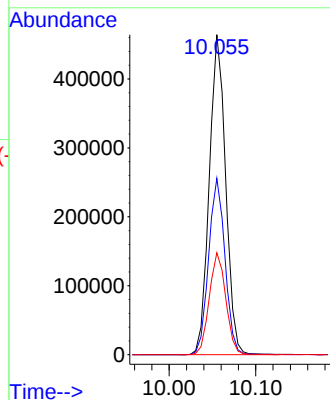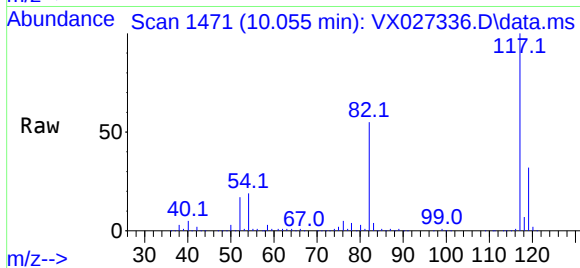

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX027336.D
Acq: 08 Mar 2022 17:11

Tgt Ion:152 Resp: 279011
Ion Ratio Lower Upper
152 100
115 59.9 37.5 112.7
150 156.5 0.0 338.2

