



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030823\
Data File : VX034372.D
Acq On : 08 Mar 2023 09:14
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X021723W.M
Title : SW846 8260
Last Update : Fri Feb 17 12:33:35 2023

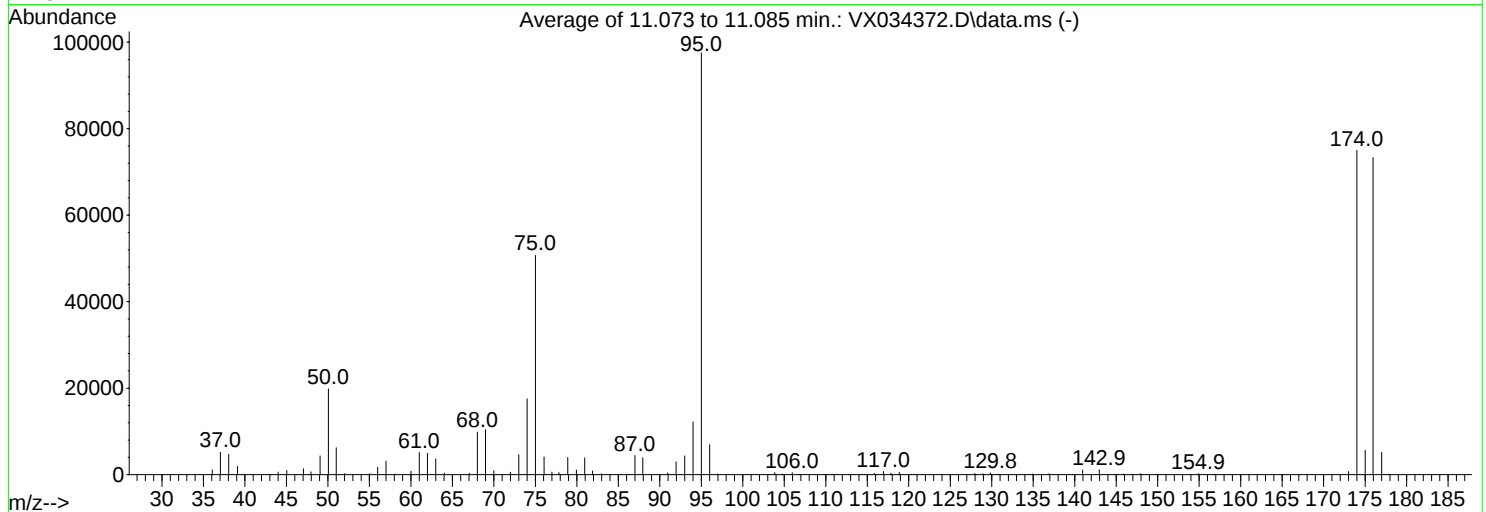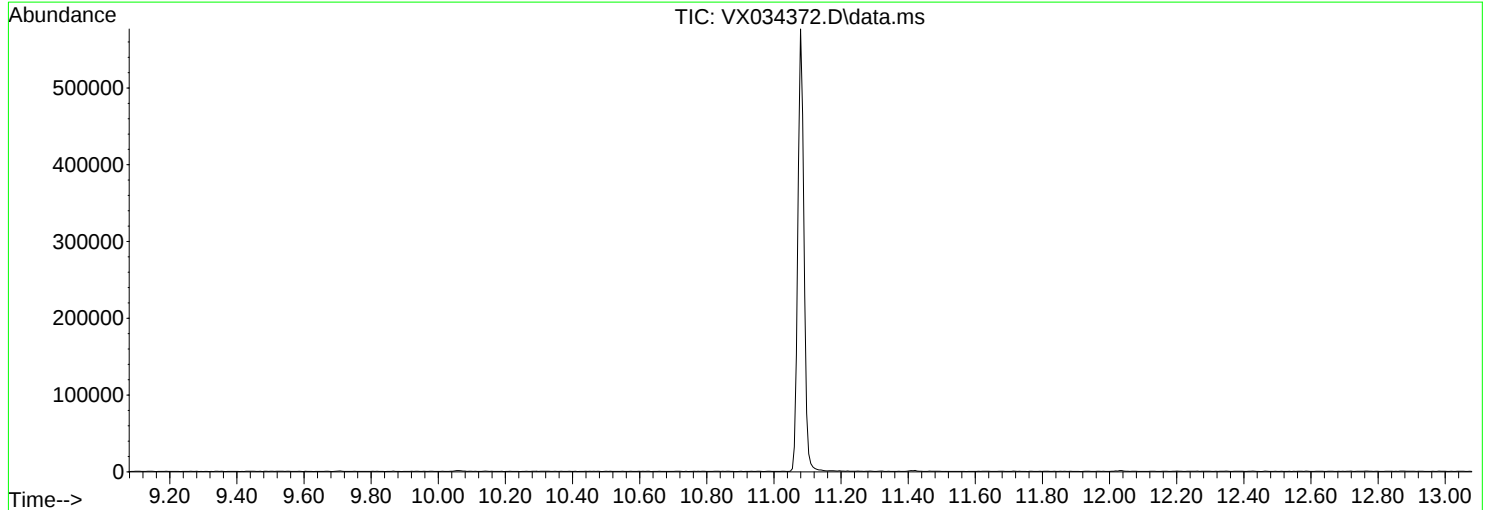

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	19840	PASS
75	95	30	60	52.0	50704	PASS
95	95	100	100	100.0	97544	PASS
96	95	5	9	7.1	6904	PASS
173	174	0.00	2	1.0	719	PASS
174	95	50	100	76.9	75000	PASS
175	174	5	9	7.5	5640	PASS
176	174	95	101	97.8	73341	PASS
177	176	5	9	7.0	5159	PASS